

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070722\
 Data File : VX029961.D
 Acq On : 07 Jul 2022 17:38
 Operator : JC/MD
 Sample : N3617-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-06

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Title : SW846 8260

Signal : TIC: VX029961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	21	25	32	rBV	18168	31710	3.33%	0.579%
2	2.538	233	238	248	rVB	16390	30305	3.18%	0.553%
3	3.117	325	333	344	rBV2	30083	71100	7.46%	1.298%
4	5.391	694	706	720	rBV2	103048	305869	32.08%	5.583%
5	5.555	723	733	750	rVB	190100	530199	55.61%	9.677%
6	5.964	790	800	817	rBV2	118591	315490	33.09%	5.758%
7	6.769	921	932	946	rBV	293760	718721	75.38%	13.118%
8	8.652	1233	1241	1250	rBV	609607	953431	100.00%	17.402%
9	10.055	1465	1471	1480	rBV	612902	821224	86.13%	14.989%
10	11.085	1634	1640	1646	rBV	456196	587455	61.61%	10.722%
11	11.896	1769	1773	1780	rVB	11648	16996	1.78%	0.310%
12	12.024	1789	1794	1805	rBV	631524	756118	79.30%	13.800%
13	12.249	1823	1831	1836	rBV	34376	47640	5.00%	0.870%
14	12.316	1836	1842	1850	rVB5	10395	16972	1.78%	0.310%
15	12.652	1891	1897	1902	rBV	14979	23040	2.42%	0.421%
16	12.841	1920	1928	1933	rBV	15310	22355	2.34%	0.408%
17	12.920	1933	1941	1945	rBV8	4636	10334	1.08%	0.189%
18	13.036	1955	1960	1964	rVB2	10189	13400	1.41%	0.245%
19	13.139	1966	1977	1979	rBV5	12101	23214	2.43%	0.424%
20	13.194	1984	1986	1990	rVB2	10428	11841	1.24%	0.216%
21	13.639	2052	2059	2060	rVV3	15983	28666	3.01%	0.523%
22	13.664	2060	2063	2074	rVB2	27577	51415	5.39%	0.938%
23	13.926	2099	2106	2110	rVB2	19059	27162	2.85%	0.496%
24	14.103	2133	2135	2141	rVB6	7366	10348	1.09%	0.189%
25	14.371	2174	2179	2185	rBV5	9182	13869	1.45%	0.253%
26	14.487	2194	2198	2210	rVB10	5661	10849	1.14%	0.198%
27	14.786	2243	2247	2253	rBV4	8080	14734	1.55%	0.269%
28	14.907	2260	2267	2275	rBV10	5413	14528	1.52%	0.265%




Sum of corrected areas: 5478985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070722\
Data File : VX029961.D
Acq On : 07 Jul 2022 17:38
Operator : JC/MD
Sample : N3617-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

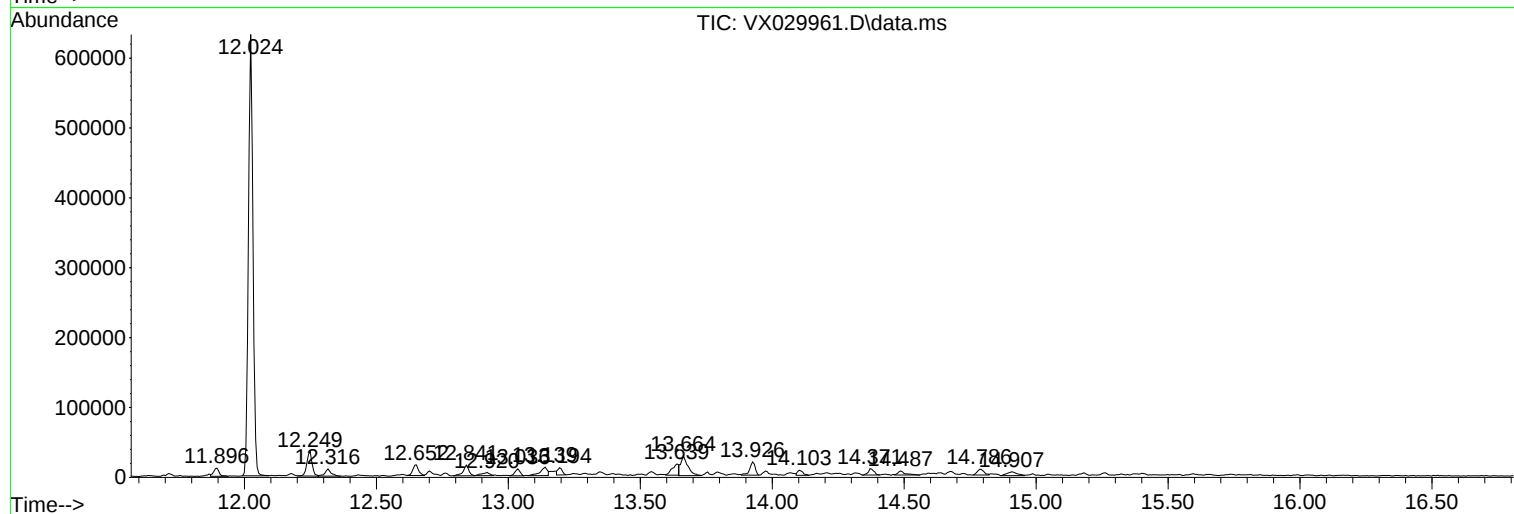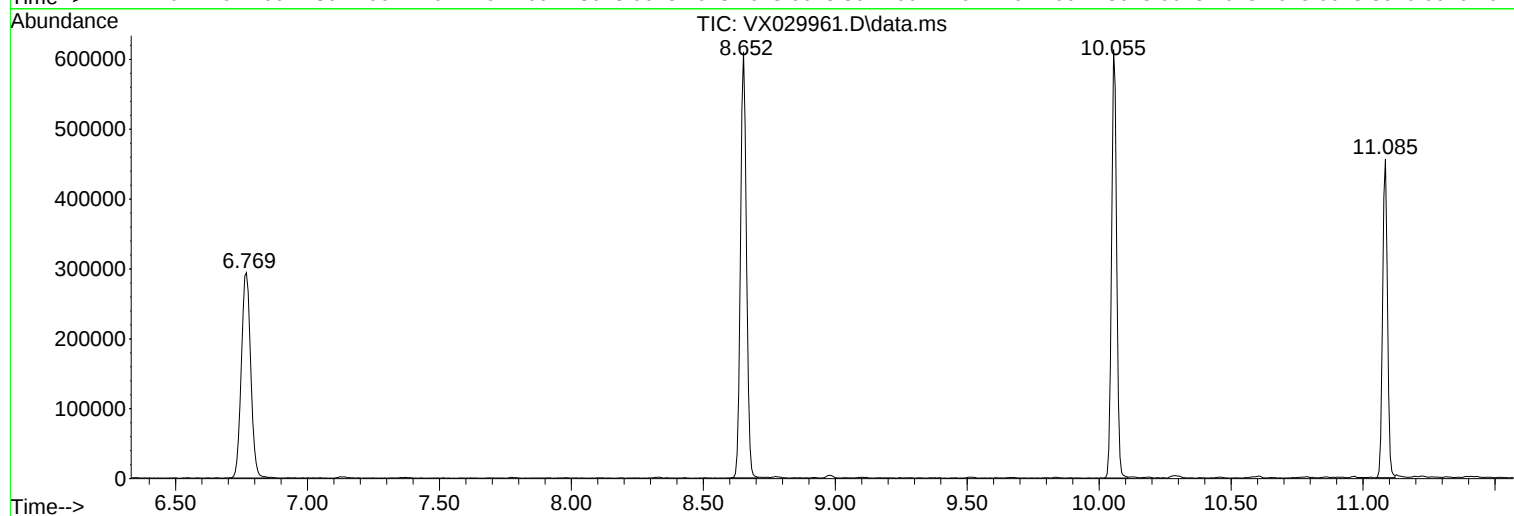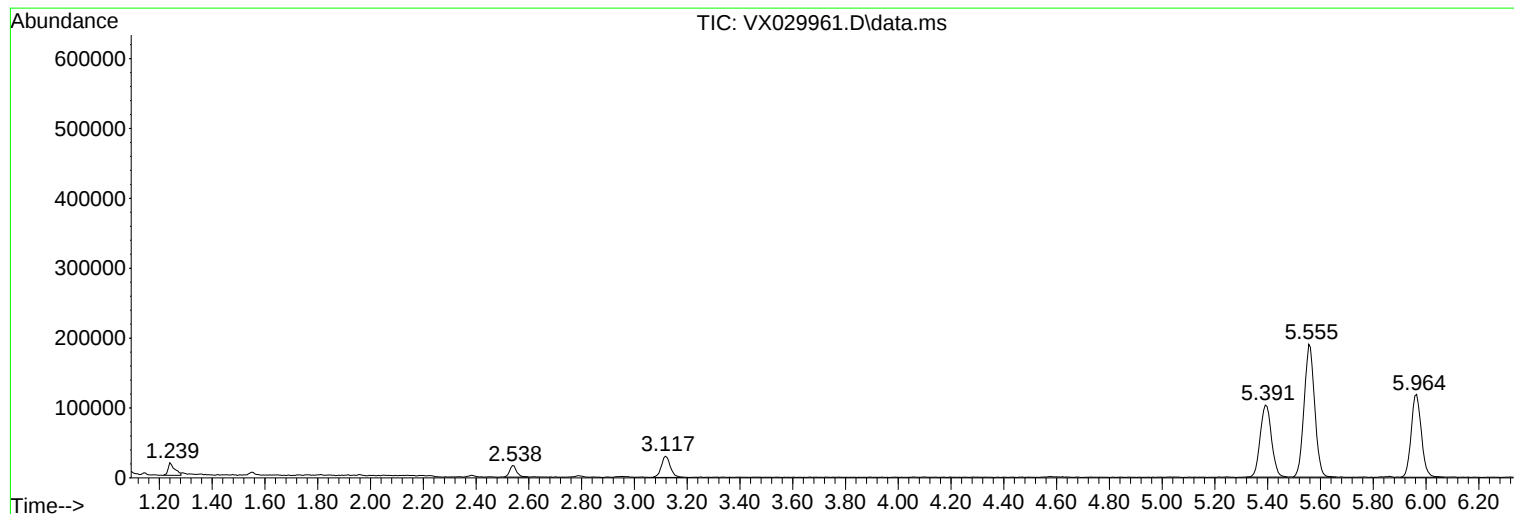

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070722\
Data File : VX029961.D
Acq On : 07 Jul 2022 17:38
Operator : JC/MD
Sample : N3617-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070722\
Data File : VX029961.D
Acq On : 07 Jul 2022 17:38
Operator : JC/MD
Sample : N3617-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------