
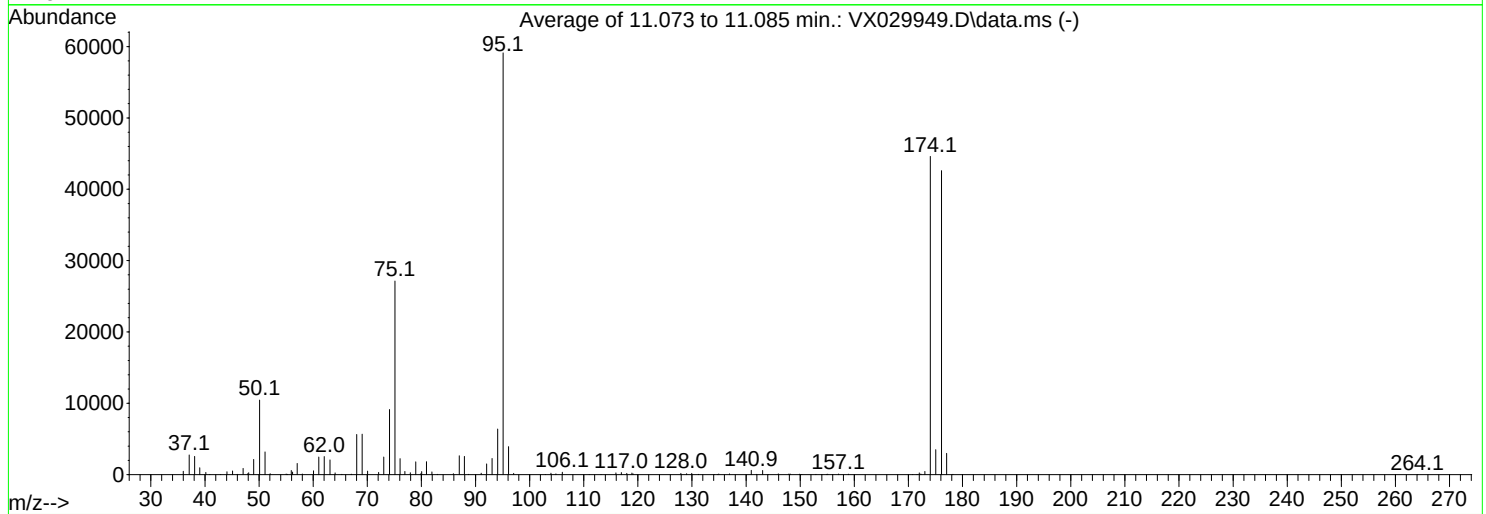


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070722\
Data File : VX029949.D
Acq On : 07 Jul 2022 08:07
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Title : SW846 8260
Last Update : Wed Jun 29 05:54:51 2022

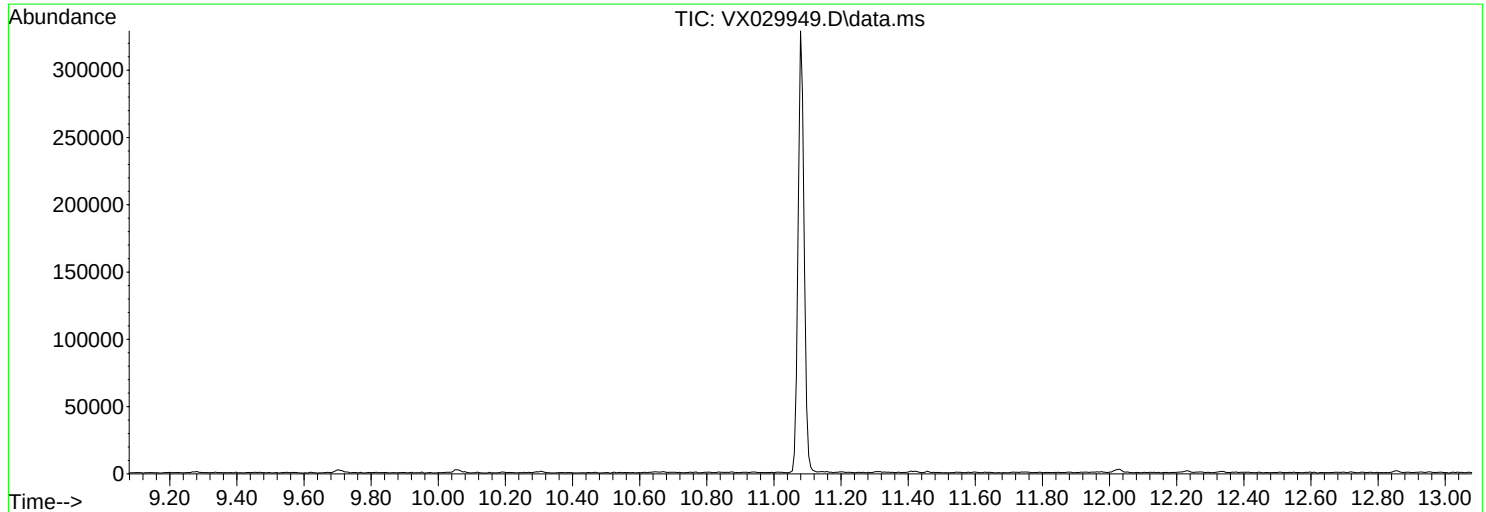

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	10447	PASS
75	95	30	60	45.9	27133	PASS
95	95	100	100	100.0	59120	PASS
96	95	5	9	6.6	3922	PASS
173	174	0.00	2	1.0	446	PASS
174	95	50	100	75.4	44597	PASS
175	174	5	9	7.8	3491	PASS
176	174	95	101	95.6	42613	PASS
177	176	5	9	7.0	2990	PASS