

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071825\
 Data File : VX047049.D
 Acq On : 18 Jul 2025 15:00
 Operator : JC/MD
 Sample : Q2637-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Jul 19 04:25:09 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 03 05:51:11 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	448042	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	792920	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	740369	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	367208	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	318516	53.812	ug/l	0.00
Spiked Amount	50.000	Range 78 - 117	Recovery	= 107.620%		
35) Dibromofluoromethane	5.397	113	264566	49.154	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	= 98.300%		
50) Toluene-d8	8.653	98	953764	50.224	ug/l	0.00
Spiked Amount	50.000	Range 92 - 112	Recovery	= 100.440%		
62) 4-Bromofluorobenzene	11.079	95	380575	52.731	ug/l	0.00
Spiked Amount	50.000	Range 83 - 123	Recovery	= 105.460%		
Target Compounds						
					Qvalue	
13) Acrolein	2.233	56	64	2.982	ug/l #	28
16) Acetone	2.410	43	1700	0.925	ug/l #	69
17) Carbon Disulfide	2.526	76	4668	0.366	ug/l	97
31) Cyclohexane	5.550	56	10152	1.200	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	38054	5.240	ug/l #	50
38) Carbon Tetrachloride	5.562	117	45917	5.981	ug/l #	17
76) 1,2,3-Trichloropropane	11.079	75	199251	35.117	ug/l #	36
81) trans-1,4-Dichloro-2-b...	11.079	75	199251	94.237	ug/l #	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071825\
Data File : VX047049.D
Acq On : 18 Jul 2025 15:00
Operator : JC/MD
Sample : Q2637-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Jul 19 04:25:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 03 05:51:11 2025
Response via : Initial Calibration




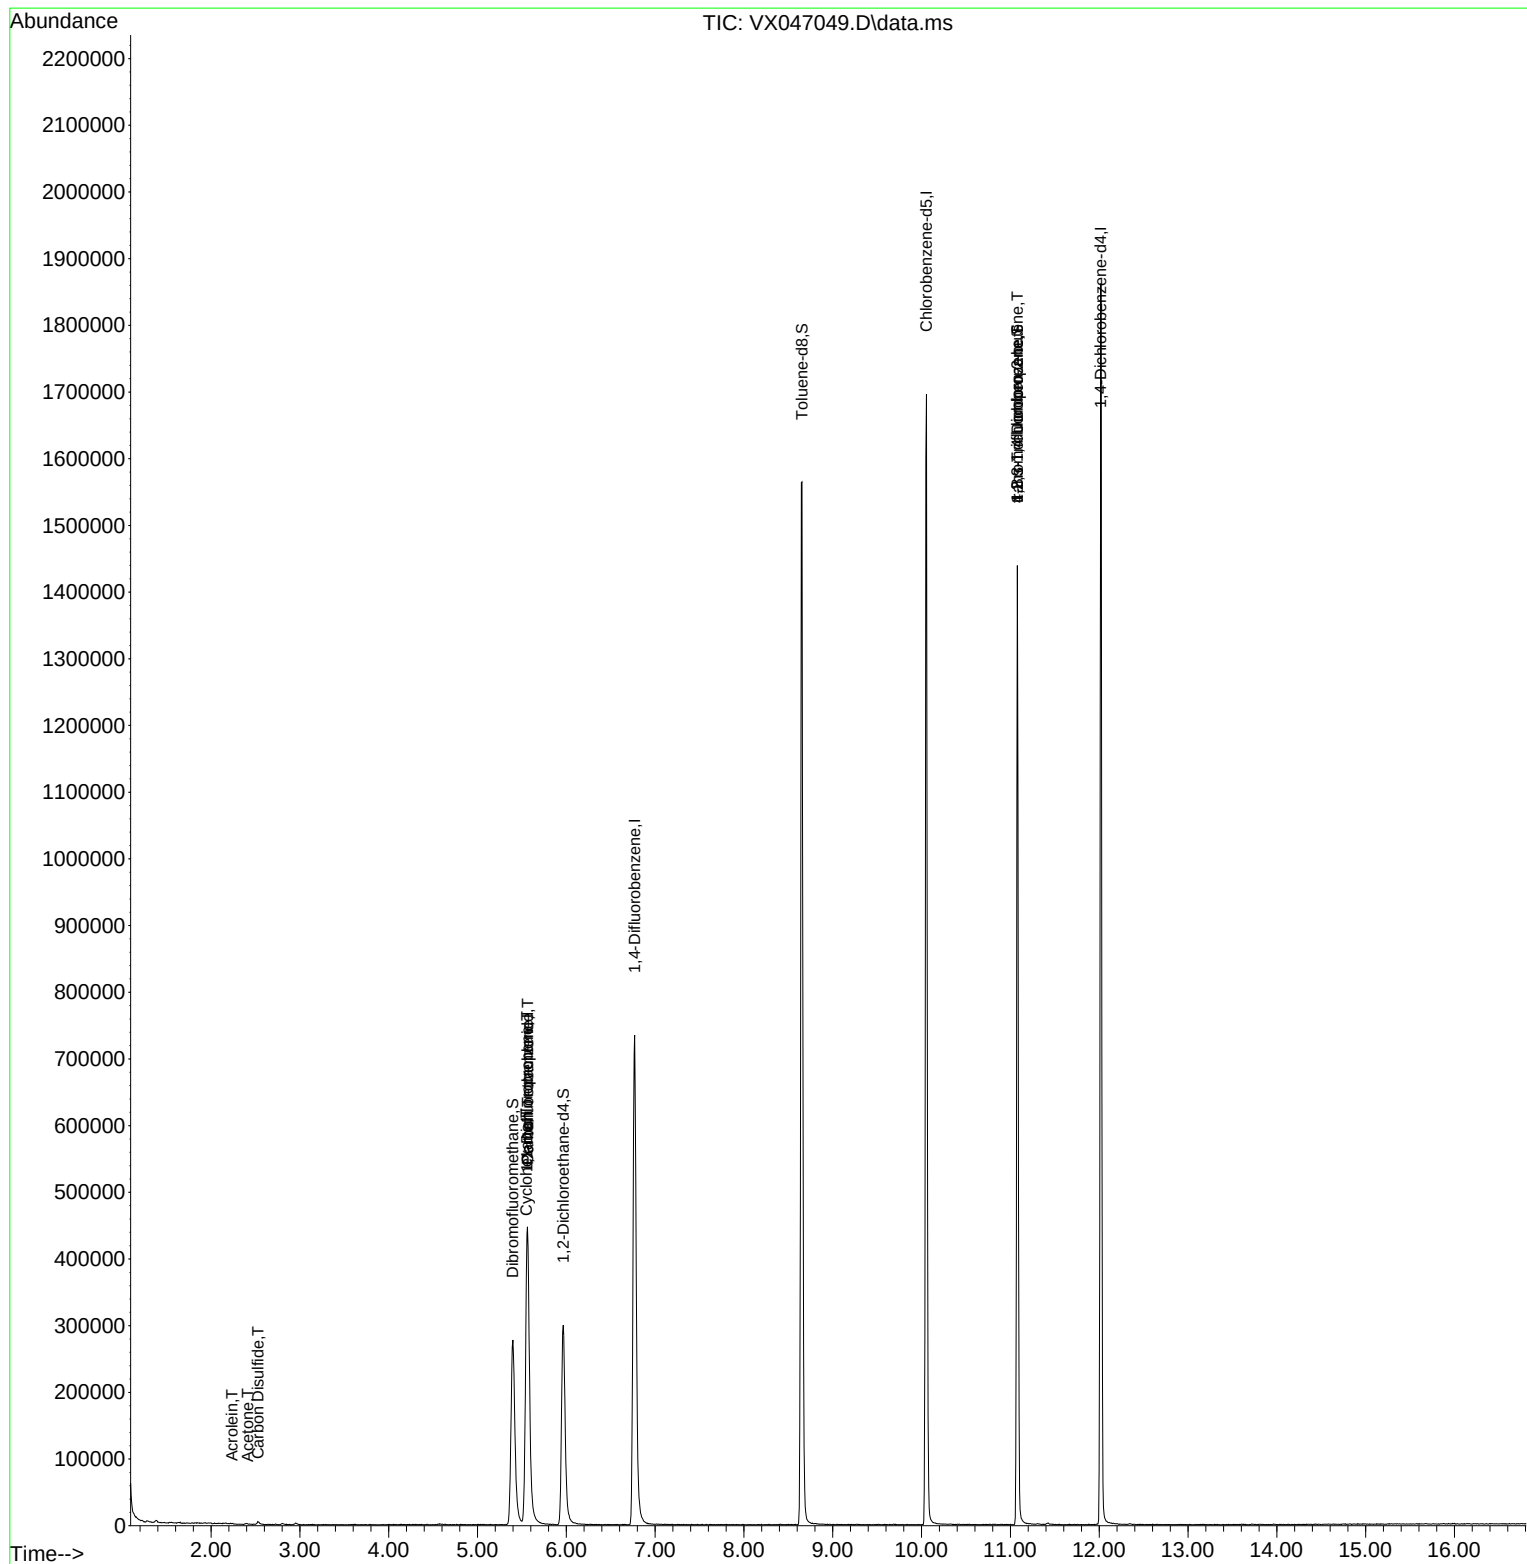




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 448042
Ion Ratio Lower Upper
168 100
99 65.5 48.8 73.2

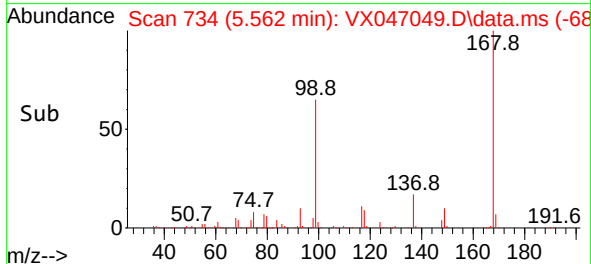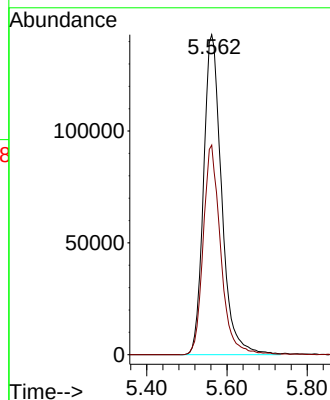

#13
Acrolein
Concen: 2.982 ug/l
RT: 2.233 min Scan# 188
Delta R.T. -0.013 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00

Tgt Ion: 56 Resp: 64
Ion Ratio Lower Upper
56 100
55 128.1 55.5 83.3#


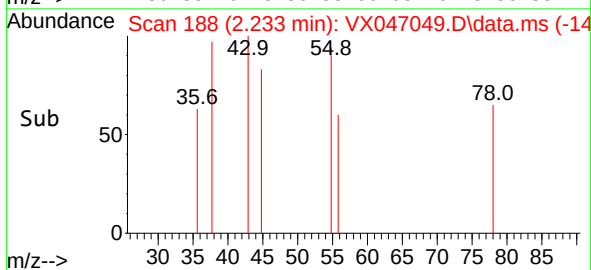
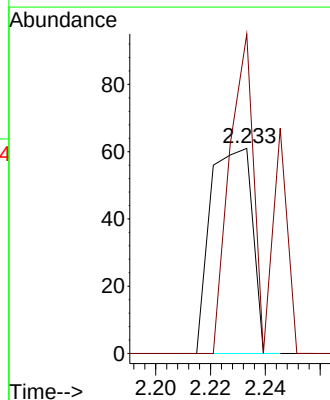
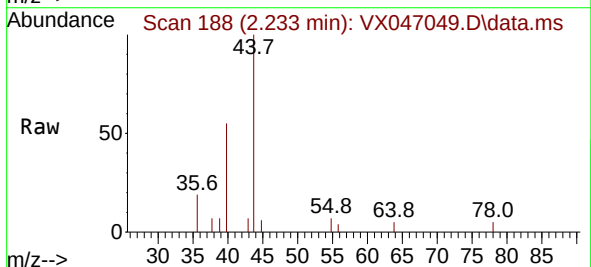


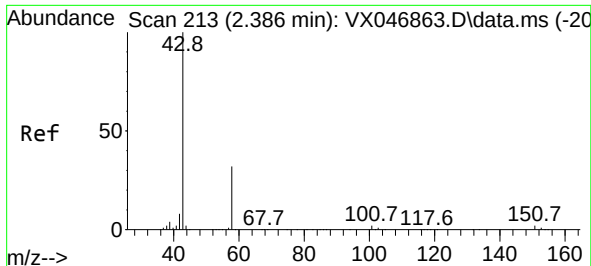

#16
Acetone
Concen: 0.925 ug/l
RT: 2.410 min Scan# 213
Delta R.T. 0.024 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 43 Resp: 1700
Ion Ratio Lower Upper
43 100
58 14.6 25.8 38.6#

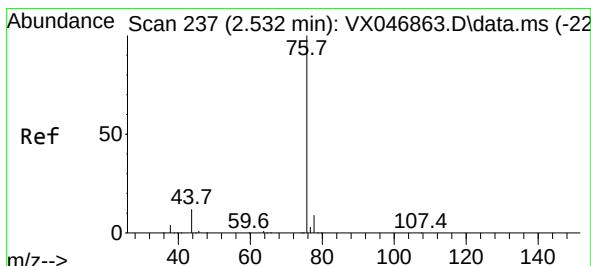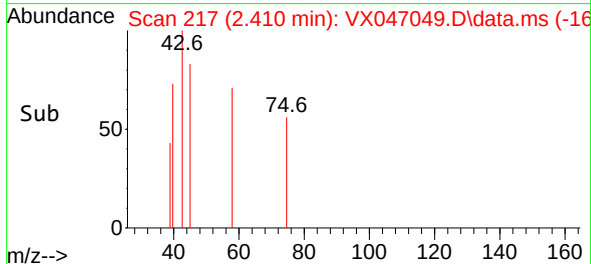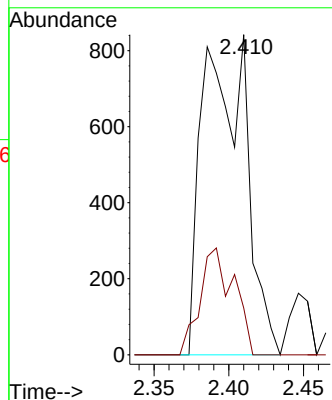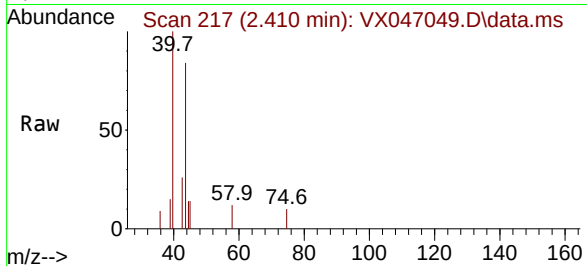

#17
Carbon Disulfide
Concen: 0.366 ug/l
RT: 2.526 min Scan# 236
Delta R.T. -0.006 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00

Tgt Ion: 76 Resp: 4668
Ion Ratio Lower Upper
76 100
78 8.1 7.4 11.2


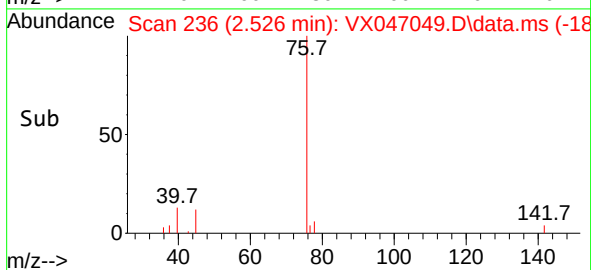
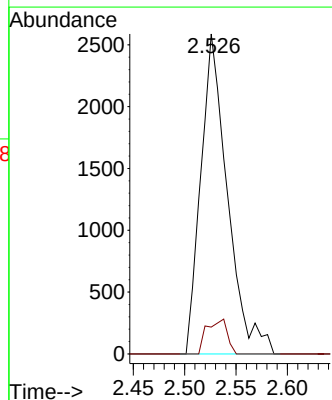
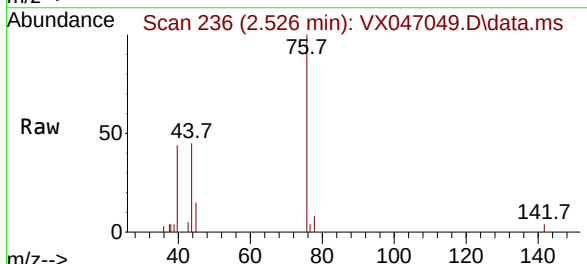


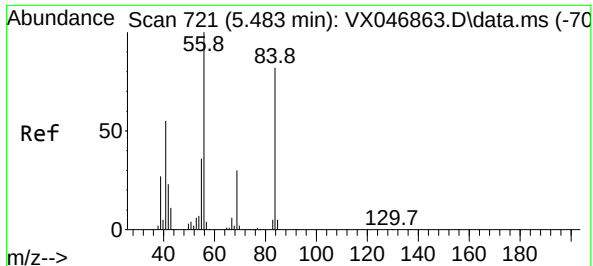

#31
Cyclohexane
Concen: 1.200 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.067 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 56 Resp: 10152
Ion Ratio Lower Upper
56 100
69 163.9 24.0 36.0#
84 128.6 66.5 99.7#

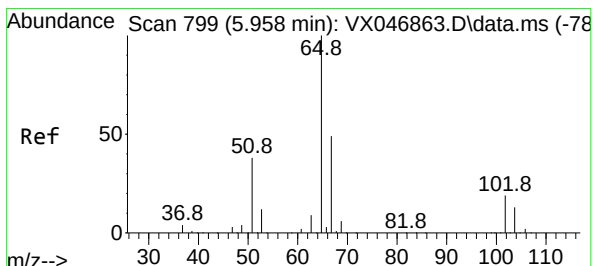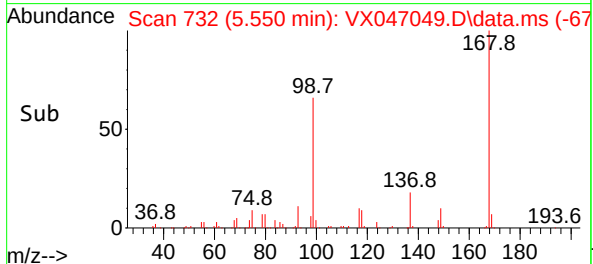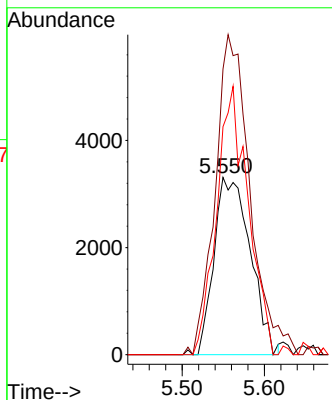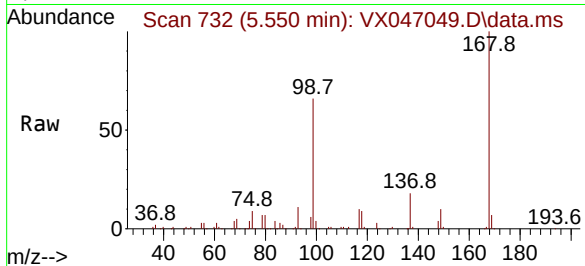

#33
1,2-Dichloroethane-d4
Concen: 53.812 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.006 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00

Tgt Ion: 65 Resp: 318516
Ion Ratio Lower Upper
65 100
67 51.7 0.0 105.2


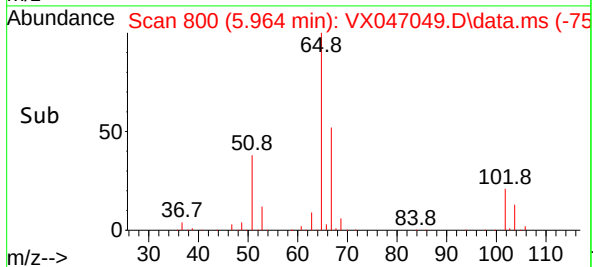
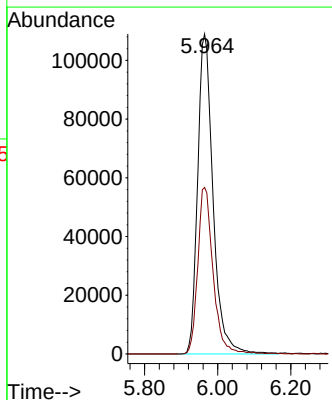
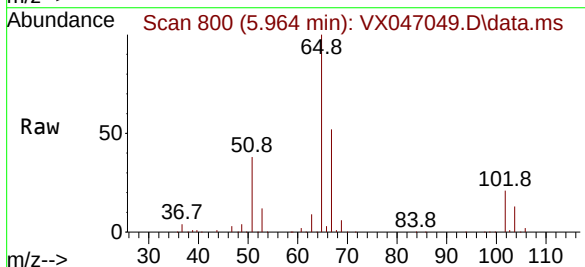


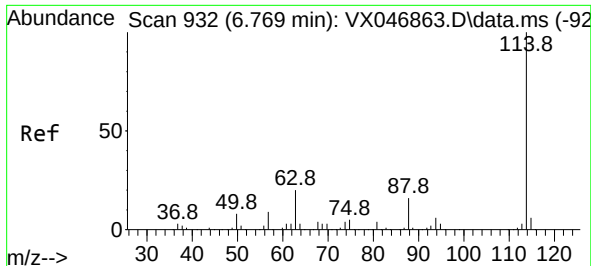

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:114 Resp: 792920
Ion Ratio Lower Upper
114 100
63 22.1 0.0 40.4
88 16.7 0.0 31.0

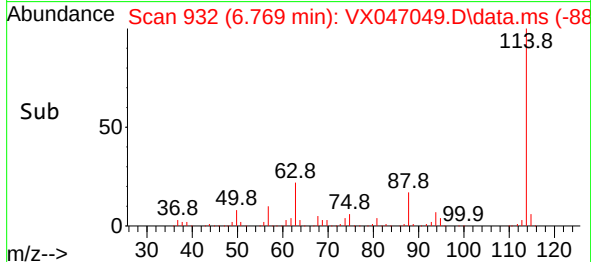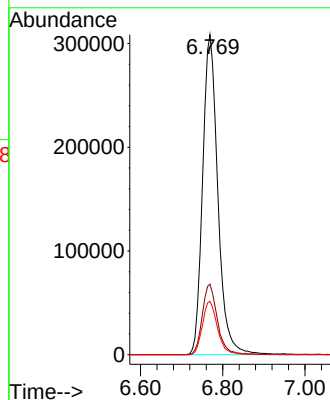

#35
Dibromofluoromethane
Concen: 49.154 ug/l
RT: 5.397 min Scan# 707
Delta R.T. -0.000 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00

Tgt Ion:113 Resp: 264566
Ion Ratio Lower Upper
113 100
111 101.2 81.2 121.8
192 18.1 15.3 22.9


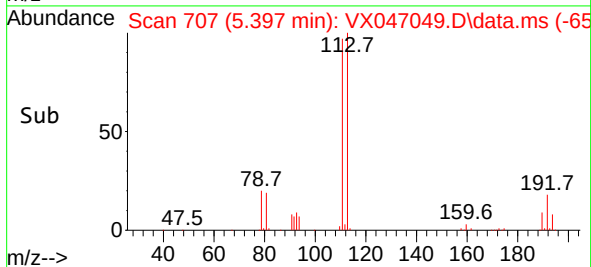
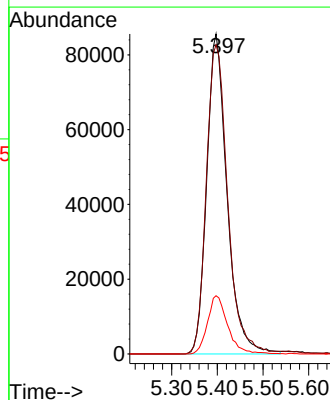
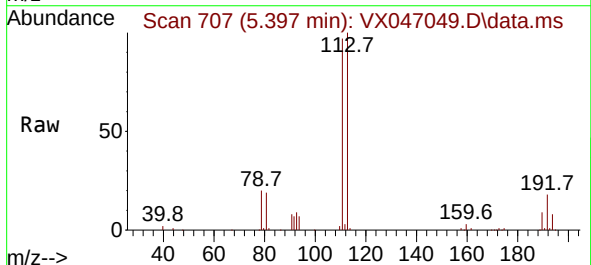




#36
1,1-Dichloropropene
Concen: 5.240 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.146 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 75 Resp: 38054
Ion Ratio Lower Upper
75 100
110 8.9 17.3 51.9#
77 0.0 24.2 36.4#

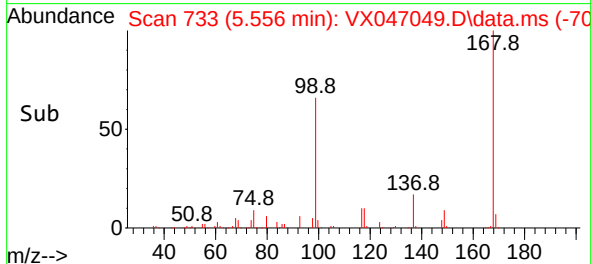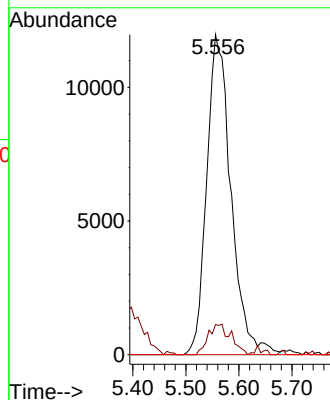

#38
Carbon Tetrachloride
Concen: 5.981 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00

Tgt Ion: 117 Resp: 45917
Ion Ratio Lower Upper
117 100
119 6.7 76.6 114.8#
121 0.0 24.1 36.1#


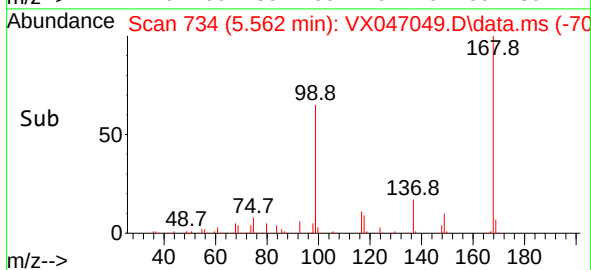
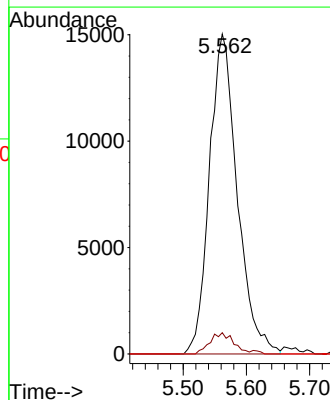
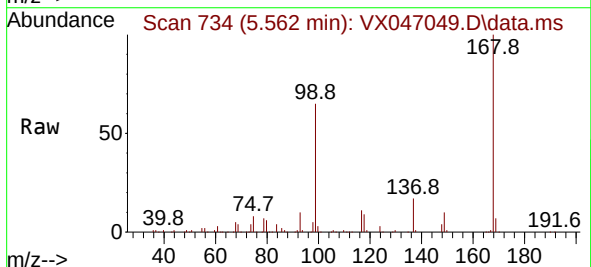


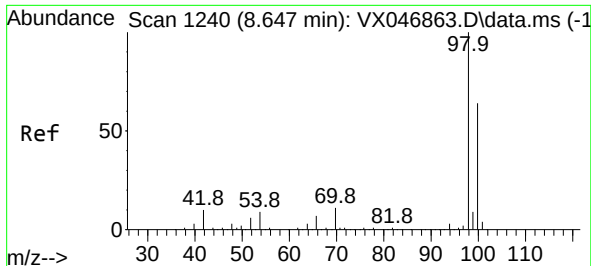

#50
Toluene-d8
Concen: 50.224 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 953764
Ion Ratio Lower Upper
98 100
100 66.5 53.0 79.6

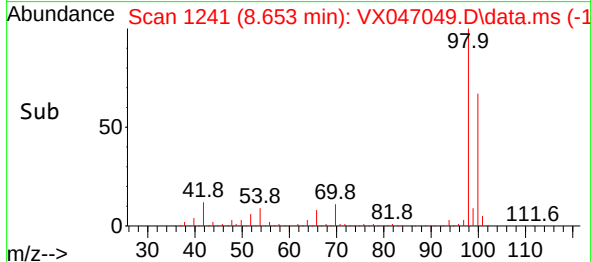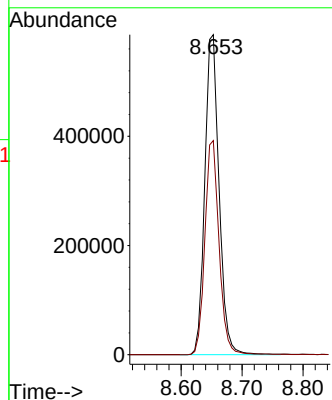

#62
4-Bromofluorobenzene
Concen: 52.731 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00

Tgt Ion: 95 Resp: 380575
Ion Ratio Lower Upper
95 100
174 72.7 0.0 152.0
176 70.1 0.0 145.2


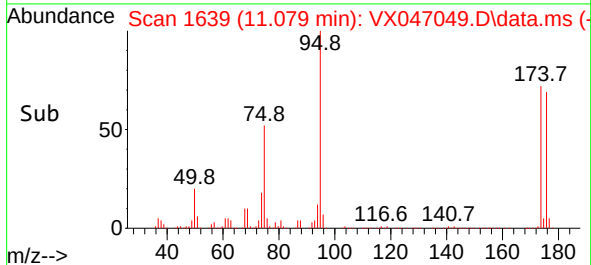
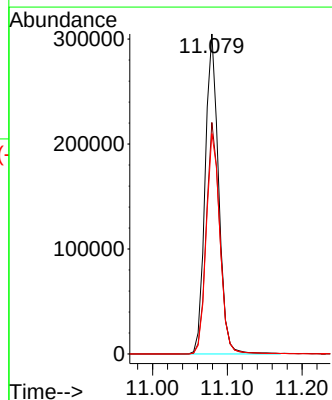
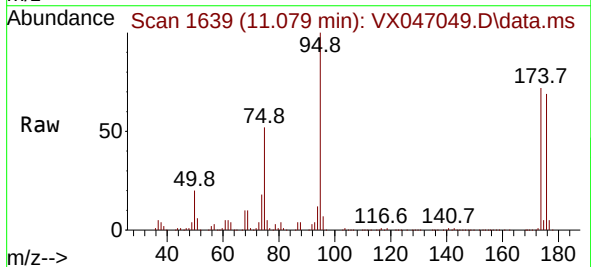


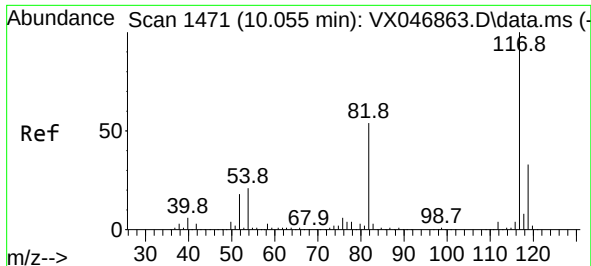

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:117 Resp: 740369
Ion Ratio Lower Upper
117 100
82 58.0 43.3 64.9
119 32.8 26.4 39.6

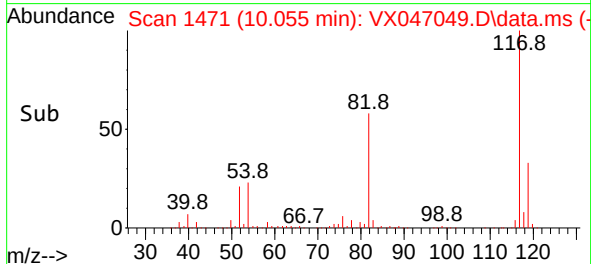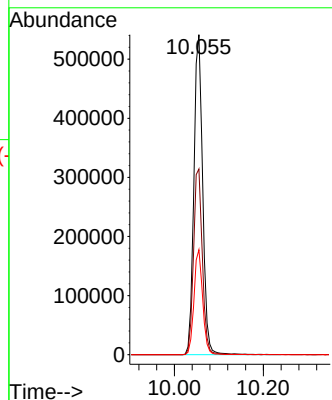

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00

Tgt Ion:152 Resp: 367208
Ion Ratio Lower Upper
152 100
115 61.2 42.4 127.1
150 155.3 0.0 349.2


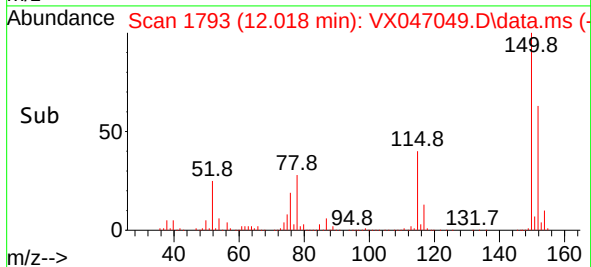
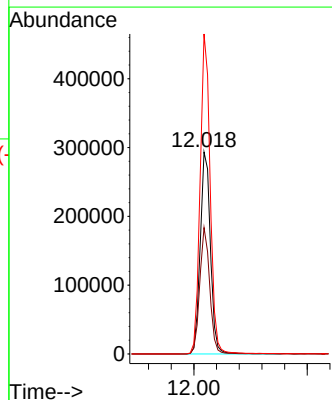
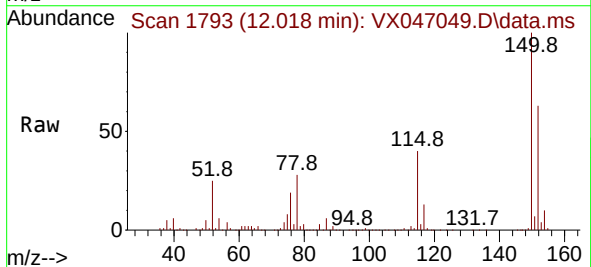


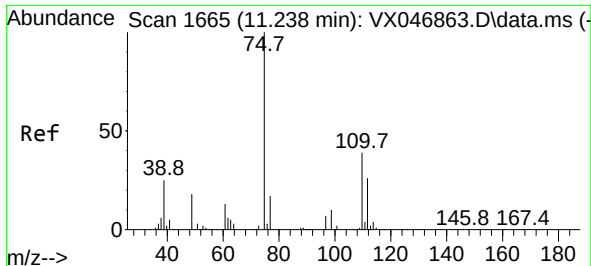

#76
1,2,3-Trichloropropane
Concen: 35.117 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion: 75 Resp: 199251
Ion Ratio Lower Upper
75 100
77 1.1 20.6 61.8#

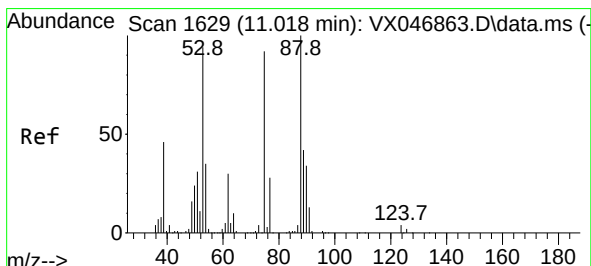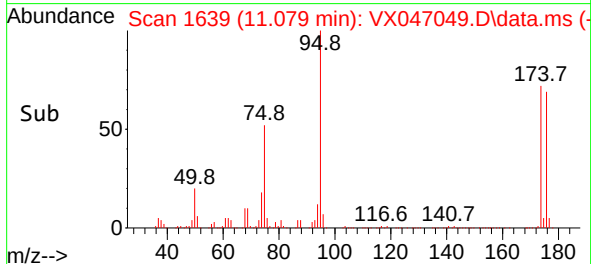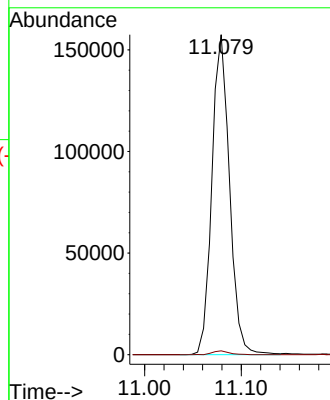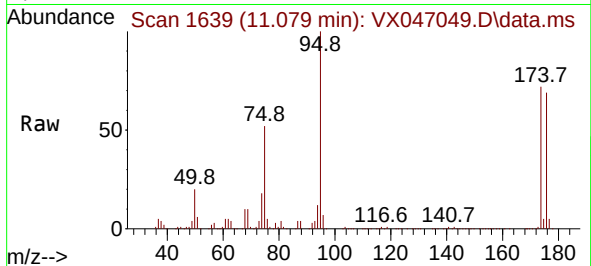

#81
trans-1,4-Dichloro-2-butene
Concen: 94.237 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX047049.D
Acq: 18 Jul 2025 15:00

Tgt Ion: 75 Resp: 199251
Ion Ratio Lower Upper
75 100
53 0.0 83.7 125.5#
89 0.0 38.2 57.2#

