

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
 Data File : VX036867.D
 Acq On : 08 Aug 2023 16:27
 Operator : JC/MD
 Sample : 03903-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-07W

Quant Time: Aug 09 04:16:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 21 12:14:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	121448	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	223402	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	205480	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	91118	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	86359	48.057	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	96.120%
35) Dibromofluoromethane	5.391	113	71796	46.756	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.520%
50) Toluene-d8	8.653	98	267559	49.135	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.280%
62) 4-Bromofluorobenzene	11.079	95	100039	48.694	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.380%


Target Compounds						Qvalue
11) Tert butyl alcohol	2.965	59	283	0.665	ug/l #	78
13) Acrolein	2.233	56	69	0.284	ug/l #	1
16) Acetone	2.386	43	3187	4.274	ug/l #	88
20) Methylene Chloride	2.794	84	444	0.268	ug/l #	77
25) 2-Butanone	4.586	43	780	0.645	ug/l	95
36) 1,1-Dichloropropene	5.556	75	9906	4.328	ug/l #	51
37) Ethyl Acetate	4.586	43	780	0.301	ug/l #	69
38) Carbon Tetrachloride	5.556	117	13038	5.358	ug/l #	14
39) Methylcyclohexane	7.385	83	1761	0.619	ug/l #	75
44) Trichloroethene	7.129	130	468	0.269	ug/l	71
52) Toluene	8.720	92	11752	2.817	ug/l	95
55) 1,1,2-Trichloroethane	9.104	97	1186	0.676	ug/l #	21
60) Dibromochloromethane	9.275	129	4880	2.531	ug/l #	11
64) Tetrachloroethene	9.275	164	4713	3.075	ug/l	96
67) Ethyl Benzene	10.195	91	265156	32.046	ug/l	100
68) m/p-Xylenes	10.299	106	363657	117.794	ug/l	98
69) o-Xylene	10.640	106	126369	41.008	ug/l	99
70) Styrene	10.640	104	6447	1.268	ug/l #	1
73) Isopropylbenzene	10.963	105	37493	4.972	ug/l	98
76) 1,2,3-Trichloropropane	11.378	75	4269	1.992	ug/l #	1
78) n-propylbenzene	11.305	91	115176	13.207	ug/l	99
79) 2-Chlorotoluene	11.378	91	60839	11.513	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	108999	17.278	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	52462	55.482	ug/l #	5
82) 4-Chlorotoluene	11.451	91	12349	2.051	ug/l #	46
83) tert-Butylbenzene	11.750	119	41018	6.619	ug/l #	58
84) 1,2,4-Trimethylbenzene	11.750	105	343535	54.452	ug/l	96
85) sec-Butylbenzene	11.750	105	343535	44.449	ug/l #	57
86) p-Isopropyltoluene	12.012	119	3351	0.527	ug/l	88
89) n-Butylbenzene	12.329	91	15514	2.725	ug/l #	33
90) Hexachloroethane	12.530	117	1899	1.473	ug/l #	17
95) Naphthalene	13.774	128	16421	2.492	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036867.D
Acq On : 08 Aug 2023 16:27
Operator : JC/MD
Sample : 03903-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07W

Quant Time: Aug 09 04:16:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 21 12:14:12 2023
Response via : Initial Calibration




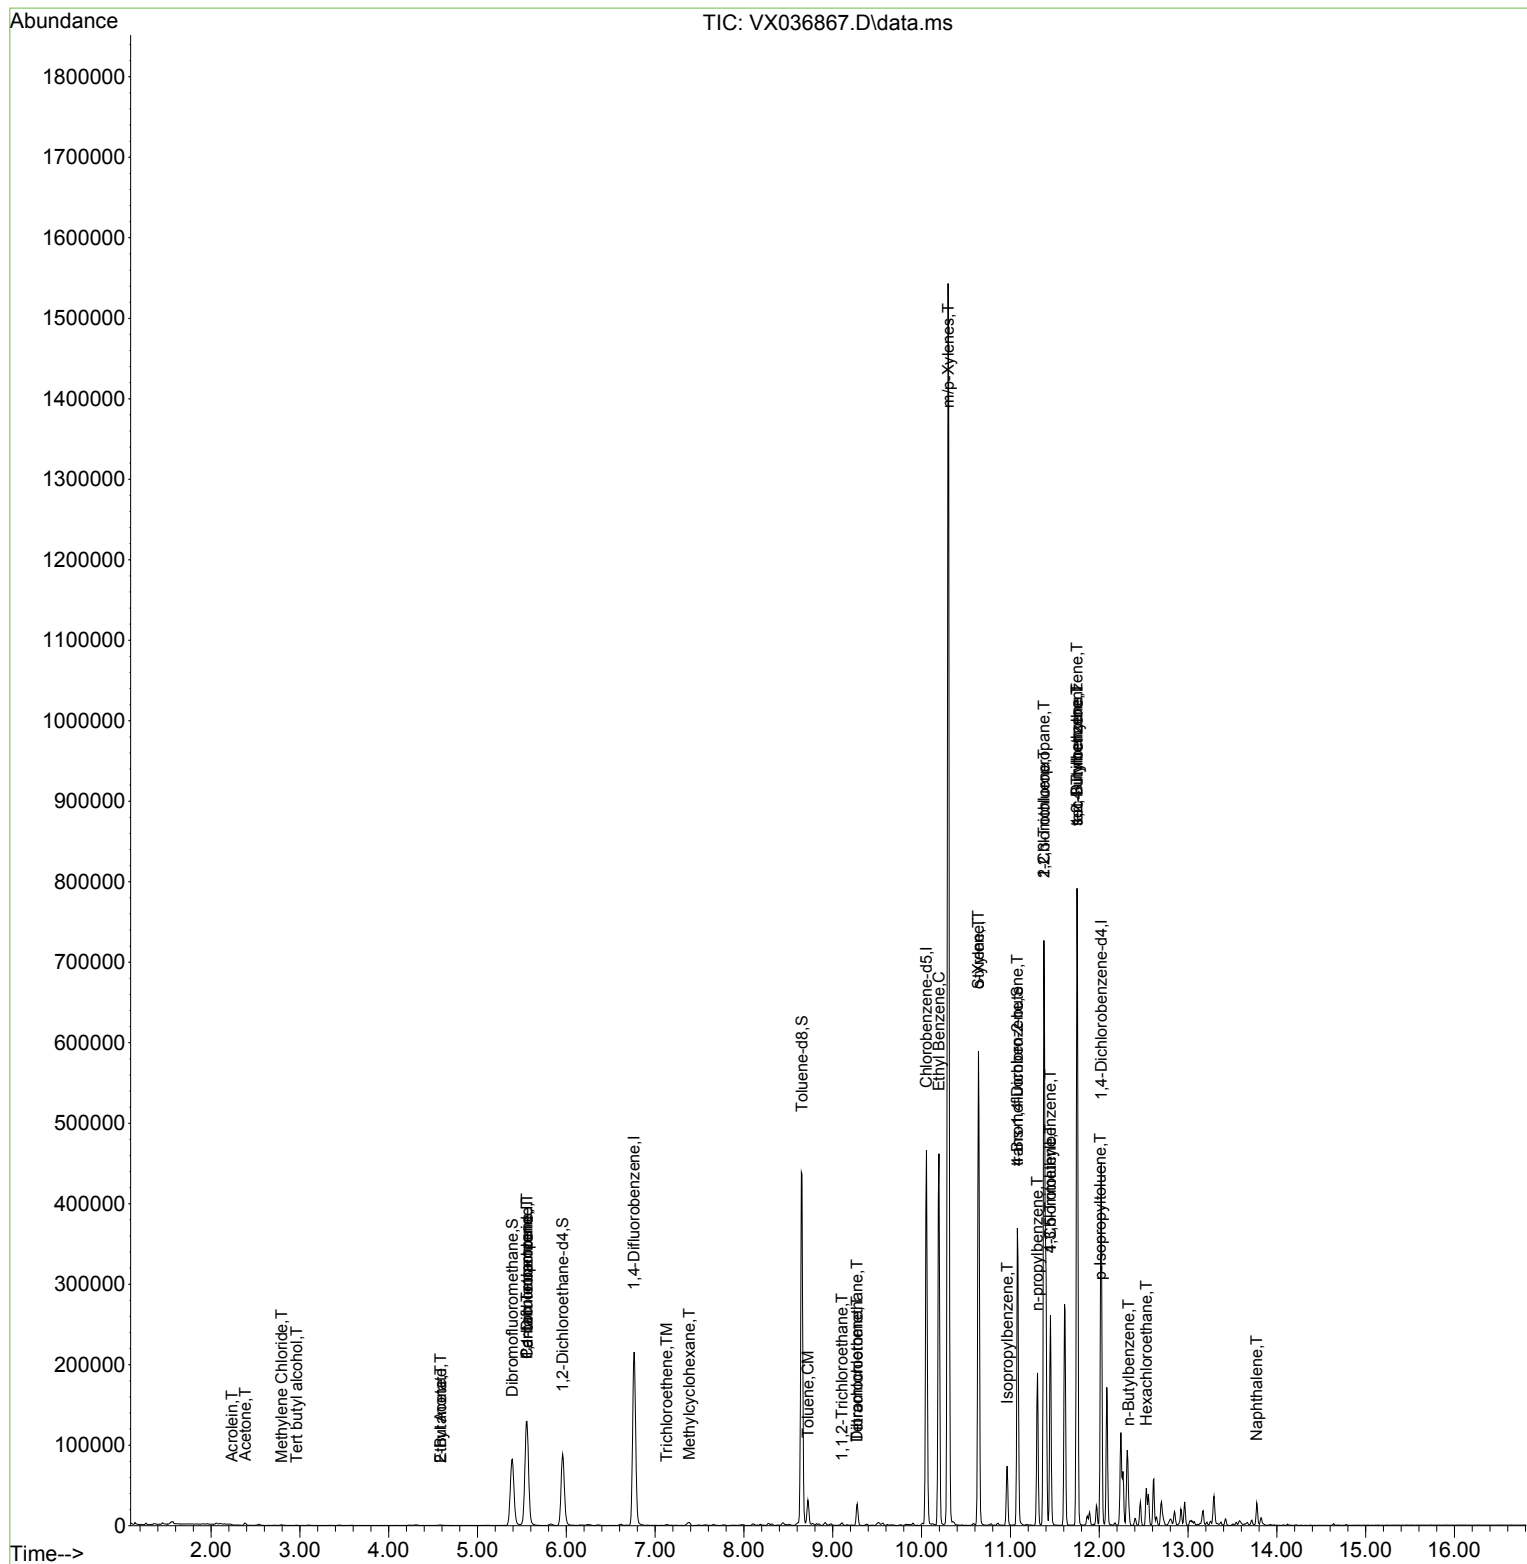


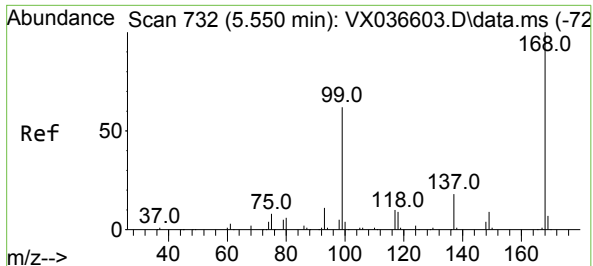

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion:168 Resp: 121448
Ion Ratio Lower Upper
168 100
99 62.3 56.6 85.0

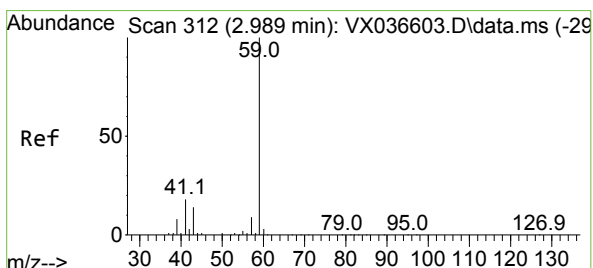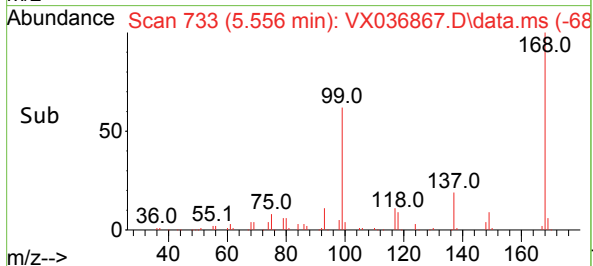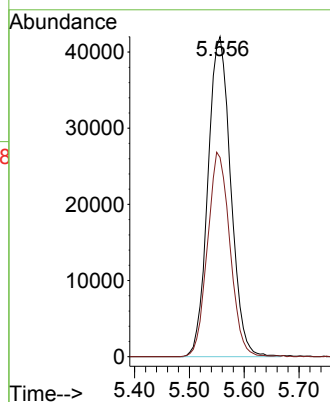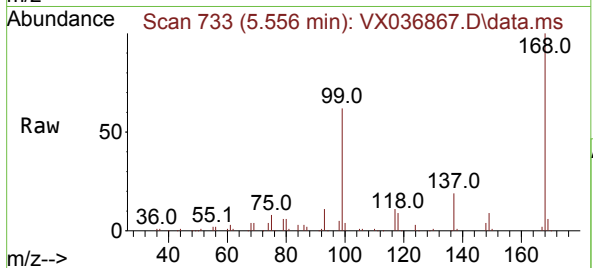

#11
Tert butyl alcohol
Concen: 0.665 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.024 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion: 59 Resp: 283
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#


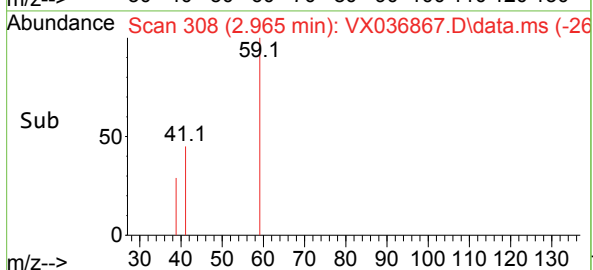

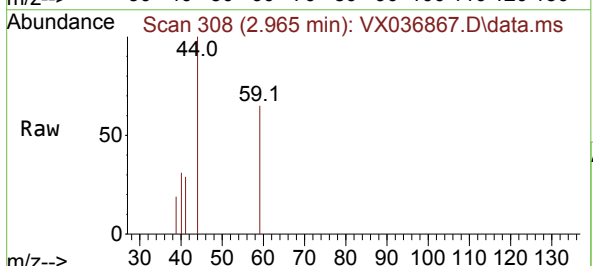


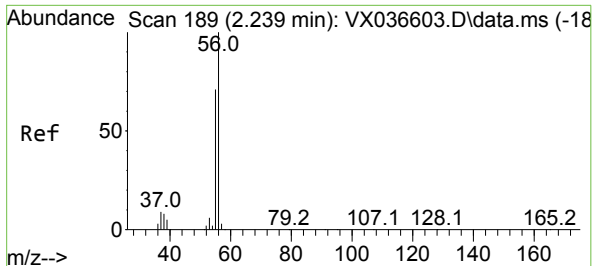

#13
Acrolein
Concen: 0.284 ug/l
RT: 2.233 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion: 56 Resp: 69
Ion Ratio Lower Upper
56 100
55 258.0 57.1 85.7#

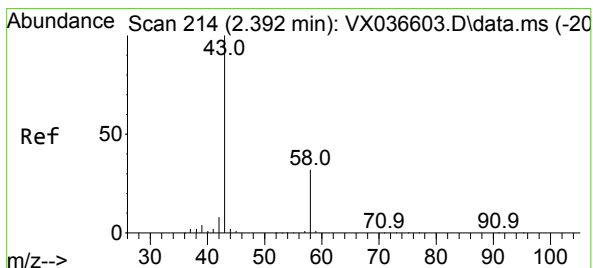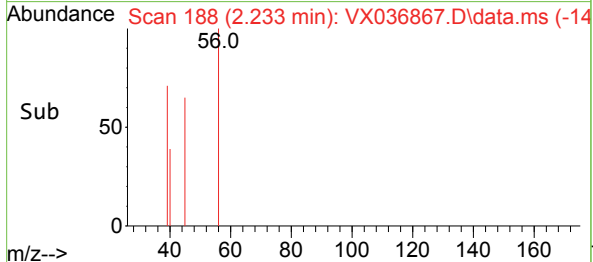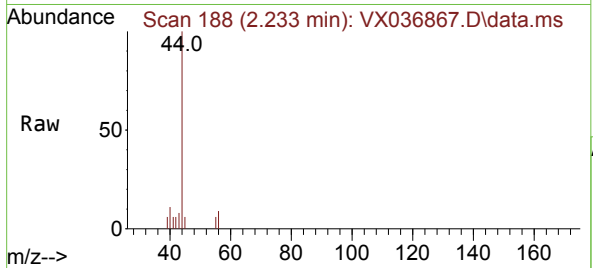

#16
Acetone
Concen: 4.274 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion: 43 Resp: 3187
Ion Ratio Lower Upper
43 100
58 33.7 21.9 32.9#

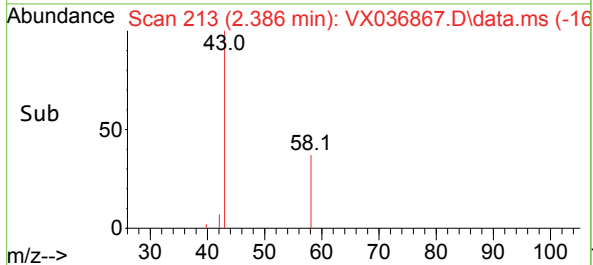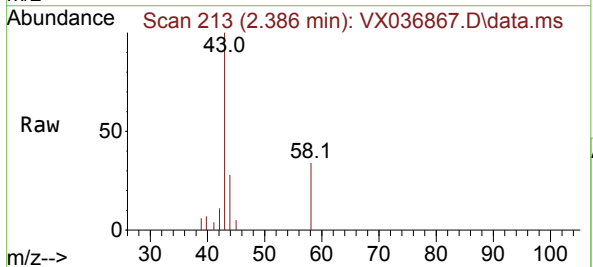

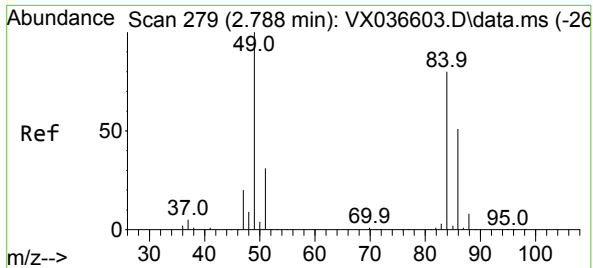

#20

Methylene Chloride

Concen: 0.268 ug/l

RT: 2.794 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX036867.D

Acq: 08 Aug 2023 16:27

Instrument :

MSVOA_X

ClientSampleId :

MW-07W

Tgt Ion: 84 Resp: 444





Ion Ratio Lower Upper

84 100

49 98.0 103.6 155.4#

51 26.6 33.8 50.6#

86 52.5 49.4 74.0

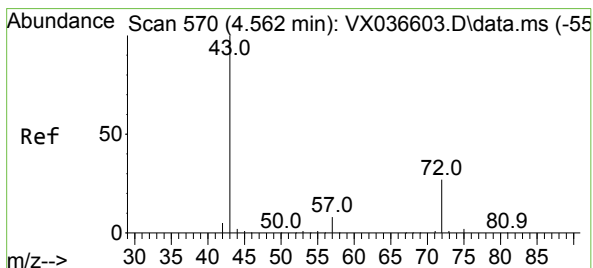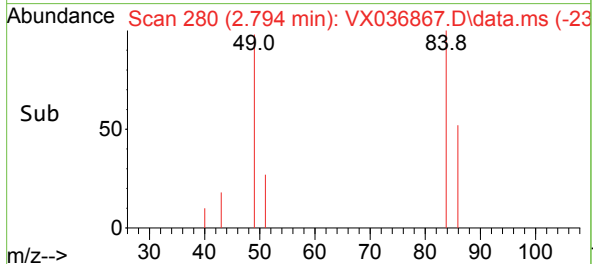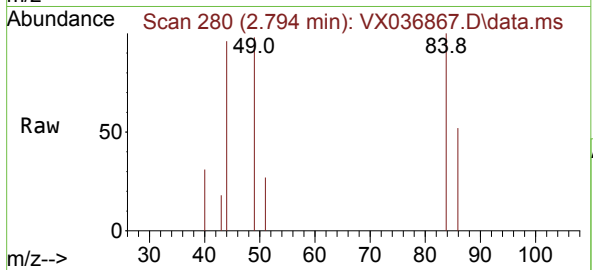

#25

2-Butanone

Concen: 0.645 ug/l

RT: 4.586 min Scan# 574

Delta R.T. 0.024 min

Lab File: VX036867.D




Acq: 08 Aug 2023 16:27


Tgt Ion: 43 Resp: 780

Ion Ratio Lower Upper

43 100

72 26.8 19.4 29.2


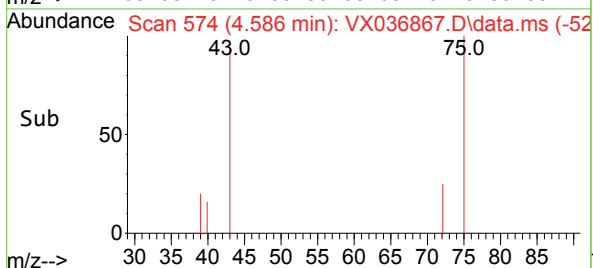

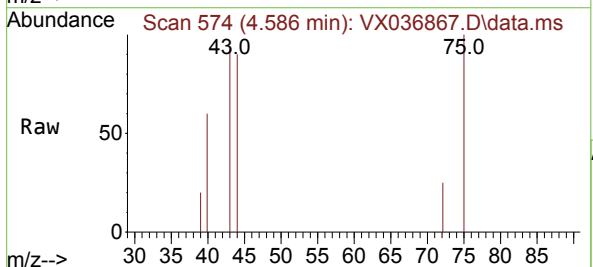




#33
 1,2-Dichloroethane-d4
 Concen: 48.057 ug/l
 RT: 5.958 min Scan# 798
 Delta R.T. 0.006 min
 Lab File: VX036867.D
 Acq: 08 Aug 2023 16:27




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-07W


Tgt Ion: 65 Resp: 86359
 Ion Ratio Lower Upper
 65 100
 67 51.7 0.0 100.2

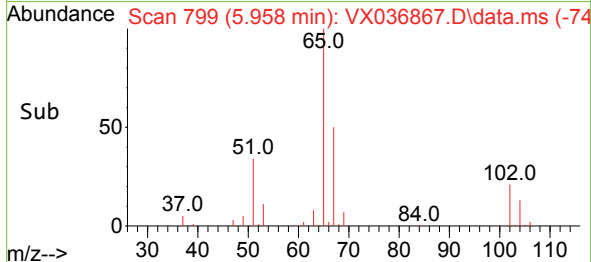

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. -0.000 min
 Lab File: VX036867.D
 Acq: 08 Aug 2023 16:27

Tgt Ion: 114 Resp: 223402
 Ion Ratio Lower Upper
 114 100
 63 20.2 0.0 45.0
 88 16.7 0.0 36.6


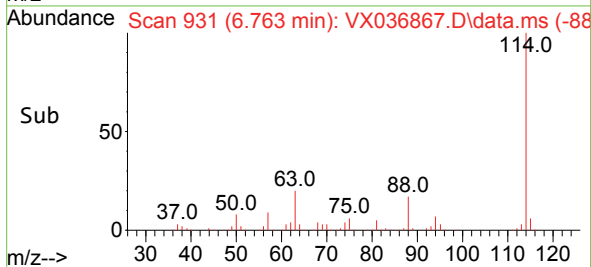

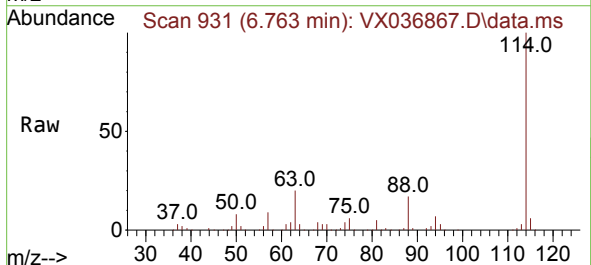


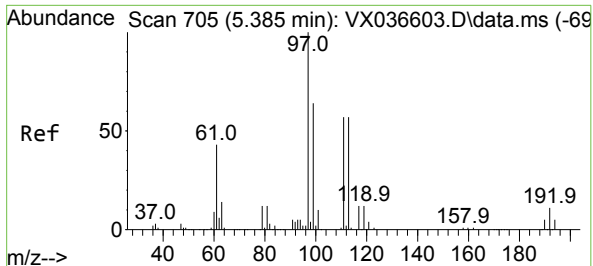

#35
Dibromofluoromethane
Concen: 46.756 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion:113 Resp: 71796
Ion Ratio Lower Upper
113 100
111 104.2 82.9 124.3
192 18.3 13.3 19.9

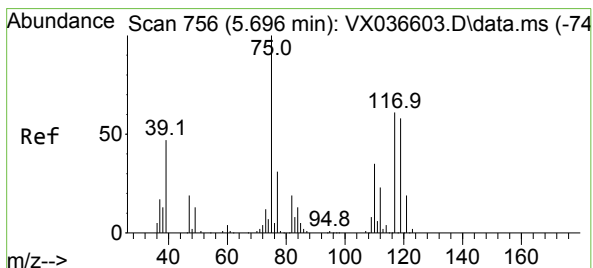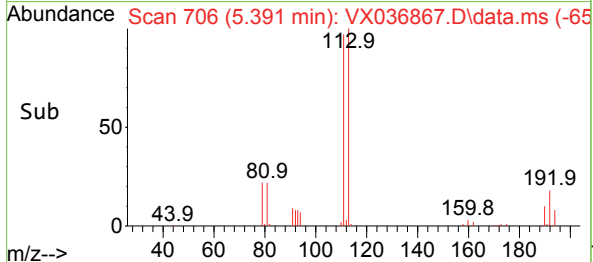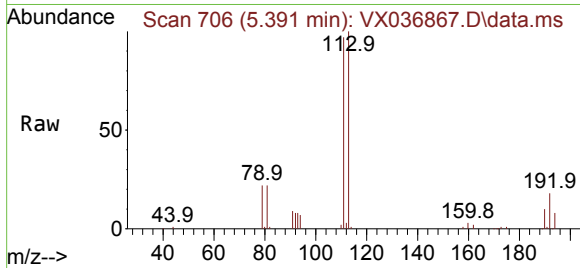

#36
1,1-Dichloropropene
Concen: 4.328 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion: 75 Resp: 9906
Ion Ratio Lower Upper
75 100
110 9.7 17.0 50.9#
77 0.0 24.7 37.1#


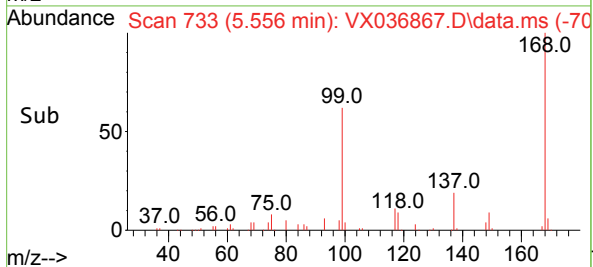

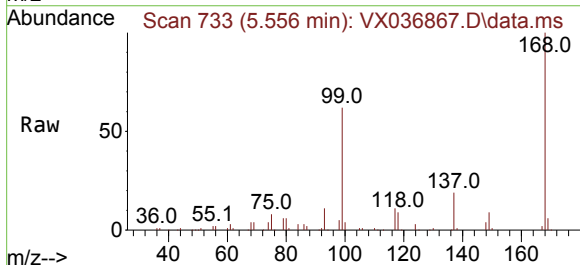




#37
Ethyl Acetate
Concen: 0.301 ug/l
RT: 4.586 min Scan# 51
Delta R.T. -0.128 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion: 43	Resp:	780
Ion	Ratio	Lower Upper
43	100	
61	0.0	10.6 16.0#
70	0.0	8.3 12.5#

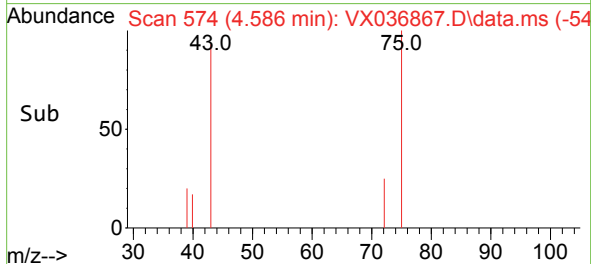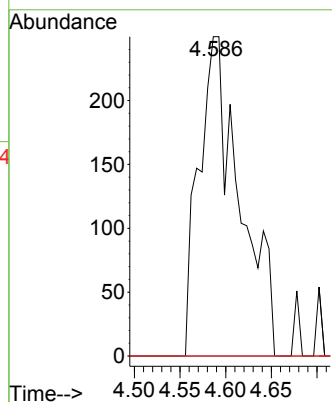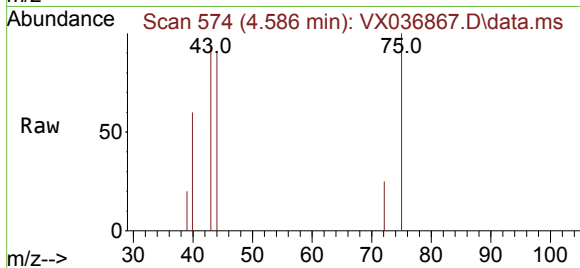

#38
Carbon Tetrachloride
Concen: 5.358 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.122 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion: 117	Resp:	13038
Ion	Ratio	Lower Upper
117	100	
119	3.7	78.2 117.2#
121	0.0	24.4 36.6#




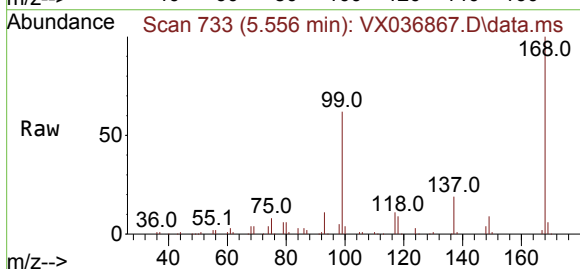




#39
Methylcyclohexane
Concen: 0.619 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion: 83 Resp: 1761
Ion Ratio Lower Upper
83 100
55 57.2 64.6 97.0#
98 59.8 36.7 55.1#

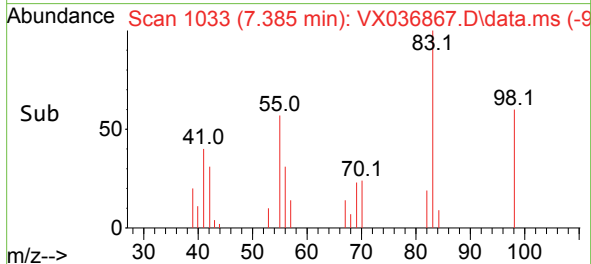

#44
Trichloroethene
Concen: 0.269 ug/l
RT: 7.129 min Scan# 991
Delta R.T. 0.006 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion:130 Resp: 468
Ion Ratio Lower Upper
130 100
95 72.7 0.0 204.4




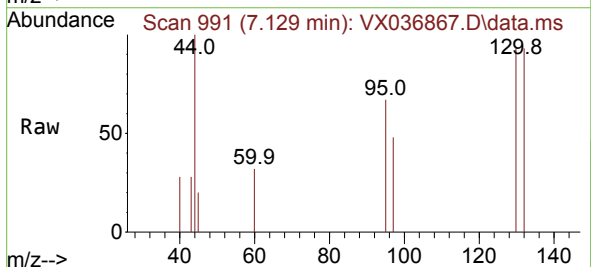




#50
Toluene-d8
Concen: 49.135 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.006 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion: 98 Resp: 267559
Ion Ratio Lower Upper
98 100
100 65.6 53.1 79.7

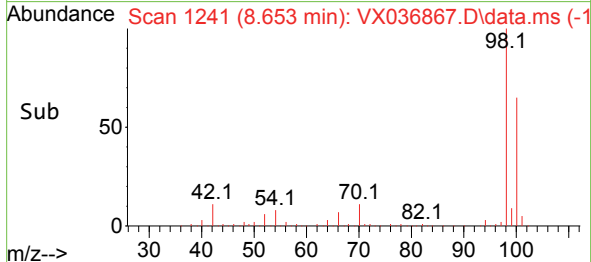

#52
Toluene
Concen: 2.817 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion: 92 Resp: 11752
Ion Ratio Lower Upper
92 100
91 174.8 134.2 201.2

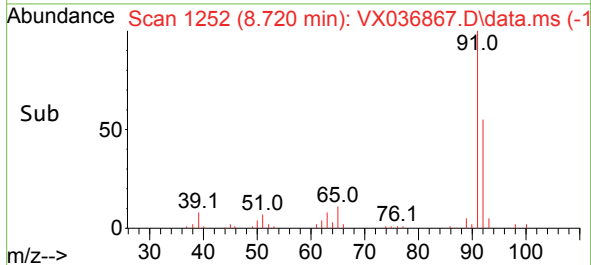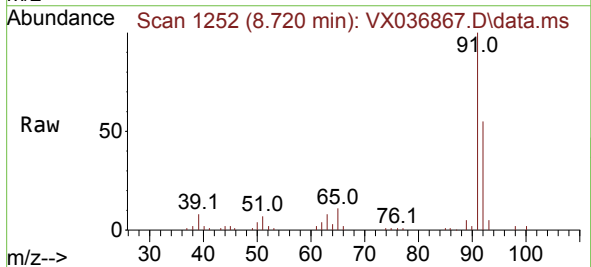



#55

1,1,2-Trichloroethane

Concen: 0.676 ug/l

RT: 9.104 min Scan# 1186

Delta R.T. -0.049 min

Lab File: VX036867.D

Acq: 08 Aug 2023 16:27

Instrument :

MSVOA_X

ClientSampleId :

MW-07W

Tgt Ion: 97 Resp: 1186





Ion Ratio Lower Upper

97 100

83 8.1 65.8 98.8#

85 0.0 41.6 62.4#

99 0.0 47.8 71.8#

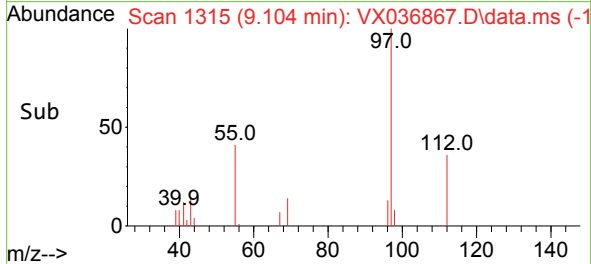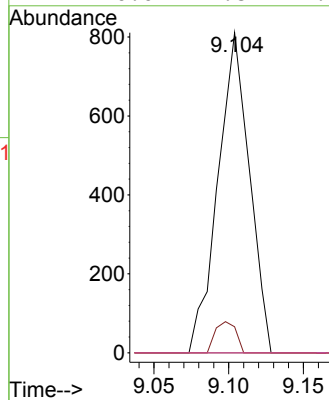

#60

Dibromochloromethane

Concen: 2.531 ug/l

RT: 9.275 min Scan# 1343

Delta R.T. -0.244 min

Lab File: VX036867.D




Acq: 08 Aug 2023 16:27


Tgt Ion: 129 Resp: 4880

Ion Ratio Lower Upper

129 100

127 0.0 38.8 116.4#



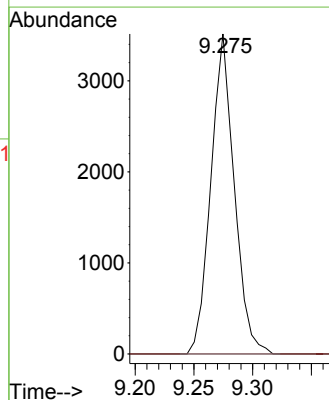
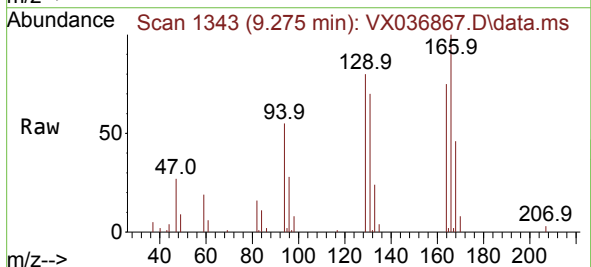




#62
4-Bromofluorobenzene
Concen: 48.694 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion: 95 Resp: 100039
Ion Ratio Lower Upper
95 100
174 72.4 0.0 135.6
176 70.7 0.0 131.0

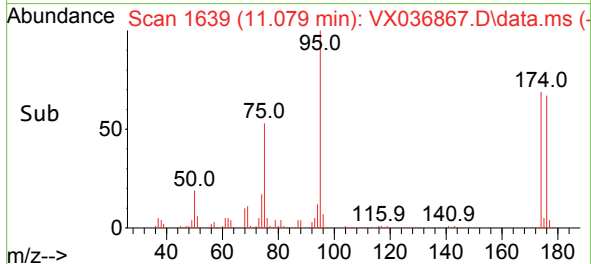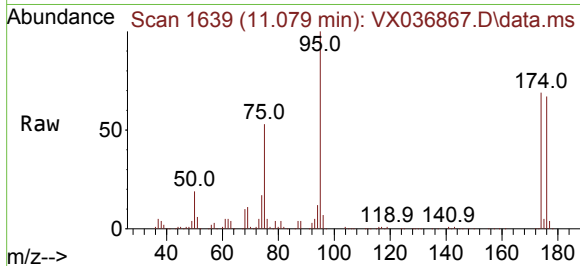

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion: 117 Resp: 205480
Ion Ratio Lower Upper
117 100
82 57.0 46.2 69.4
119 32.5 25.5 38.3

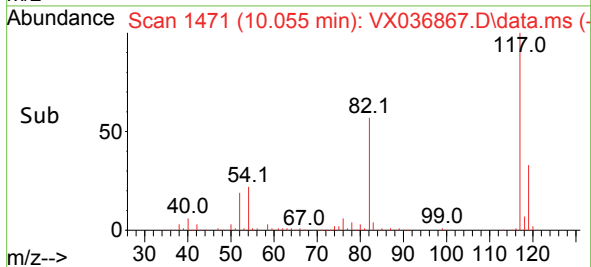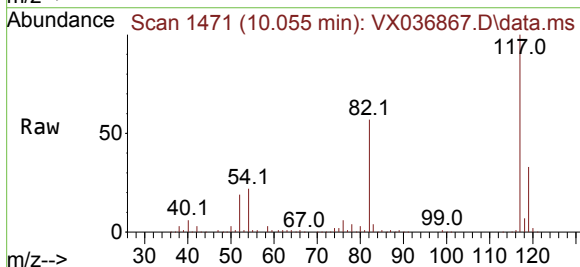







#64
Tetrachloroethene
Concen: 3.075 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Instrument :
MSVOA_X
ClientSampleId :
MW-07W

Tgt Ion:164 Resp: 4713




Ion	Ratio	Lower	Upper
164	100		
166	132.8	102.7	154.1
129	105.9	80.4	120.6
131	92.4	76.5	114.7

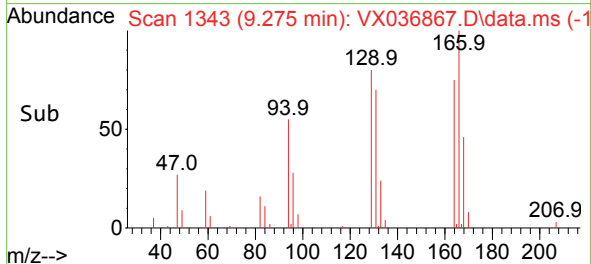


#67
Ethyl Benzene
Concen: 32.046 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion: 91 Resp: 265156

Ion	Ratio	Lower	Upper
91	100		
106	31.3	24.9	37.3




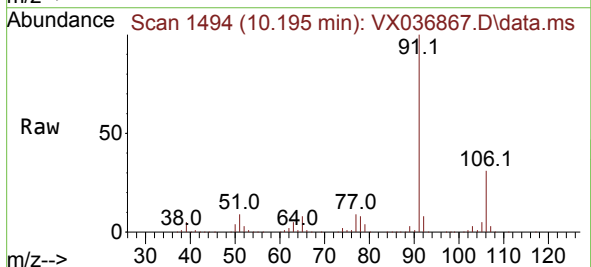


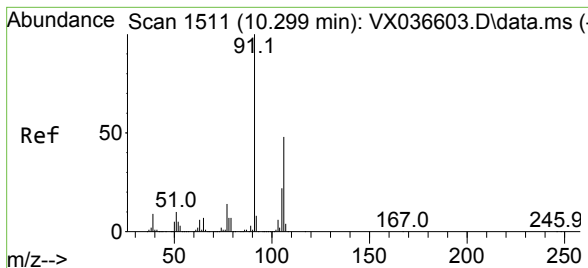

#68
m/p-Xylenes
Concen: 117.794 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion:106 Resp: 363657
Ion Ratio Lower Upper
106 100
91 203.4 165.5 248.3

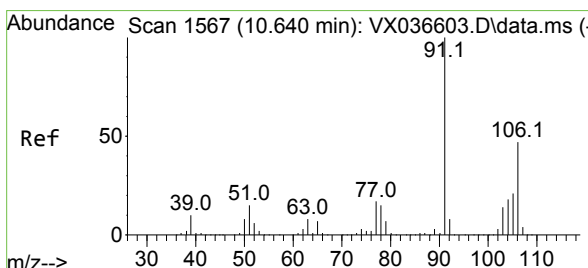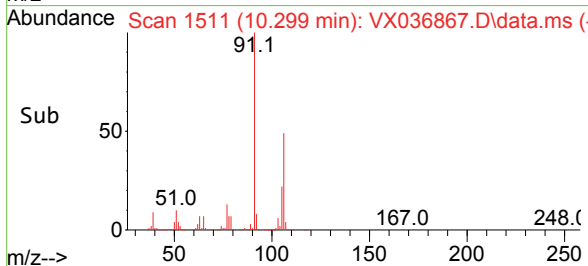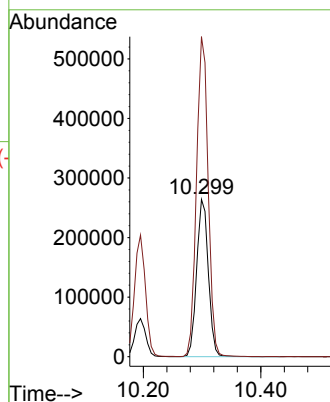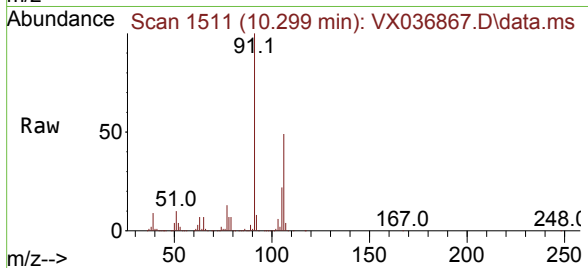

#69
o-Xylene
Concen: 41.008 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion:106 Resp: 126369
Ion Ratio Lower Upper
106 100
91 219.9 108.9 326.8

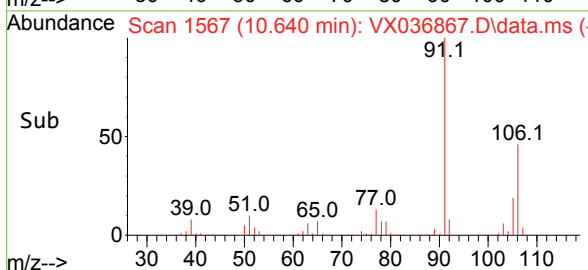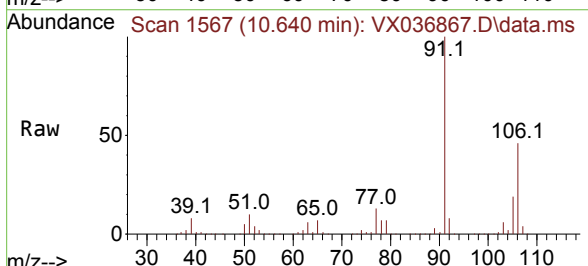



#70

Styrene

Concen: 1.268 ug/l

RT: 10.640 min Scan# 11

Delta R.T. -0.012 min

Lab File: VX036867.D

Acq: 08 Aug 2023 16:27

Instrument :

MSVOA_X

ClientSampleId :

MW-07W





Tgt Ion:104 Resp: 6447

Ion Ratio Lower Upper

104 100

78 309.7 43.6 65.4#

103 270.8 43.6 65.4#

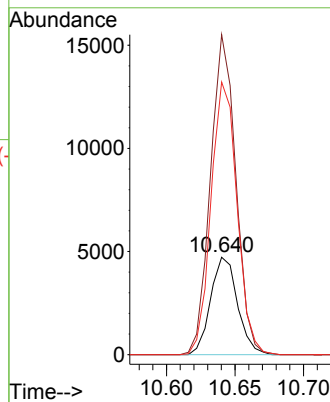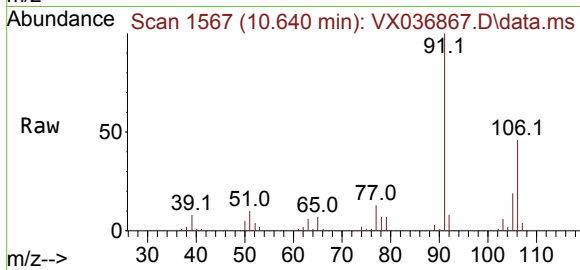

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX036867.D

Acq: 08 Aug 2023 16:27




Tgt Ion:152 Resp: 91118


Ion Ratio Lower Upper

152 100

115 62.5 43.3 129.9

150 157.2 0.0 345.0


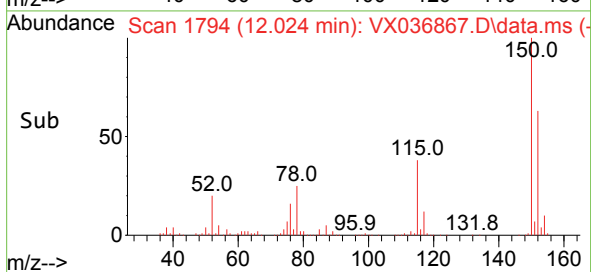

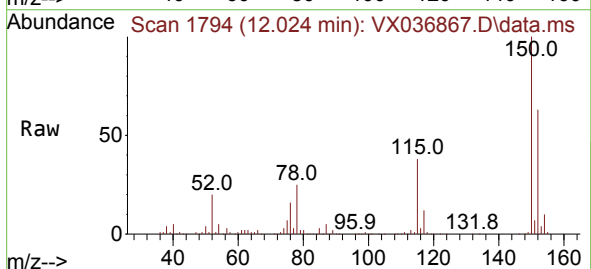




#73
Isopropylbenzene
Concen: 4.972 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion:105 Resp: 37493
Ion Ratio Lower Upper
105 100
120 26.8 12.9 38.6

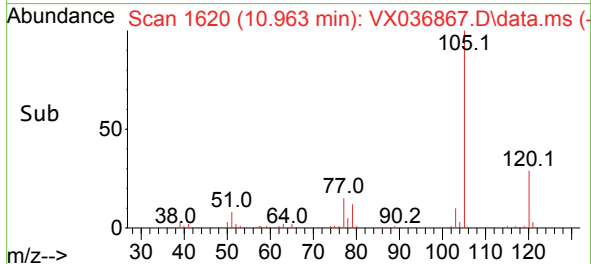

#76
1,2,3-Trichloropropane
Concen: 1.992 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.140 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion: 75 Resp: 4269
Ion Ratio Lower Upper
75 100
77 1357.9 19.1 57.5#

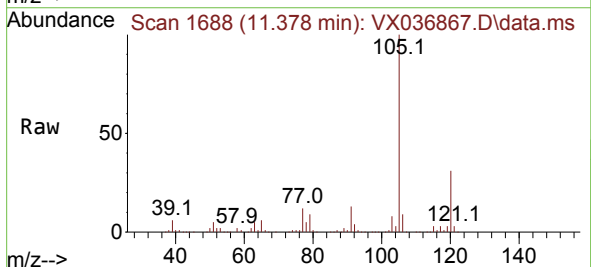

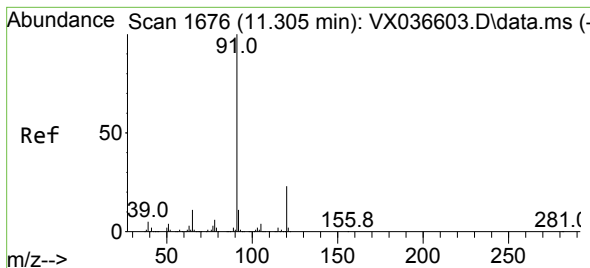

#78

n-propylbenzene

Concen: 13.207 ug/l

RT: 11.305 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX036867.D

Acq: 08 Aug 2023 16:27

Instrument :

MSVOA_X

ClientSampleId :





MW-07W

Tgt Ion: 91 Resp: 115176

Ion Ratio Lower Upper

91 100

120 22.6 11.5 34.4

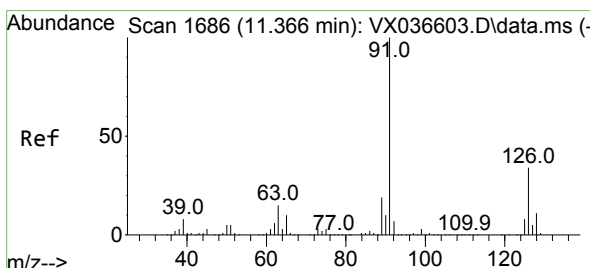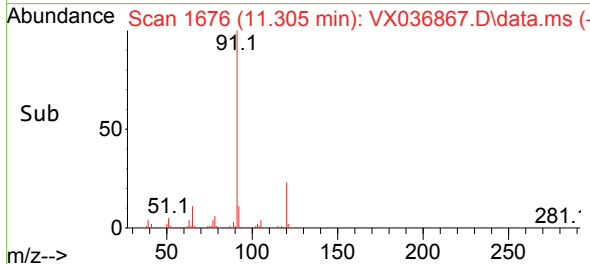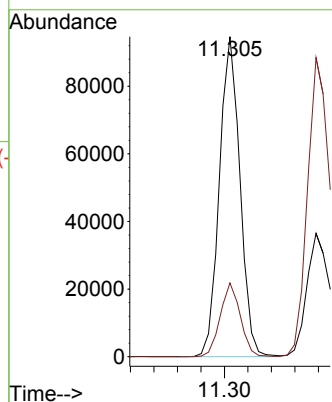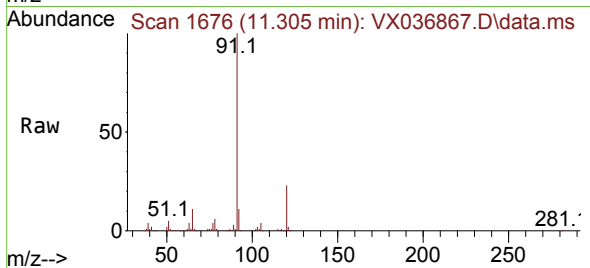

#79

2-Chlorotoluene

Concen: 11.513 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.012 min

Lab File: VX036867.D




Acq: 08 Aug 2023 16:27


Tgt Ion: 91 Resp: 60839

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.8#

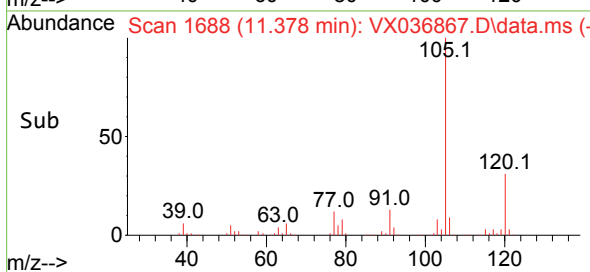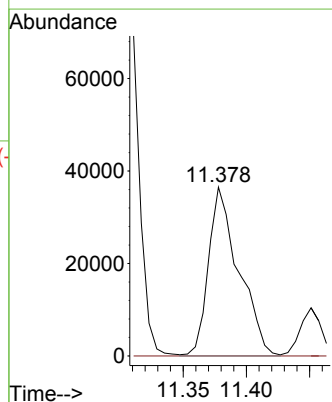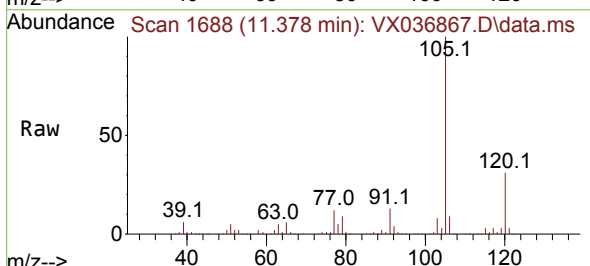



#80

1,3,5-Trimethylbenzene

Concen: 17.278 ug/l

RT: 11.451 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX036867.D

Acq: 08 Aug 2023 16:27

Instrument :

MSVOA_X

ClientSampleId :





MW-07W

Tgt Ion:105 Resp: 108999

Ion Ratio Lower Upper

105 100

120 48.0 24.1 72.3

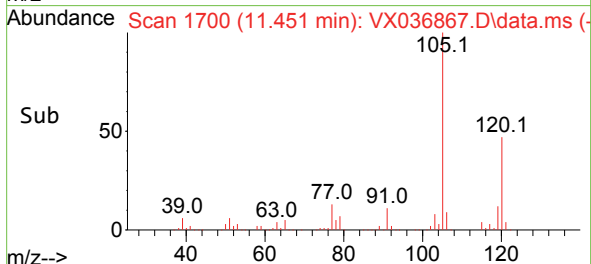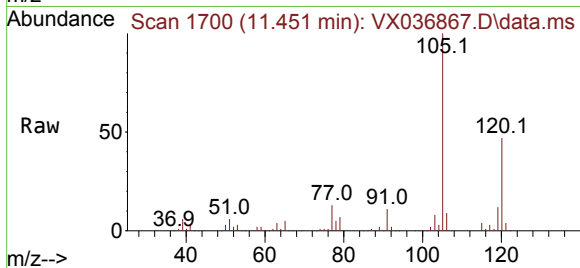

#81

trans-1,4-Dichloro-2-butene

Concen: 55.482 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX036867.D

Acq: 08 Aug 2023 16:27




Tgt Ion: 75 Resp: 52462


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#




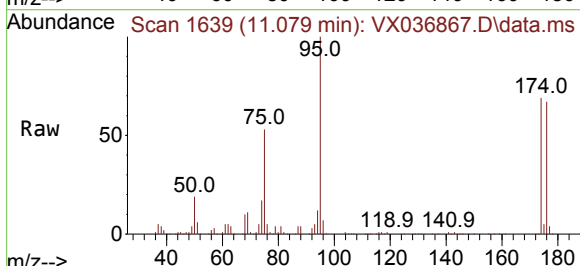




#82
4-Chlorotoluene
Concen: 2.051 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion: 91 Resp: 12349
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.6#



#83
tert-Butylbenzene
Concen: 6.619 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.037 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion: 119 Resp: 41018
Ion Ratio Lower Upper
119 100
91 93.3 31.2 93.6
134 0.0 11.7 35.0#









#84
1,2,4-Trimethylbenzene
Concen: 54.452 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27




Instrument :
MSVOA_X
ClientSampleId :
MW-07W


Tgt Ion:105 Resp: 343535
Ion Ratio Lower Upper
105 100
120 44.9 21.2 63.6

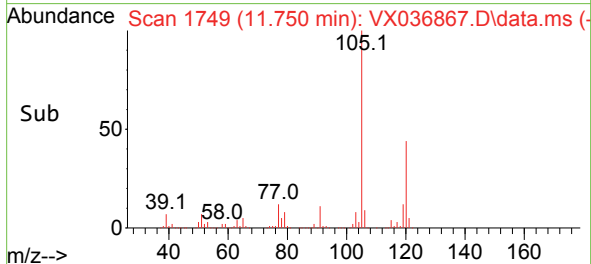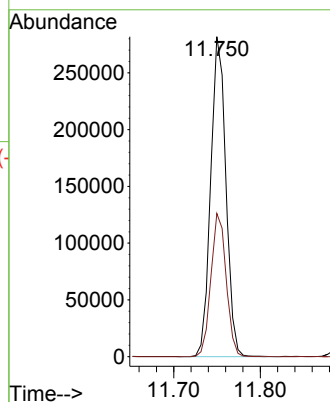

#85
sec-Butylbenzene
Concen: 44.449 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion:105 Resp: 343535
Ion Ratio Lower Upper
105 100
134 0.0 9.8 29.4#





#86

p-Isopropyltoluene

Concen: 0.527 ug/l

RT: 12.012 min Scan# 119

Delta R.T. 0.006 min

Lab File: VX036867.D

Acq: 08 Aug 2023 16:27

Instrument :

MSVOA_X

ClientSampleId :

MW-07W





Tgt Ion:119 Resp: 3351

Ion Ratio Lower Upper

119 100

134 26.9 12.8 38.3

91 37.2 13.1 39.3

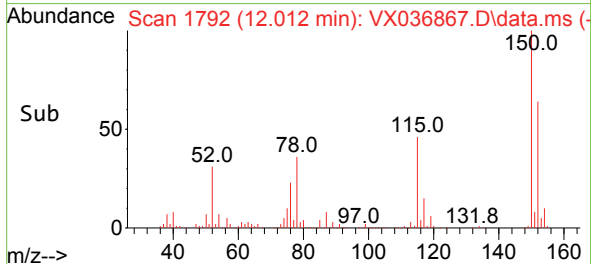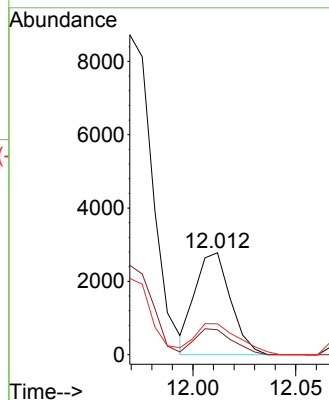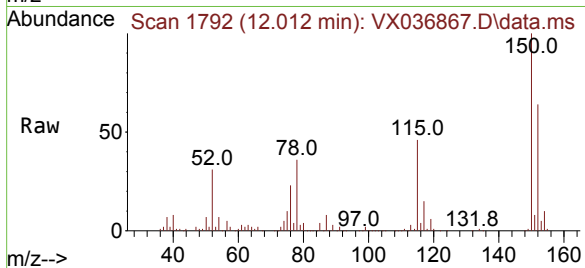

#89

n-Butylbenzene

Concen: 2.725 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min

Lab File: VX036867.D

Acq: 08 Aug 2023 16:27




Tgt Ion: 91 Resp: 15514


Ion Ratio Lower Upper

91 100

92 32.0 27.4 82.0

134 97.2 12.6 37.8#


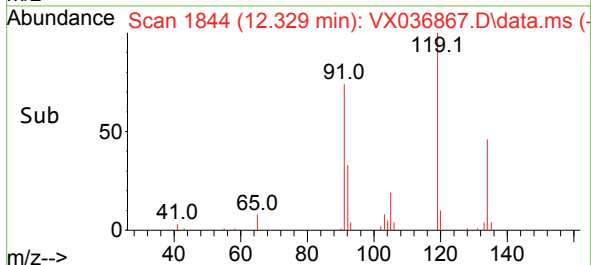
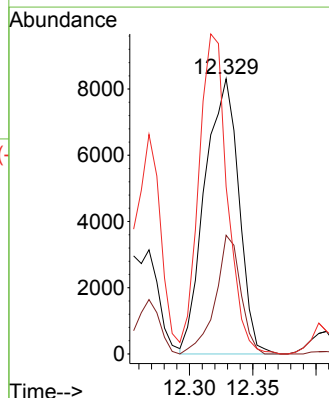
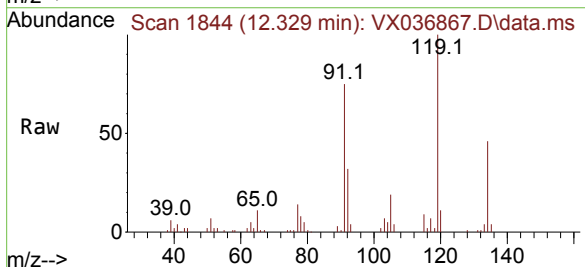




#90
Hexachloroethane
Concen: 1.473 ug/l
RT: 12.530 min Scan# 1878
Delta R.T. -0.006 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Instrument :
MSVOA_X
ClientSampleId :
MW-07W

Tgt Ion:117 Resp: 1899
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

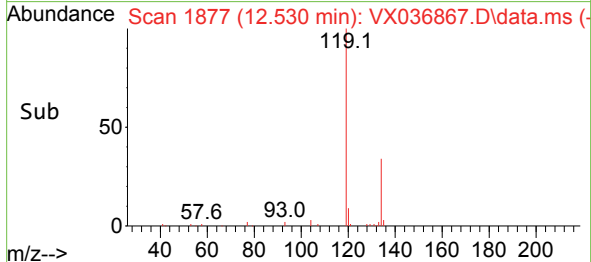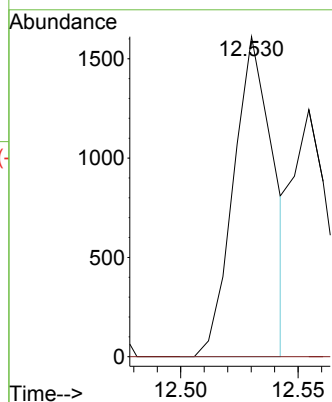

#95
Naphthalene
Concen: 2.492 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX036867.D
Acq: 08 Aug 2023 16:27

Tgt Ion:128 Resp: 16421
Ion Ratio Lower Upper
128 100
127 12.6 10.3 15.5
129 10.8 8.8 13.2

