

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
 Data File : VX036863.D
 Acq On : 08 Aug 2023 14:51
 Operator : JC/MD
 Sample : 03903-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-03W

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260

Signal : TIC: VX036863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	19	rVB	6498	8000	1.13%	0.178%
2	1.453	55	60	65	rBV	6995	8563	1.21%	0.190%
3	2.105	163	167	172	rVB2	5635	8320	1.18%	0.185%
4	2.379	206	212	221	rBV	8171	14178	2.01%	0.315%
5	5.391	694	706	720	rBV	81875	242269	34.27%	5.380%
6	5.556	722	733	750	rVB	131988	375374	53.10%	8.336%
7	5.958	788	799	810	rBV	88702	233062	32.97%	5.176%
8	6.763	922	931	948	rBV	215719	518101	73.29%	11.506%
9	8.647	1234	1240	1249	rBV	437028	706941	100.00%	15.700%
10	10.055	1465	1471	1482	rBV	472525	633063	89.55%	14.059%
11	10.195	1489	1494	1505	rVV	159352	211092	29.86%	4.688%
12	10.305	1505	1512	1519	rVB	13852	20564	2.91%	0.457%
13	10.640	1562	1567	1574	rBV	51308	68939	9.75%	1.531%
14	10.963	1614	1620	1626	rBV	9614	12979	1.84%	0.288%
15	11.079	1634	1639	1651	rBV	372758	487385	68.94%	10.824%
16	11.305	1671	1676	1683	rBV	11007	13511	1.91%	0.300%
17	11.451	1696	1700	1708	rVB	8179	10854	1.54%	0.241%
18	11.609	1722	1726	1732	rBV	28456	36433	5.15%	0.809%
19	11.750	1745	1749	1758	rVB	50675	63724	9.01%	1.415%
20	12.018	1788	1793	1800	rBV	452584	585343	82.80%	12.999%
21	12.085	1800	1804	1809	rVB	18572	23049	3.26%	0.512%
22	12.243	1822	1830	1838	rBV2	34449	51421	7.27%	1.142%
23	12.317	1838	1842	1852	rVB4	4122	8771	1.24%	0.195%
24	12.530	1873	1877	1879	rBV	6331	7960	1.13%	0.177%
25	12.615	1885	1891	1894	rBV	12887	16577	2.34%	0.368%
26	12.701	1900	1905	1912	rVB2	12217	18071	2.56%	0.401%
27	12.847	1925	1929	1937	rBV3	6414	9873	1.40%	0.219%
28	12.920	1937	1941	1944	rVV	6741	7773	1.10%	0.173%
29	12.963	1944	1948	1952	rVB	14818	17613	2.49%	0.391%
30	13.170	1976	1982	1990	rBV	12100	15796	2.23%	0.351%
31	13.292	1995	2002	2007	rBV2	30553	42076	5.95%	0.934%
32	13.420	2019	2023	2028	rVB2	9867	12047	1.70%	0.268%
33	13.780	2077	2082	2091	rVB	9330	13229	1.87%	0.294%




Sum of corrected areas: 4502951

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036863.D
Acq On : 08 Aug 2023 14:51
Operator : JC/MD
Sample : 03903-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-03W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

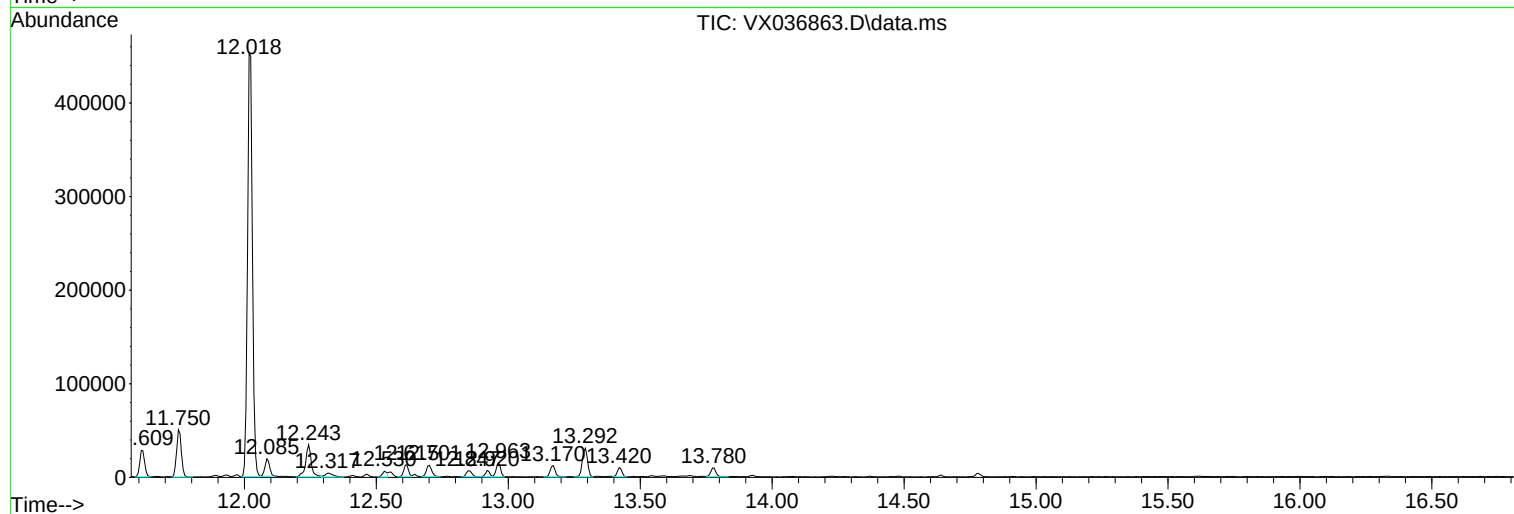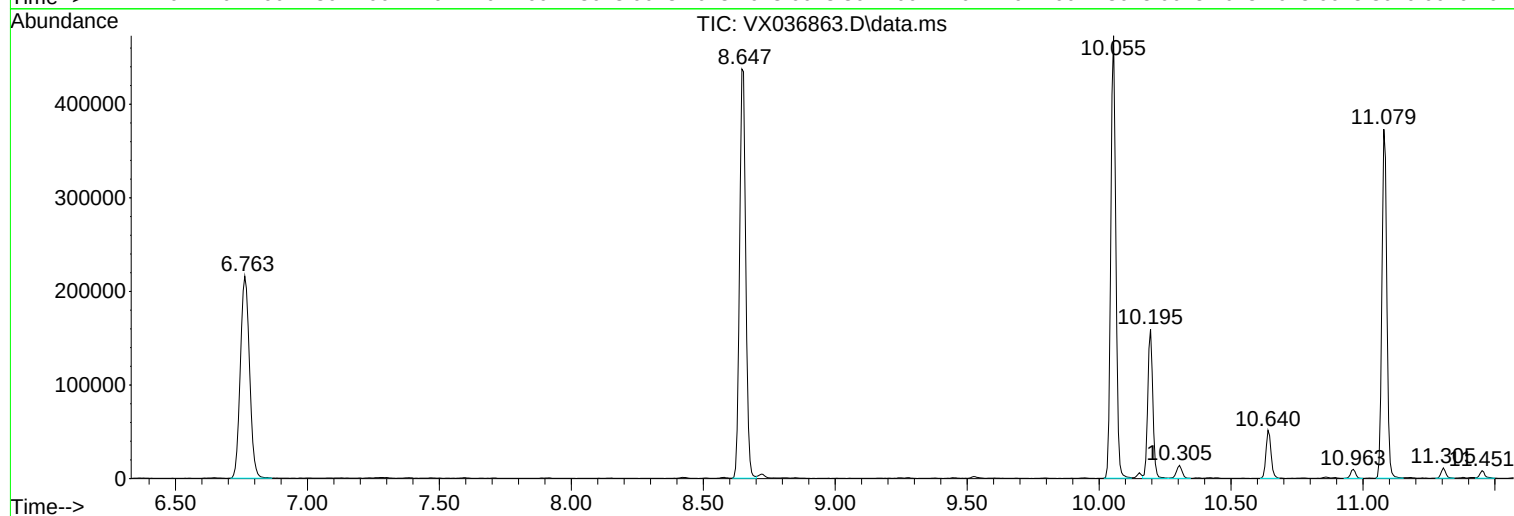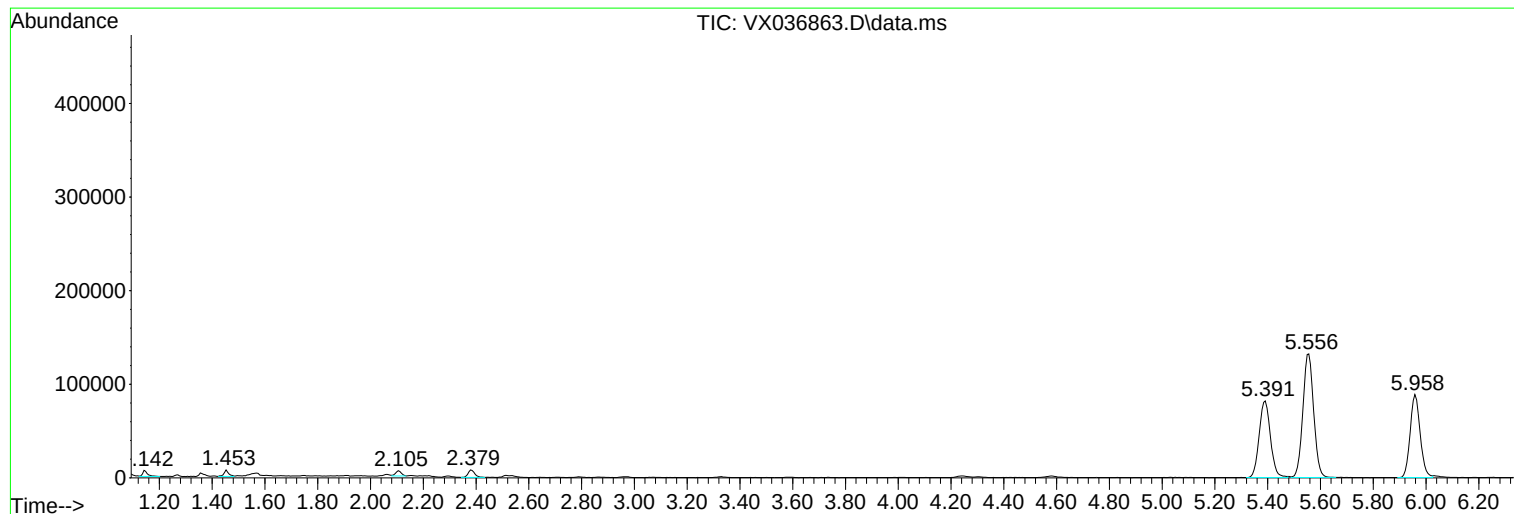

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036863.D
Acq On : 08 Aug 2023 14:51
Operator : JC/MD
Sample : 03903-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-03W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036863.D
Acq On : 08 Aug 2023 14:51
Operator : JC/MD
Sample : 03903-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-03W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------