

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
 Data File : VX036864.D
 Acq On : 08 Aug 2023 15:15
 Operator : JC/MD
 Sample : 03903-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-04W

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260

Signal : TIC: VX036864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	19	rVB	14981	16865	2.24%	0.398%
2	1.355	41	44	50	rBV2	6306	9384	1.24%	0.222%
3	1.569	70	79	82	rBV6	3703	8371	1.11%	0.198%
4	2.379	205	212	223	rVB	6429	11422	1.52%	0.270%
5	5.391	692	706	721	rBV	90175	261015	34.63%	6.165%
6	5.556	722	733	749	rVB	143419	408432	54.19%	9.648%
7	5.958	788	799	815	rBV	93980	251504	33.37%	5.941%
8	6.763	921	931	948	rBV	237691	561391	74.48%	13.261%
9	8.647	1234	1240	1250	rBV	483456	753753	100.00%	17.804%
10	9.275	1337	1343	1350	rBV	10288	14287	1.90%	0.337%
11	9.525	1376	1384	1390	rBV	8584	13627	1.81%	0.322%
12	10.055	1465	1471	1487	rBV	498506	665542	88.30%	15.721%
13	10.860	1597	1603	1609	rBV	6355	8768	1.16%	0.207%
14	11.079	1634	1639	1652	rVB	383073	497767	66.04%	11.758%
15	11.927	1774	1778	1788	rBV	24226	32666	4.33%	0.772%
16	12.024	1788	1794	1802	rVV	454528	583306	77.39%	13.778%
17	12.219	1820	1826	1835	rBV	12860	21684	2.88%	0.512%
18	12.853	1925	1930	1945	rBV	88429	113764	15.09%	2.687%




Sum of corrected areas: 4233548

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036864.D
Acq On : 08 Aug 2023 15:15
Operator : JC/MD
Sample : 03903-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-04W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

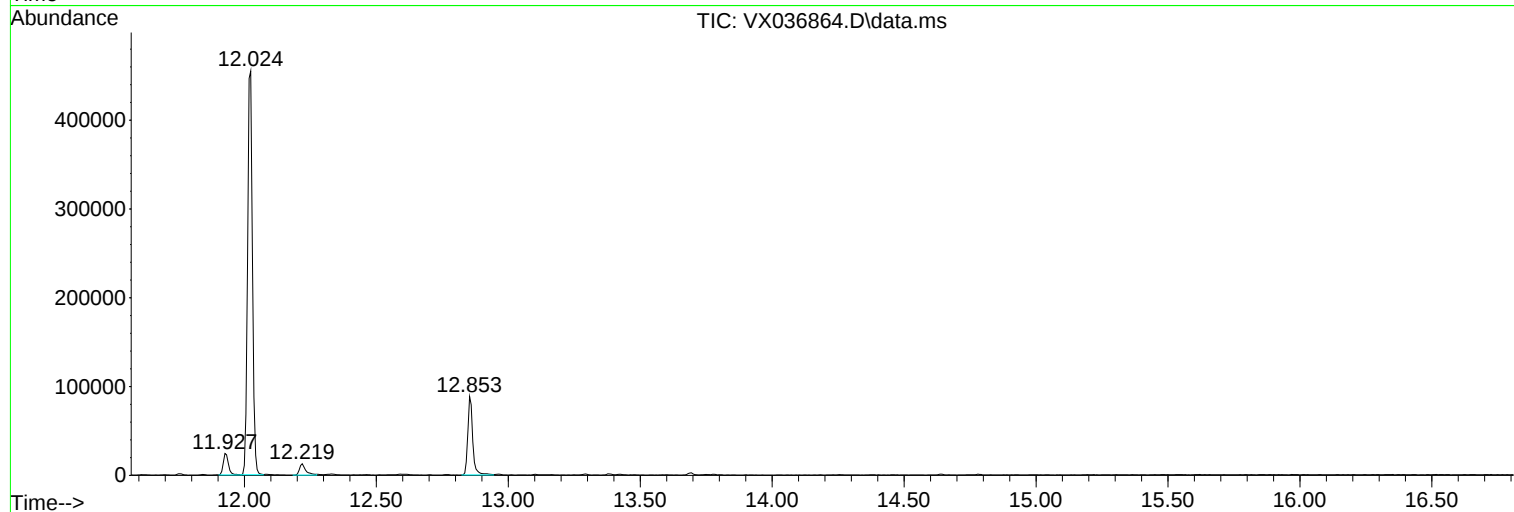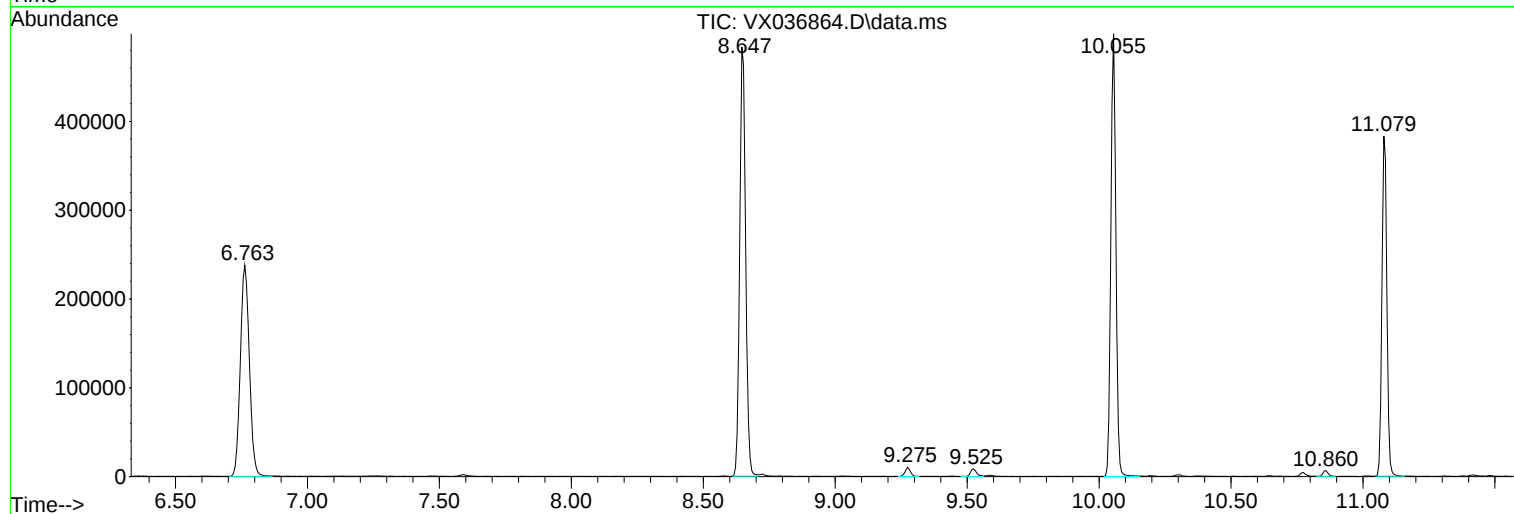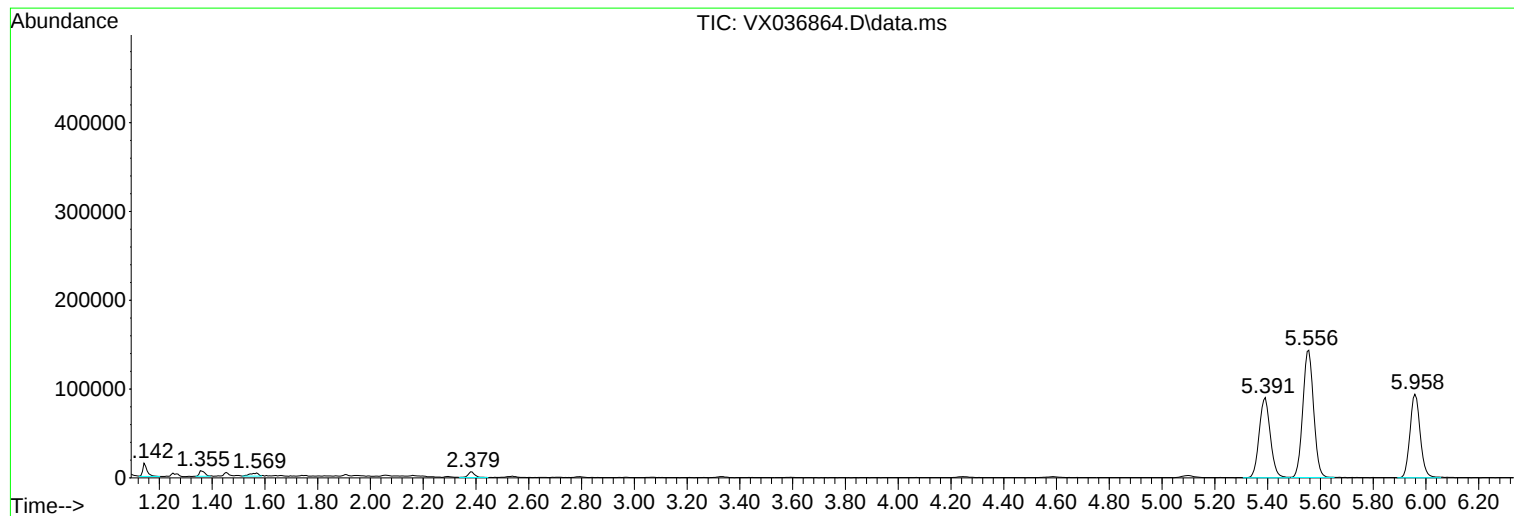

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036864.D
Acq On : 08 Aug 2023 15:15
Operator : JC/MD
Sample : 03903-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-04W










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Nonanal Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.853	9.75 ug/l	113764	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Nonanal	142	C9H18O	000124-19-6	91
2			Cyclohexanol, 2-methyl-, trans-	114	C7H14O	007443-52-9	38
3			Cycloheptane	98	C7H14	000291-64-5	30
4			Heptane, 2-chloro-	134	C7H15Cl	001001-89-4	22
5			2-Heptene, (E)-	98	C7H14	014686-13-6	18

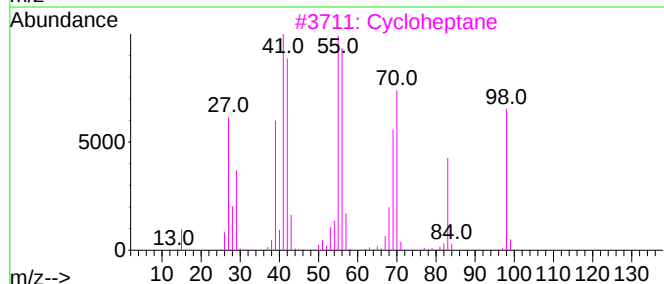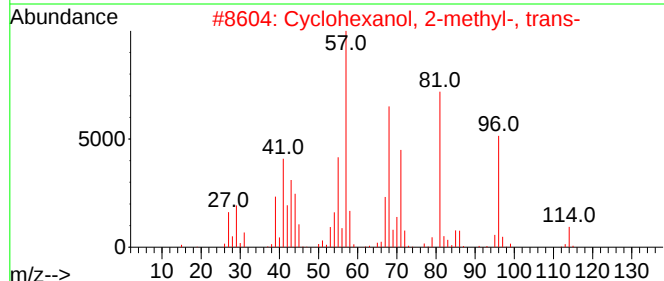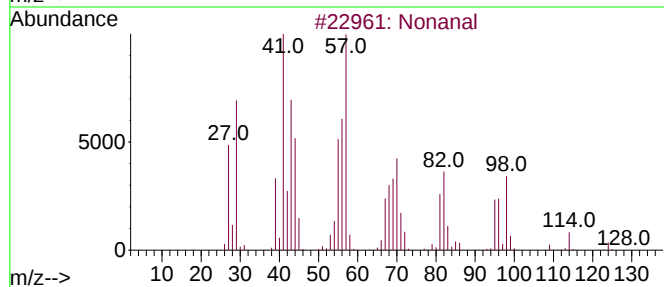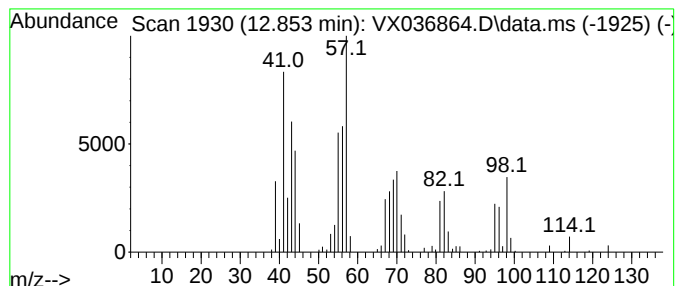

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036864.D
Acq On : 08 Aug 2023 15:15
Operator : JC/MD
Sample : 03903-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-04W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Nonanal	12.853	9.8	ug/l	113764	4	12.024	583306	50.0