

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
 Data File : VX036865.D
 Acq On : 08 Aug 2023 15:39
 Operator : JC/MD
 Sample : 03903-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-05W

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260

Signal : TIC: VX036865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	70	79	84	rBV6	3525	7830	1.05%	0.191%
2	2.379	206	212	221	rBV	6979	11297	1.52%	0.275%
3	4.574	561	572	588	rBV2	4107	14611	1.97%	0.356%
4	5.391	692	706	722	rBV	85018	253371	34.09%	6.173%
5	5.556	722	733	750	rVB	138528	393649	52.96%	9.590%
6	5.958	789	799	812	rBV	91748	243579	32.77%	5.934%
7	6.763	919	931	946	rBV	231375	547383	73.64%	13.336%
8	8.647	1234	1240	1250	rBV	462648	743295	100.00%	18.109%
9	9.275	1337	1343	1350	rVB	43687	63746	8.58%	1.553%
10	10.055	1465	1471	1488	rBV	497374	665822	89.58%	16.221%
11	11.079	1634	1639	1649	rBV	400866	510485	68.68%	12.437%
12	12.024	1788	1794	1803	rBV	478544	610639	82.15%	14.877%
13	12.219	1820	1826	1833	rBV	11889	18574	2.50%	0.453%
14	12.853	1924	1930	1938	rBV	14377	20340	2.74%	0.496%




Sum of corrected areas: 4104621

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036865.D
Acq On : 08 Aug 2023 15:39
Operator : JC/MD
Sample : 03903-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-05W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

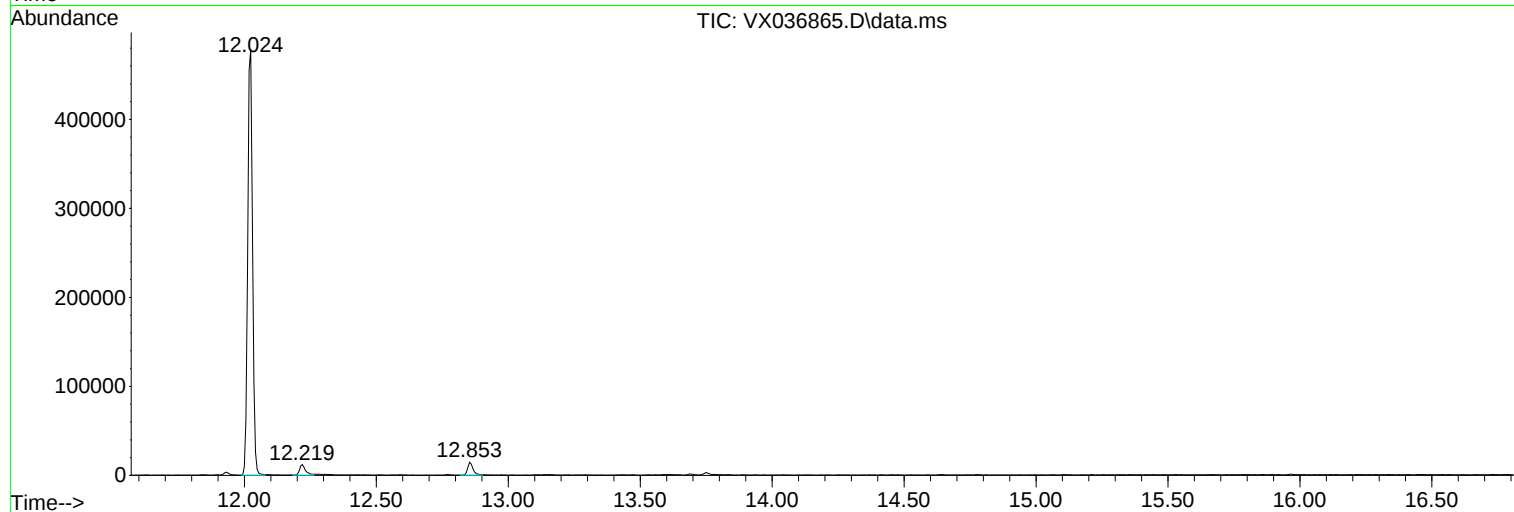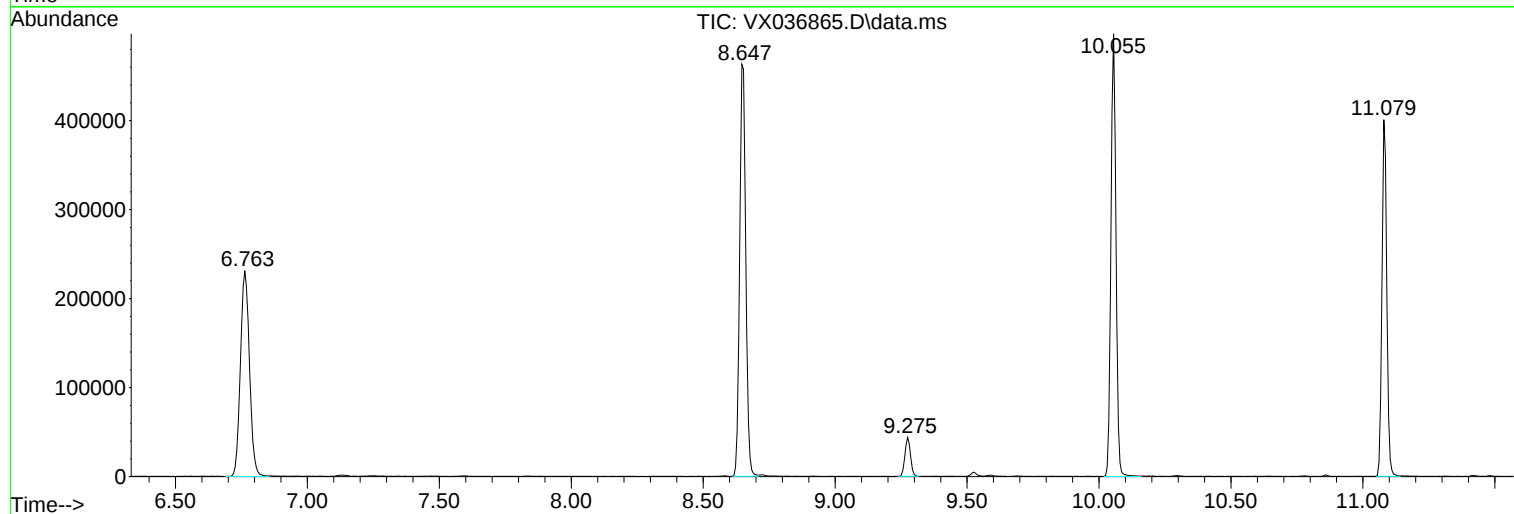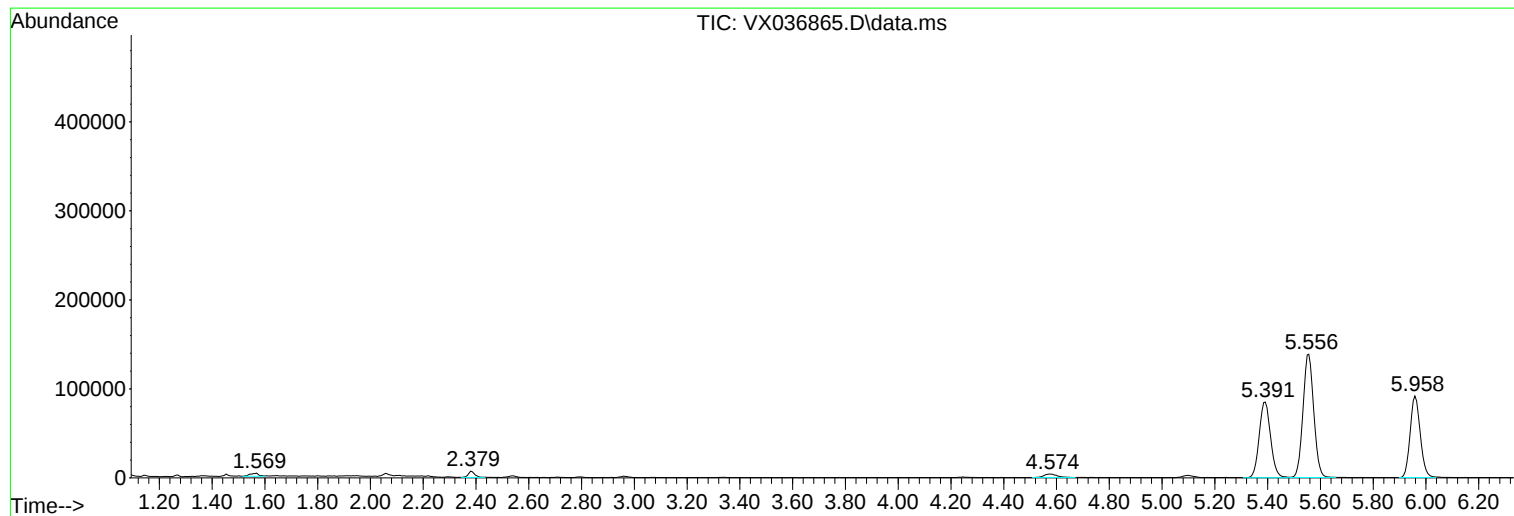

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036865.D
Acq On : 08 Aug 2023 15:39
Operator : JC/MD
Sample : 03903-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-05W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036865.D
Acq On : 08 Aug 2023 15:39
Operator : JC/MD
Sample : 03903-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-05W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------