

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
 Data File : VX036866.D
 Acq On : 08 Aug 2023 16:03
 Operator : JC/MD
 Sample : 03903-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-06W

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260

Signal : TIC: VX036866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	55	60	68	rBV	14821	18750	2.70%	0.488%
2	1.563	70	78	82	rVV5	3209	7286	1.05%	0.190%
3	2.380	207	212	219	rBV	7240	12417	1.79%	0.323%
4	3.331	361	368	379	rVB3	3315	7623	1.10%	0.198%
5	5.099	649	658	667	rVB3	3550	9895	1.42%	0.258%
6	5.391	695	706	722	rBV2	79666	237133	34.14%	6.175%
7	5.556	722	733	751	rVB2	129395	368614	53.07%	9.598%
8	5.958	788	799	817	rBV	87616	230850	33.23%	6.011%
9	6.361	858	865	875	rBV3	4758	13002	1.87%	0.339%
10	6.763	921	931	946	rBV	217974	511900	73.70%	13.329%
11	7.824	1100	1105	1116	rVB3	4561	8469	1.22%	0.221%
12	8.647	1234	1240	1249	rVV	431381	694603	100.00%	18.087%
13	9.275	1337	1343	1349	rBV	7360	9725	1.40%	0.253%
14	9.525	1377	1384	1388	rBV4	7154	11718	1.69%	0.305%
15	10.055	1465	1471	1479	rBV	469027	623932	89.83%	16.247%
16	11.079	1634	1639	1650	rBV	386335	485403	69.88%	12.640%
17	12.018	1788	1793	1802	rBV	452401	589040	84.80%	15.338%




Sum of corrected areas: 3840360

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036866.D
Acq On : 08 Aug 2023 16:03
Operator : JC/MD
Sample : 03903-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

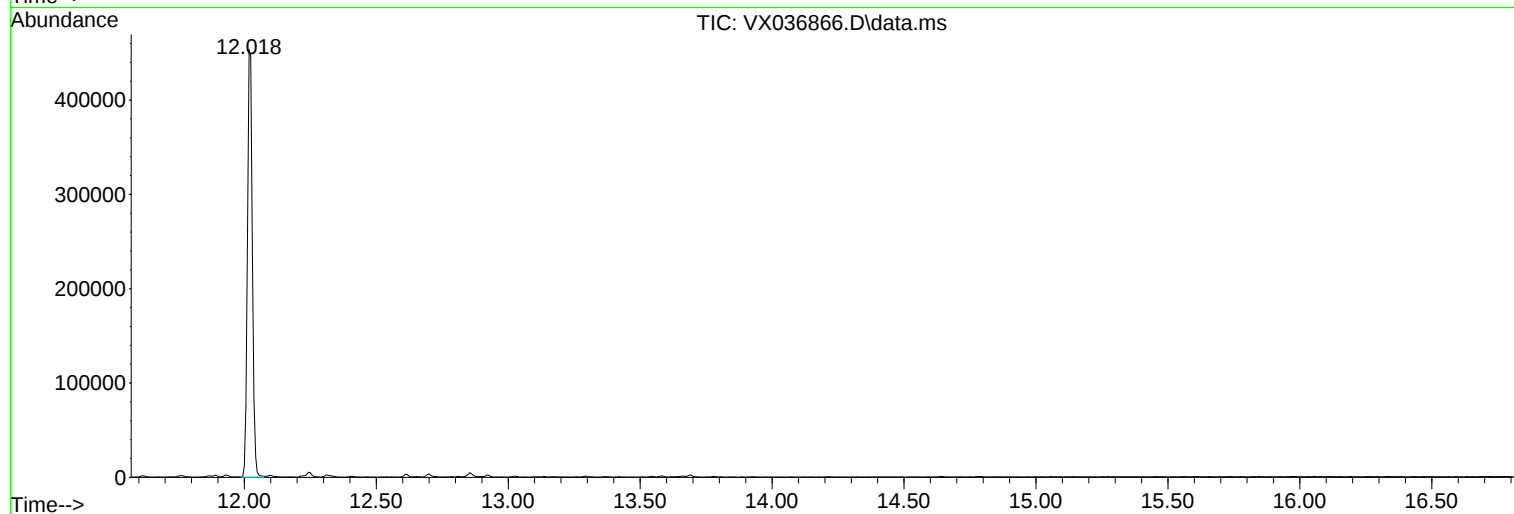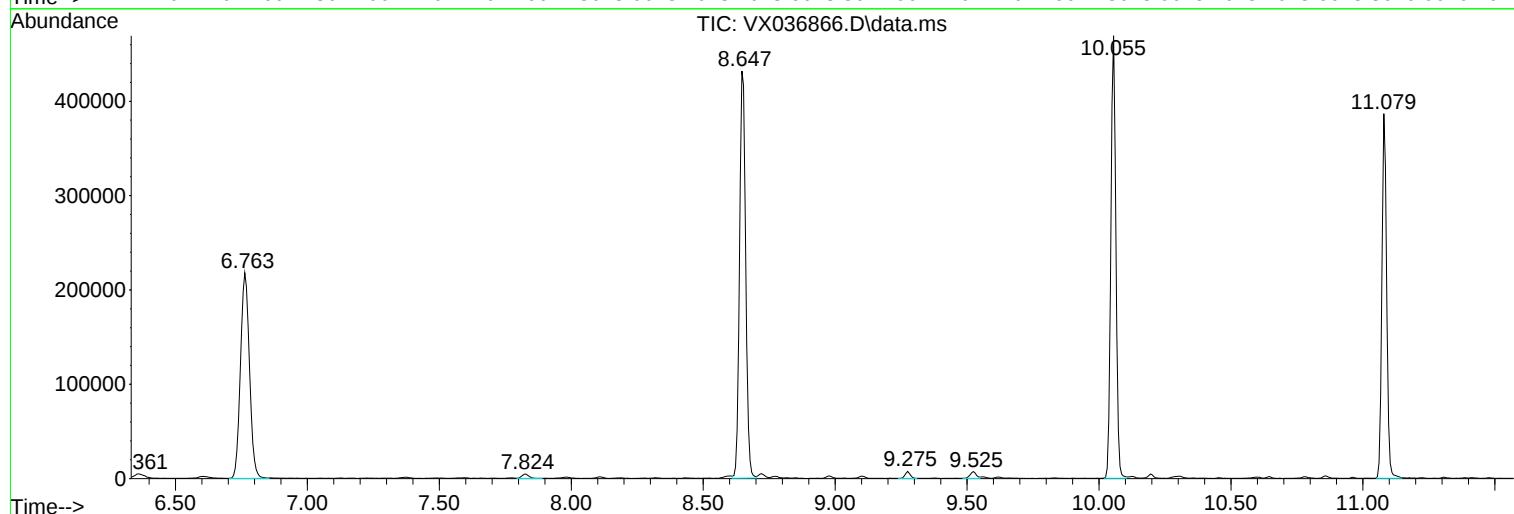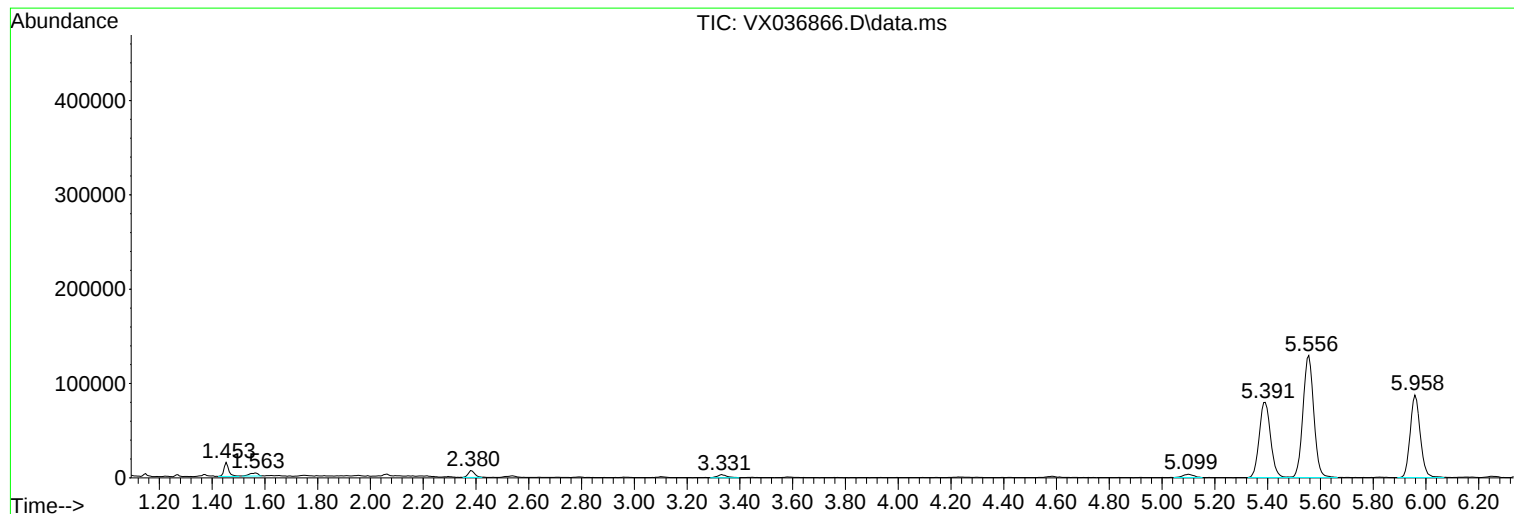

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036866.D
Acq On : 08 Aug 2023 16:03
Operator : JC/MD
Sample : 03903-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080823\
Data File : VX036866.D
Acq On : 08 Aug 2023 16:03
Operator : JC/MD
Sample : 03903-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06W

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------