



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082224\
Data File : VX043083.D
Acq On : 22 Aug 2024 11:44
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082224W.M
Title : SW846 8260
Last Update : Fri Aug 23 08:42:59 2024

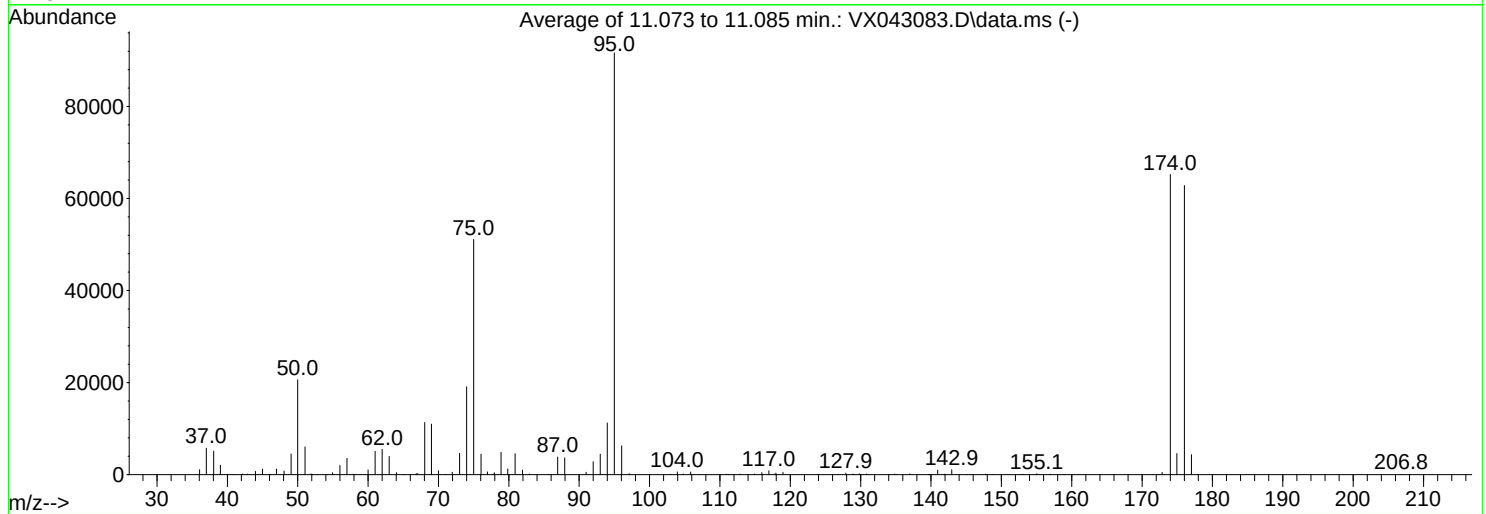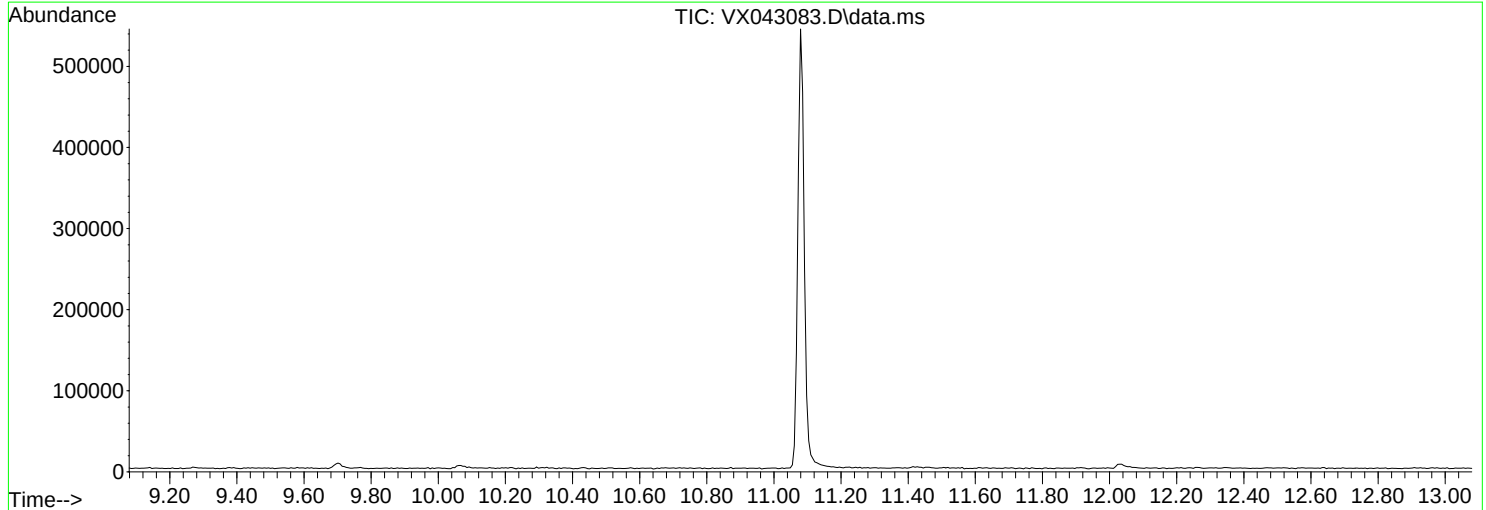

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	20608	PASS
75	95	30	60	55.8	51107	PASS
95	95	100	100	100.0	91651	PASS
96	95	5	9	6.8	6258	PASS
173	174	0.00	2	0.7	488	PASS
174	95	50	100	71.2	65221	PASS
175	174	5	9	7.0	4583	PASS
176	174	95	101	96.3	62821	PASS
177	176	5	9	6.9	4348	PASS