

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
 Data File : VX030727.D
 Acq On : 23 Aug 2022 13:21
 Operator : JC/MD
 Sample : N4245-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW17811-20220816

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
 Title : SW846 8260

Signal : TIC: VX030727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	548	559	571	rBV	196222	532238	7.41%	3.766%
2	5.391	692	706	721	rBV2	156204	450983	6.28%	3.191%
3	5.556	722	733	750	rVB	140398	404665	5.63%	2.863%
4	5.964	789	800	813	rBV	166377	440550	6.13%	3.117%
5	6.769	921	932	943	rBV	288589	676641	9.42%	4.788%
6	7.128	981	991	1012	rBV	3293807	7182069	100.00%	50.818%
7	7.433	1033	1041	1054	rVB	189823	397380	5.53%	2.812%
8	8.652	1232	1241	1257	rBV	866568	1324176	18.44%	9.369%
9	9.274	1335	1343	1354	rBV	332623	490397	6.83%	3.470%
10	10.055	1465	1471	1479	rBV	560344	779084	10.85%	5.513%
11	11.085	1634	1640	1648	rBV	613161	776355	10.81%	5.493%
12	12.024	1789	1794	1808	rVB	573817	678449	9.45%	4.800%




Sum of corrected areas: 14132987

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030727.D
Acq On : 23 Aug 2022 13:21
Operator : JC/MD
Sample : N4245-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

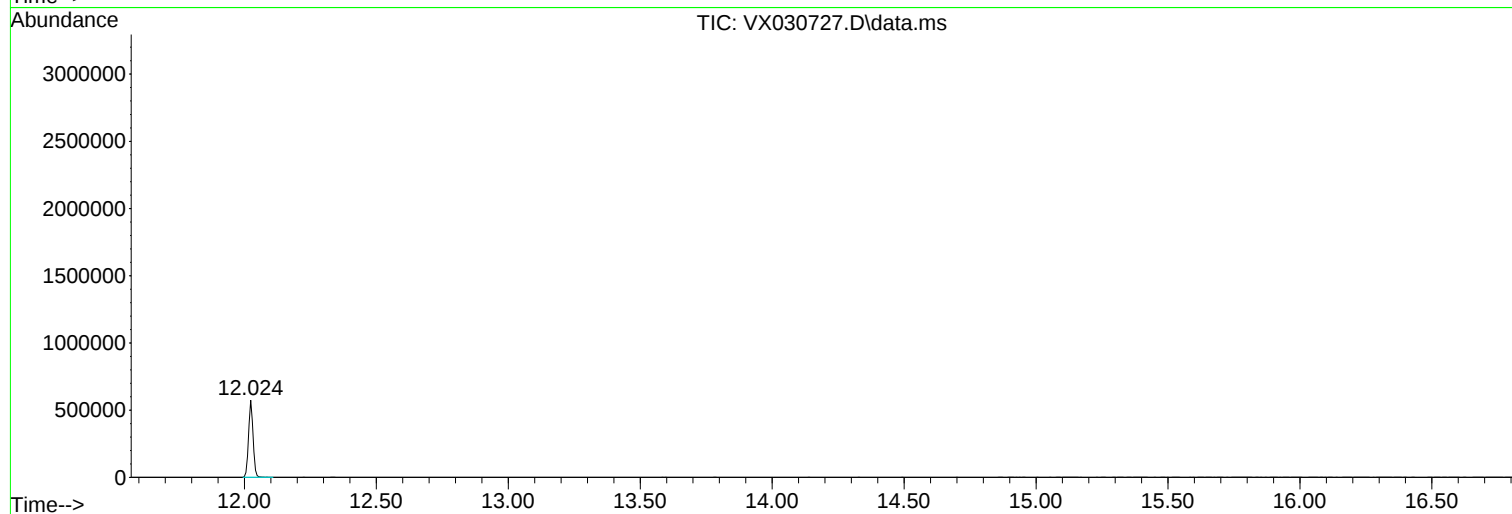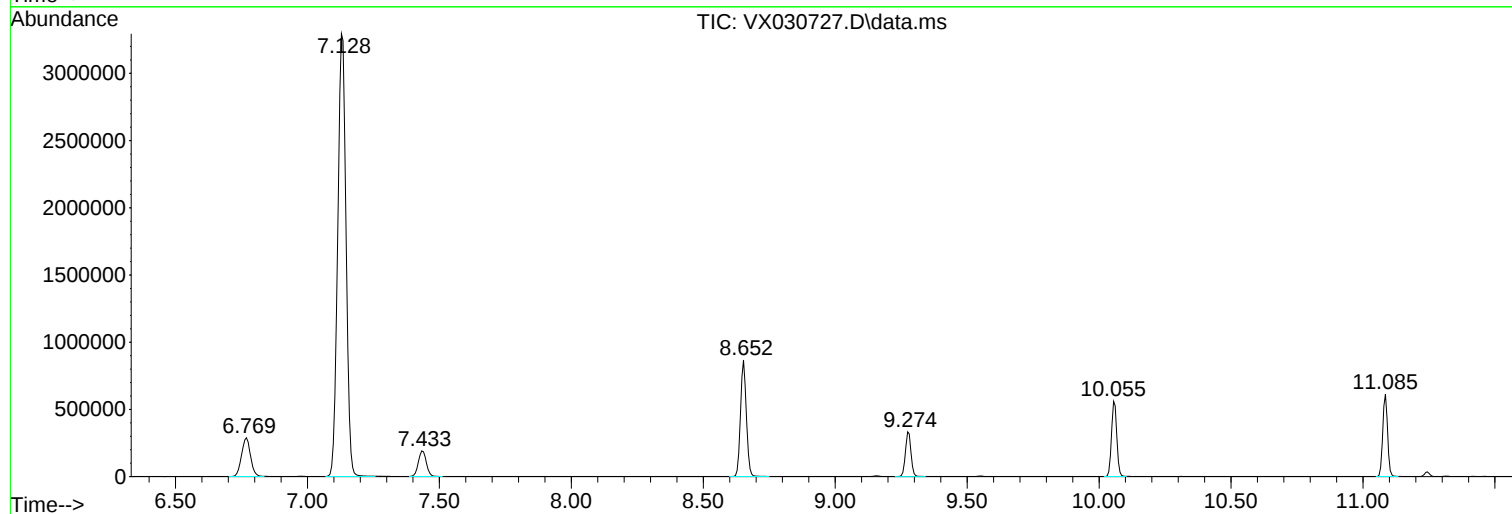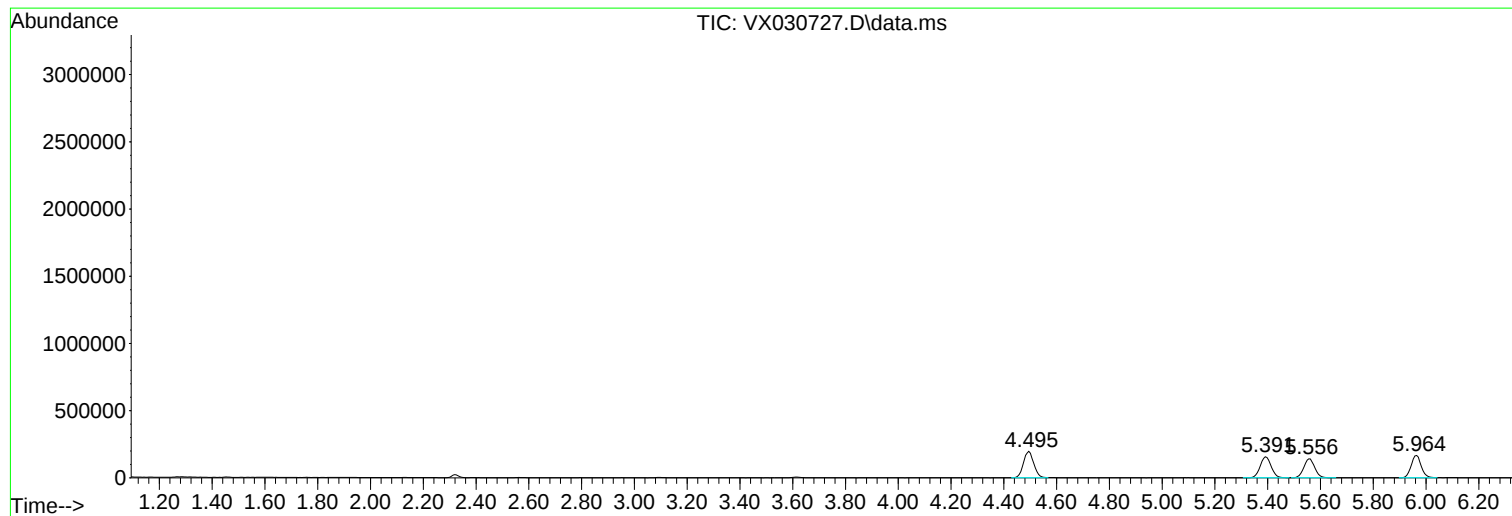

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030727.D
Acq On : 23 Aug 2022 13:21
Operator : JC/MD
Sample : N4245-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178I1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030727.D
Acq On : 23 Aug 2022 13:21
Operator : JC/MD
Sample : N4245-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178I1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------