

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030729.D
Acq On : 23 Aug 2022 14:08
Operator : JC/MD
Sample : N4245-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	547	559	574	rBV	126564	341859	9.21%	3.476%
2	5.391	694	706	721	rBV	155191	452747	12.20%	4.604%
3	5.562	723	734	747	rVB2	138608	396095	10.68%	4.028%
4	5.964	789	800	817	rBV2	164107	430884	11.61%	4.381%
5	6.769	920	932	944	rBV	272484	650525	17.53%	6.615%
6	7.129	981	991	1008	rBV	1720112	3710003	100.00%	37.724%
7	8.653	1234	1241	1251	rBV	858247	1295769	34.93%	13.175%
8	9.275	1336	1343	1352	rBV	265469	390781	10.53%	3.973%
9	10.055	1465	1471	1485	rBV	557506	762272	20.55%	7.751%
10	11.085	1634	1640	1648	rBV	618092	768248	20.71%	7.812%
11	12.024	1788	1794	1806	rBV	522040	635518	17.13%	6.462%




Sum of corrected areas: 9834701

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030729.D
Acq On : 23 Aug 2022 14:08
Operator : JC/MD
Sample : N4245-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

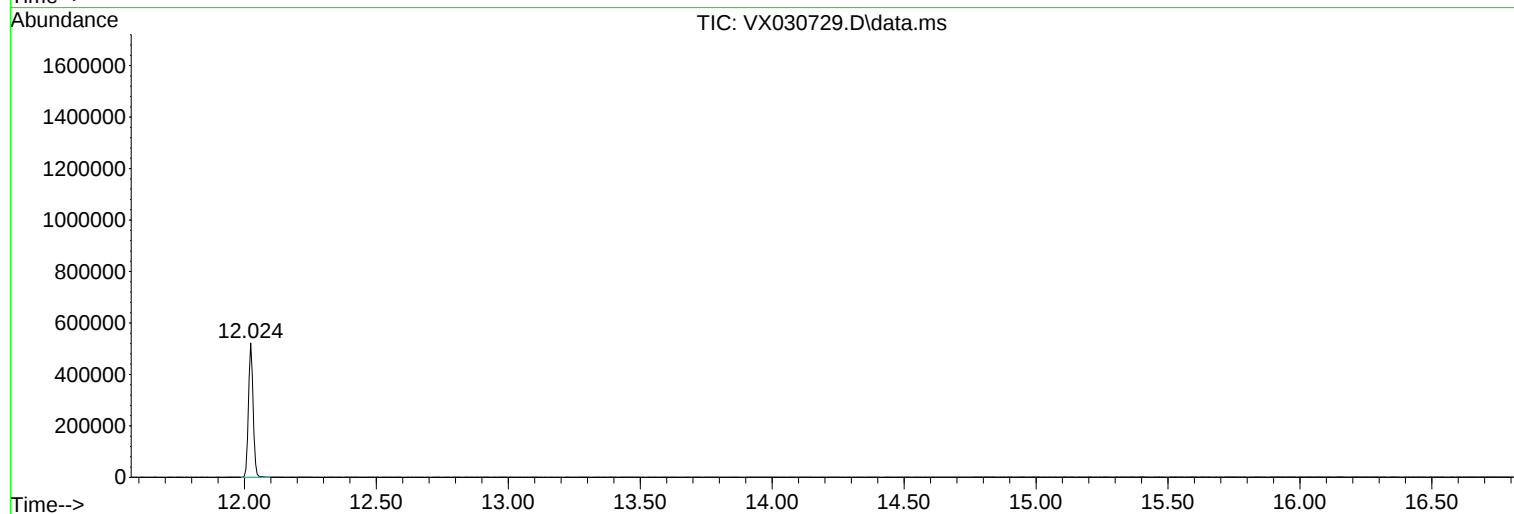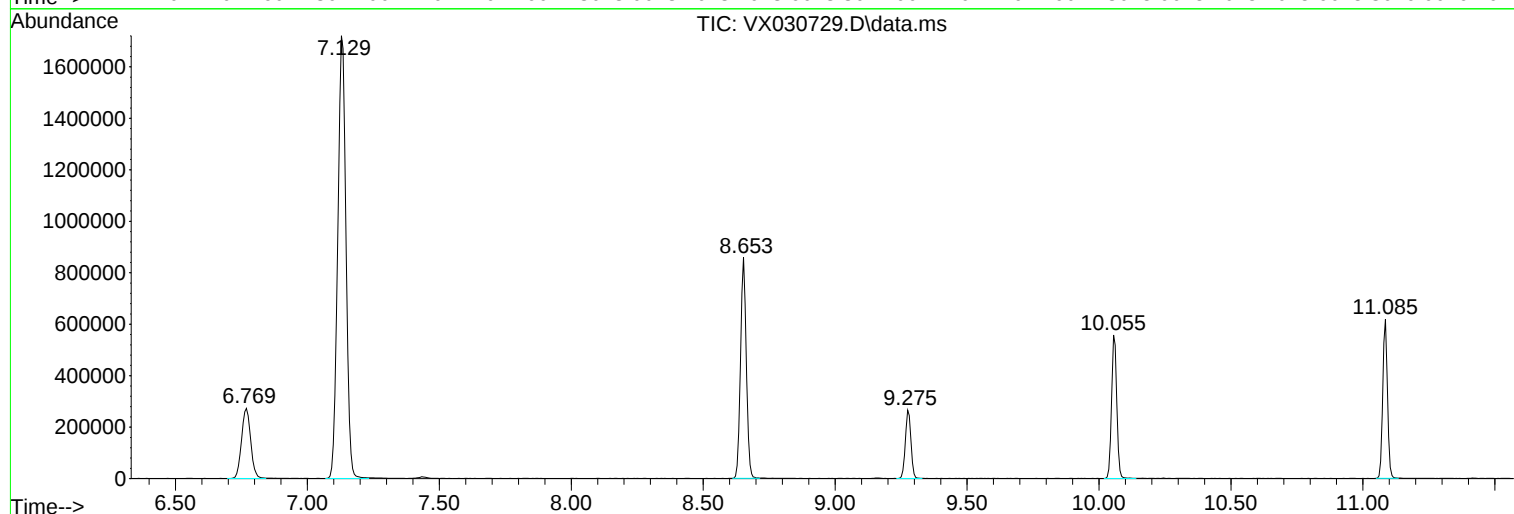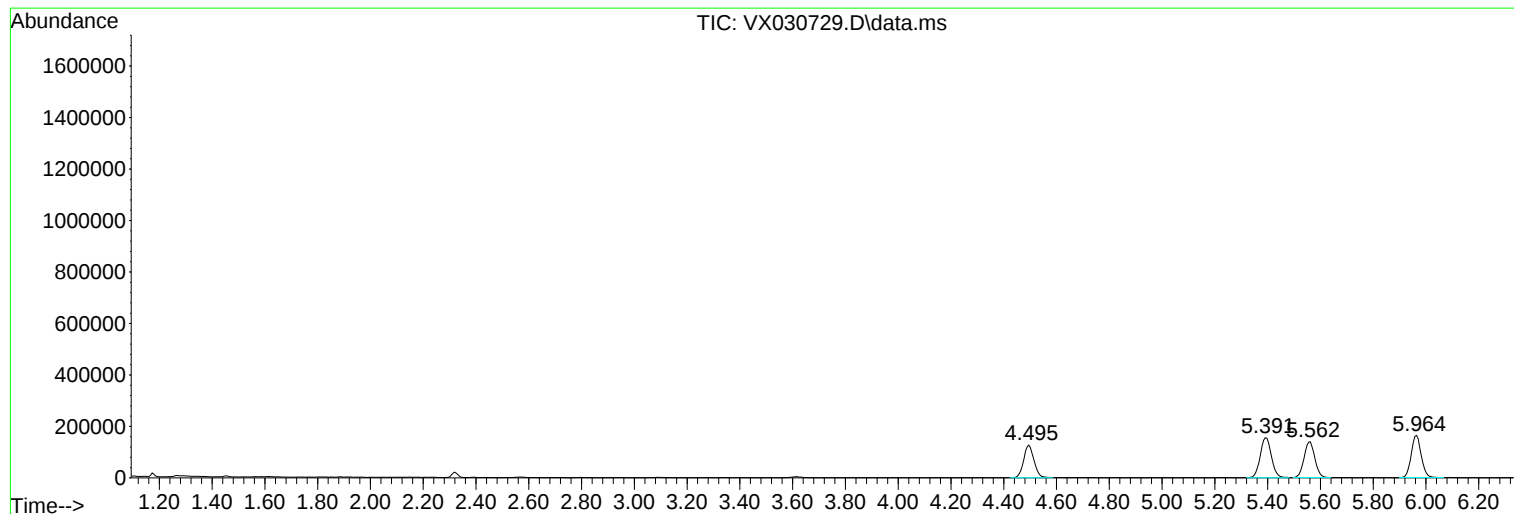

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030729.D
Acq On : 23 Aug 2022 14:08
Operator : JC/MD
Sample : N4245-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030729.D
Acq On : 23 Aug 2022 14:08
Operator : JC/MD
Sample : N4245-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc