

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
 Data File : VX030734.D
 Acq On : 23 Aug 2022 16:05
 Operator : JC/MD
 Sample : N4245-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW179D1-20220816

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
 Title : SW846 8260

Signal : TIC: VX030734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	25	29	37	rBV3	7860	16860	1.10%	0.232%
2	4.495	548	559	572	rBV2	52240	144660	9.48%	1.987%
3	5.391	694	706	723	rBV	155871	451590	29.60%	6.203%
4	5.556	723	733	747	rVV	135898	385206	25.24%	5.291%
5	5.964	788	800	814	rBV2	164545	435239	28.52%	5.978%
6	6.769	920	932	946	rBV	271063	645571	42.31%	8.868%
7	7.129	982	991	1006	rBV	714059	1525890	100.00%	20.960%
8	8.653	1233	1241	1251	rBV	845221	1300712	85.24%	17.867%
9	9.275	1336	1343	1353	rBV	144068	210254	13.78%	2.888%
10	10.055	1466	1471	1482	rBV	540539	741839	48.62%	10.190%
11	11.085	1634	1640	1652	rBV	601410	766284	50.22%	10.526%
12	12.024	1787	1794	1803	rBV	533047	655966	42.99%	9.010%




Sum of corrected areas: 7280071

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030734.D
Acq On : 23 Aug 2022 16:05
Operator : JC/MD
Sample : N4245-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

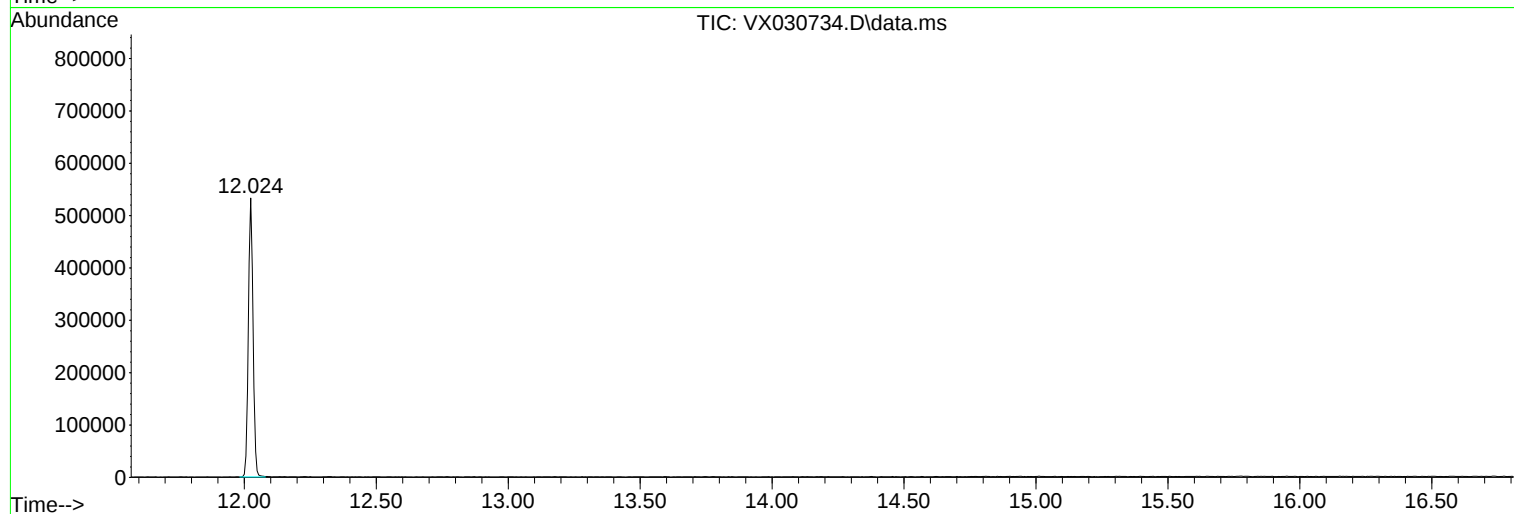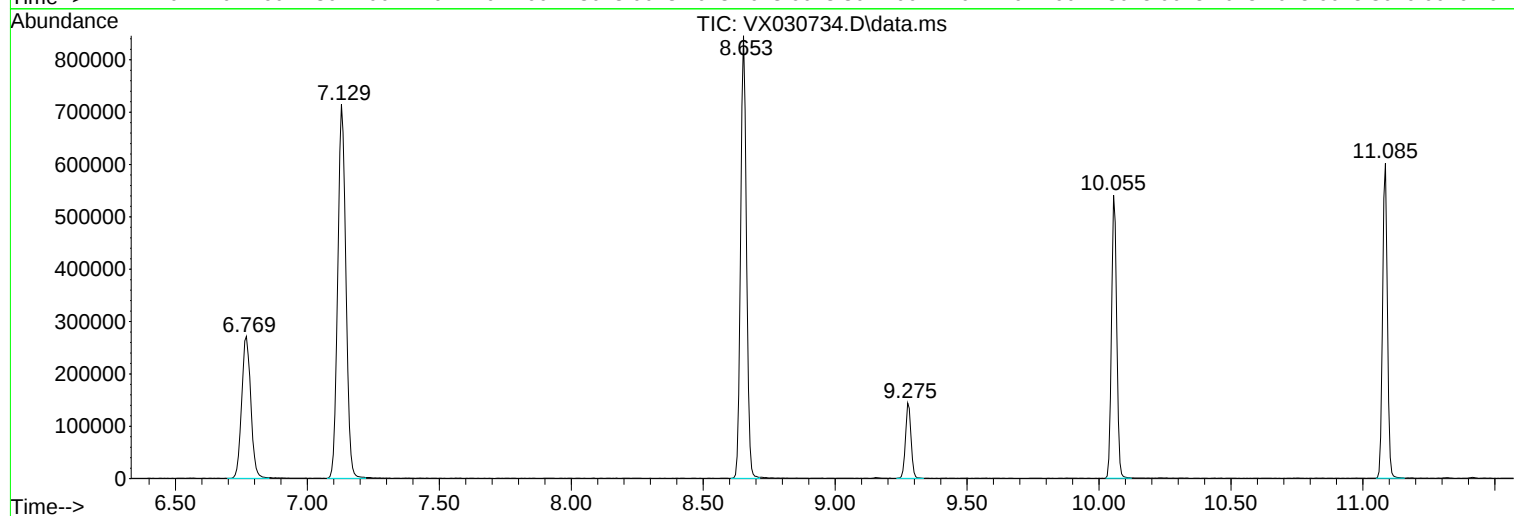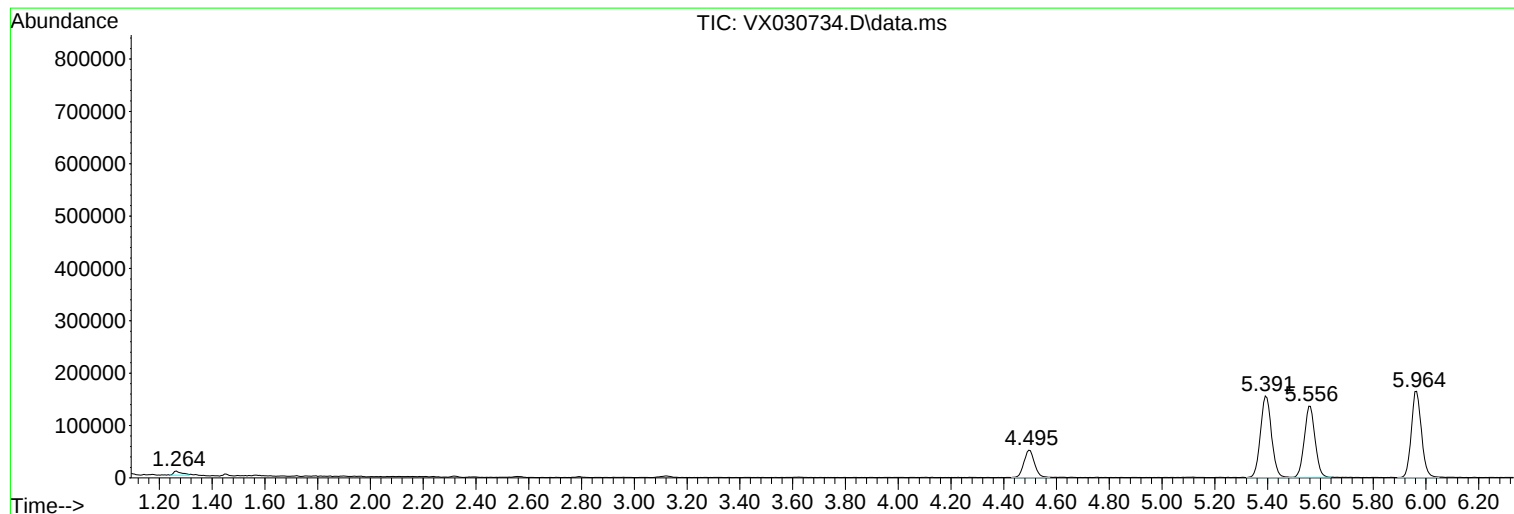

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030734.D
Acq On : 23 Aug 2022 16:05
Operator : JC/MD
Sample : N4245-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030734.D
Acq On : 23 Aug 2022 16:05
Operator : JC/MD
Sample : N4245-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc