

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
 Data File : VX030737.D
 Acq On : 23 Aug 2022 17:15
 Operator : JC/MD
 Sample : N4245-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RW8-MW01D1-20220816

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
 Title : SW846 8260

Signal : TIC: VX030737.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	23	29	41	rBV3	11904	30048	2.25%	0.553%
2	5.019	637	645	658	rBV3	15964	49867	3.73%	0.917%
3	5.391	693	706	722	rBV	158641	462611	34.60%	8.508%
4	5.562	722	734	746	rVV	131351	373844	27.96%	6.875%
5	5.964	789	800	816	rBV2	171095	443814	33.19%	8.162%
6	6.769	922	932	942	rBV	255364	612370	45.80%	11.262%
7	8.653	1234	1241	1250	rBV	865797	1337066	100.00%	24.589%
8	10.055	1465	1471	1479	rBV	543352	728293	54.47%	13.394%
9	11.085	1634	1640	1651	rBV	617748	780011	58.34%	14.345%
10	12.024	1789	1794	1804	rBV	494683	603919	45.17%	11.106%
11	12.225	1819	1827	1836	rBV4	8456	15723	1.18%	0.289%




Sum of corrected areas: 5437566

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030737.D
Acq On : 23 Aug 2022 17:15
Operator : JC/MD
Sample : N4245-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01D1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

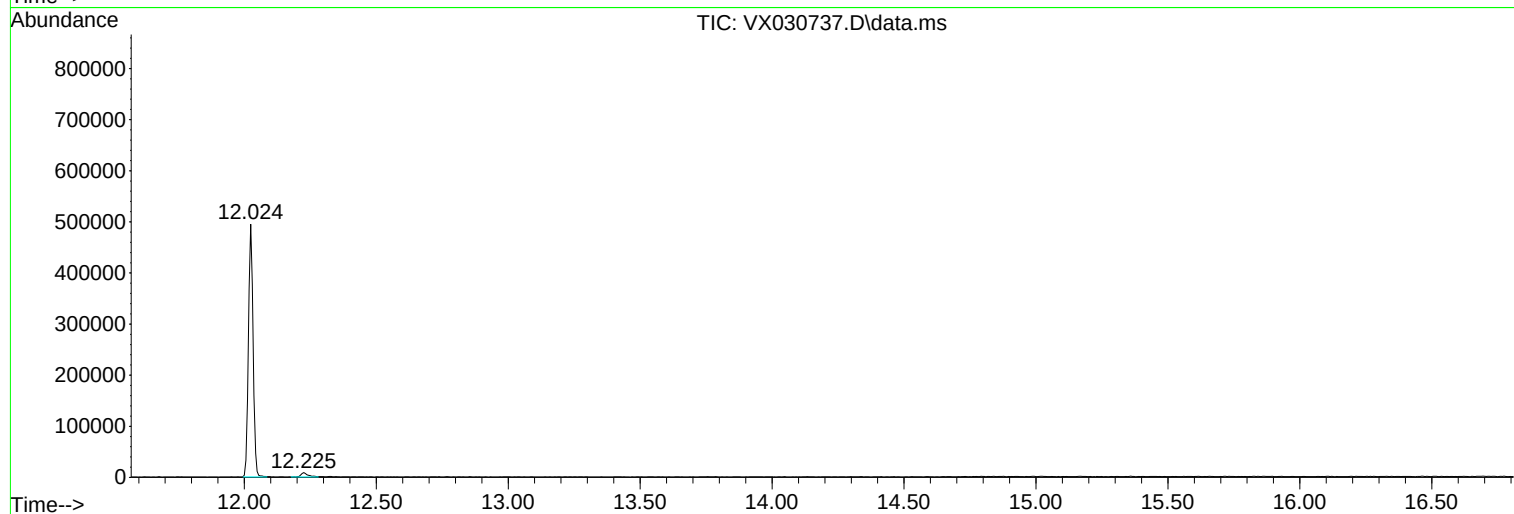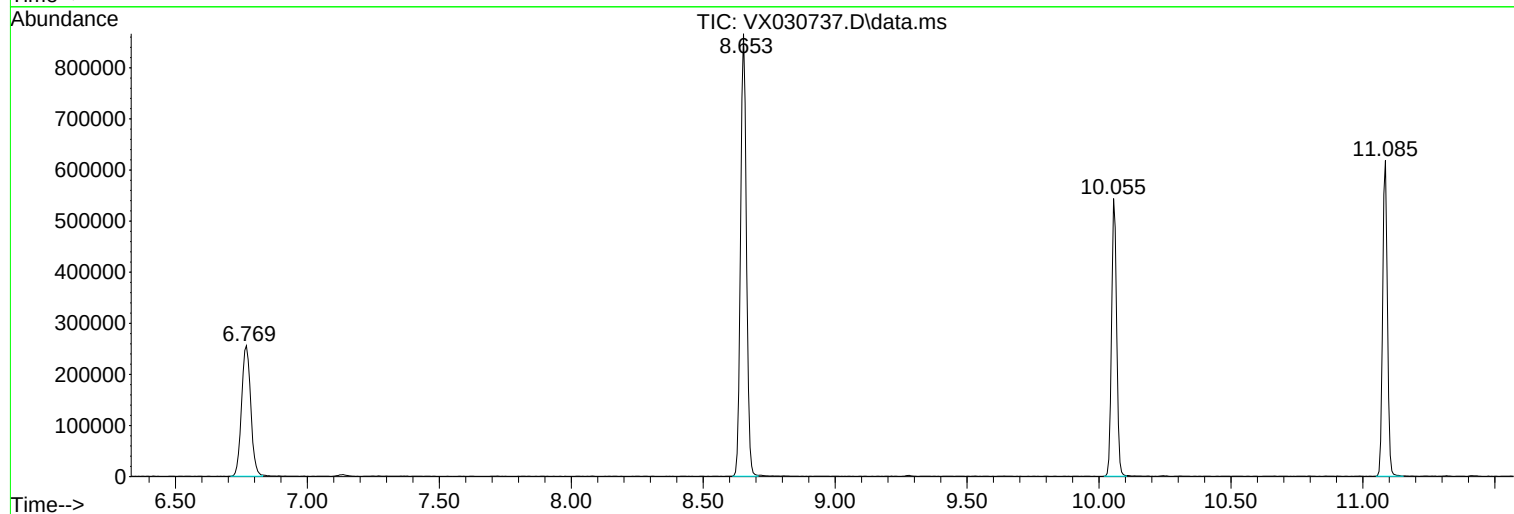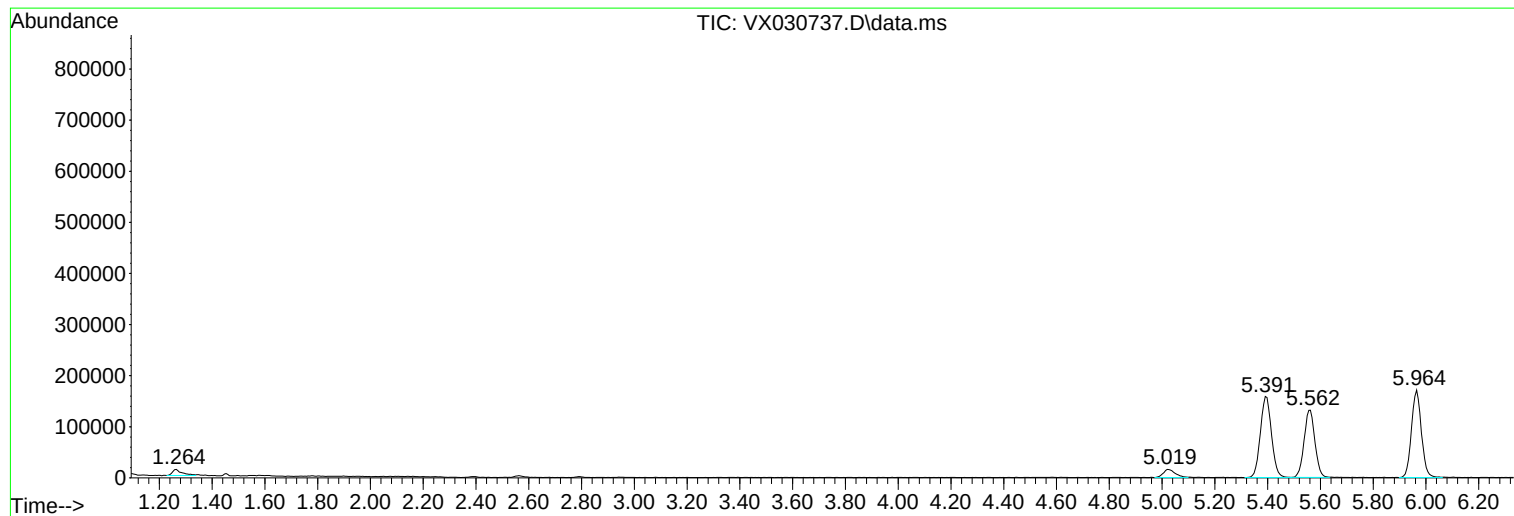

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030737.D
Acq On : 23 Aug 2022 17:15
Operator : JC/MD
Sample : N4245-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01D1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030737.D
Acq On : 23 Aug 2022 17:15
Operator : JC/MD
Sample : N4245-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01D1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------