

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
 Data File : VX030740.D
 Acq On : 23 Aug 2022 18:25
 Operator : JC/MD
 Sample : N4245-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP04-20220816

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	25	29	35	rBV2	11900	22649	1.64%	0.337%
2	2.318	197	202	209	rVB3	12166	23616	1.71%	0.352%
3	5.391	695	706	721	rBV	155485	448415	32.39%	6.680%
4	5.555	721	733	745	rVV2	129746	371467	26.83%	5.533%
5	5.964	789	800	814	rBV2	160951	428123	30.92%	6.377%
6	6.769	922	932	946	rBV	260307	618412	44.66%	9.212%
7	7.128	981	991	1007	rBV2	649717	1384623	100.00%	20.626%
8	8.652	1234	1241	1252	rBV	832640	1296619	93.64%	19.315%
9	10.055	1465	1471	1485	rBV	520096	721851	52.13%	10.753%
10	11.085	1634	1640	1653	rBV	603673	769509	55.58%	11.463%
11	12.024	1789	1794	1806	rVB	521409	627859	45.35%	9.353%




Sum of corrected areas: 6713143

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030740.D
Acq On : 23 Aug 2022 18:25
Operator : JC/MD
Sample : N4245-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

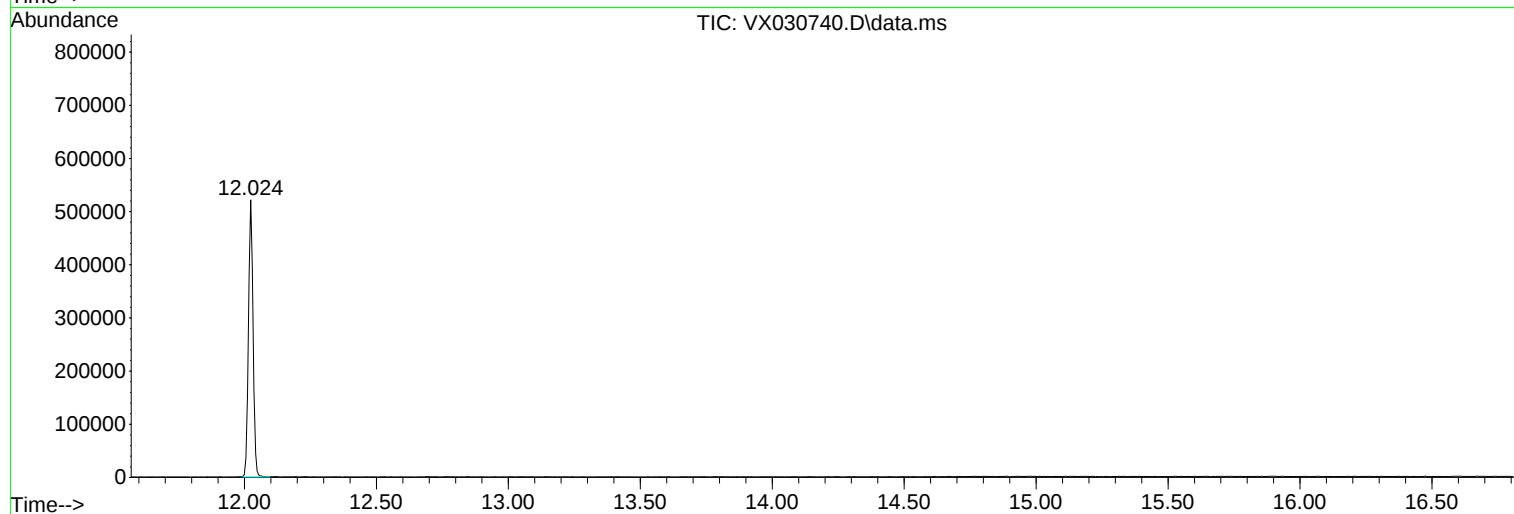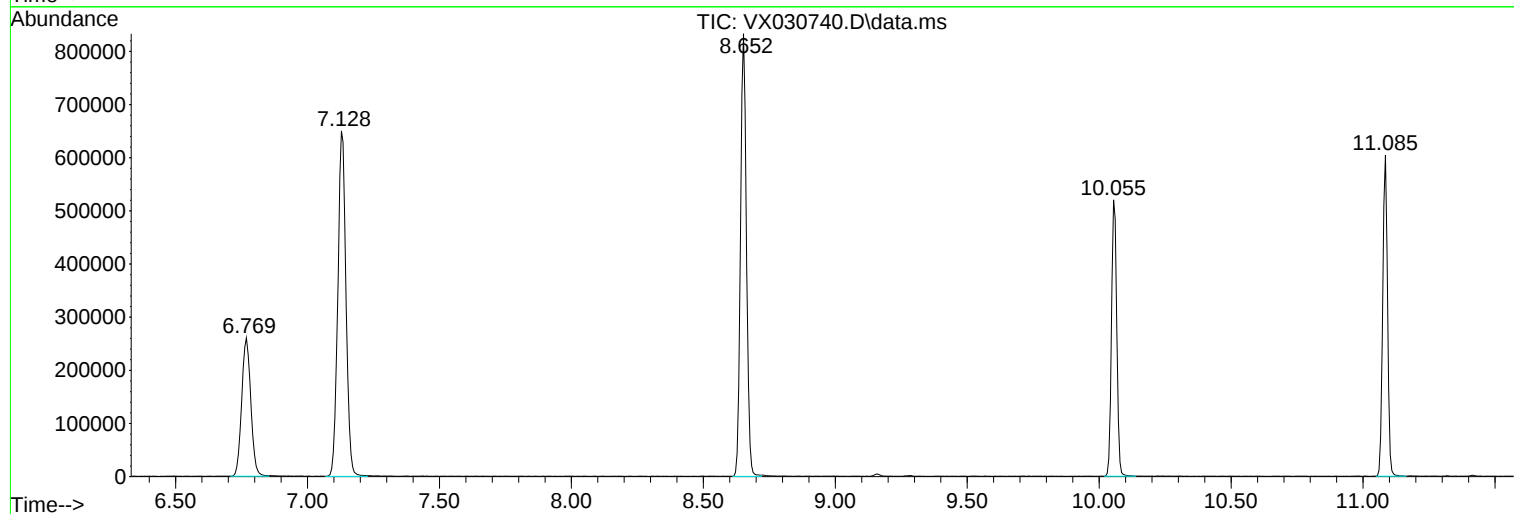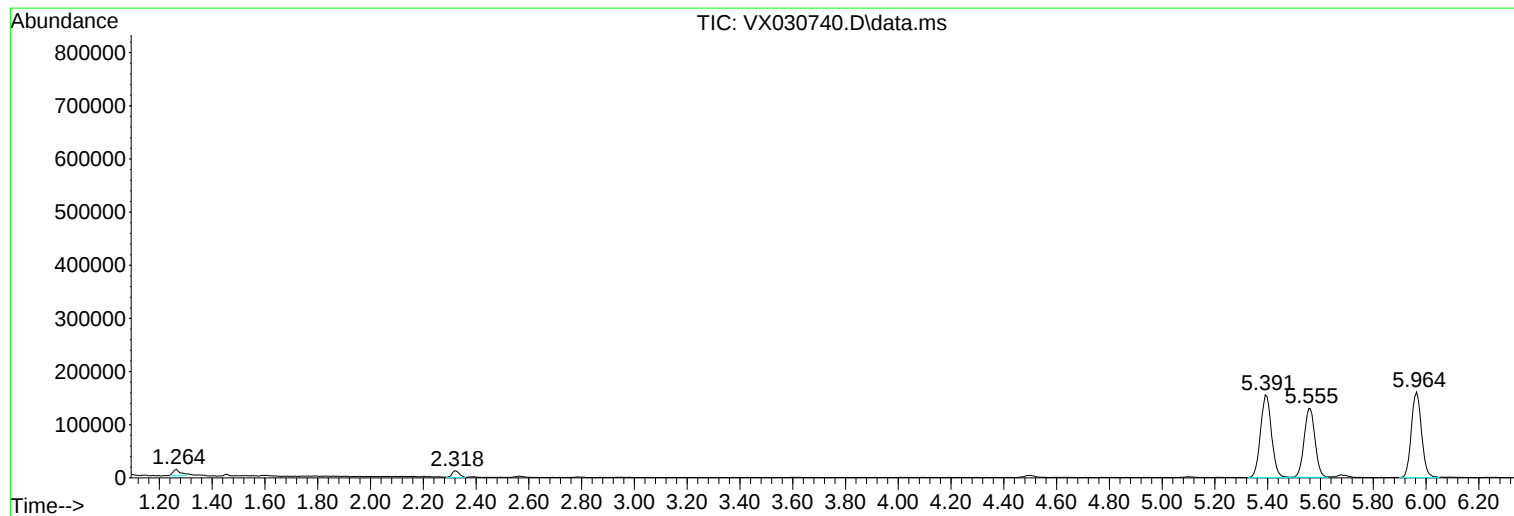

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030740.D
Acq On : 23 Aug 2022 18:25
Operator : JC/MD
Sample : N4245-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030740.D
Acq On : 23 Aug 2022 18:25
Operator : JC/MD
Sample : N4245-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------