

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
 Data File : VX030741.D
 Acq On : 23 Aug 2022 18:49
 Operator : JC/MD
 Sample : N4245-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE126D1-20220817

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	24	29	36	rBV3	12214	27821	2.14%	0.487%
2	5.391	693	706	723	rBV2	157461	451789	34.69%	7.915%
3	5.562	723	734	747	rVB	129826	371443	28.52%	6.507%
4	5.964	789	800	815	rBV2	162195	431465	33.13%	7.559%
5	6.769	922	932	944	rBV	257721	623988	47.91%	10.932%
6	7.129	983	991	1006	rBV	159651	334417	25.68%	5.859%
7	8.653	1234	1241	1251	rBV	845393	1302408	100.00%	22.818%
8	9.275	1339	1343	1350	rBV	10774	15597	1.20%	0.273%
9	10.055	1465	1471	1483	rBV	530098	730838	56.11%	12.804%
10	11.085	1634	1640	1654	rBV	608724	782362	60.07%	13.707%
11	12.024	1789	1794	1804	rBV	519793	635797	48.82%	11.139%




Sum of corrected areas: 5707925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030741.D
Acq On : 23 Aug 2022 18:49
Operator : JC/MD
Sample : N4245-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE126D1-20220817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

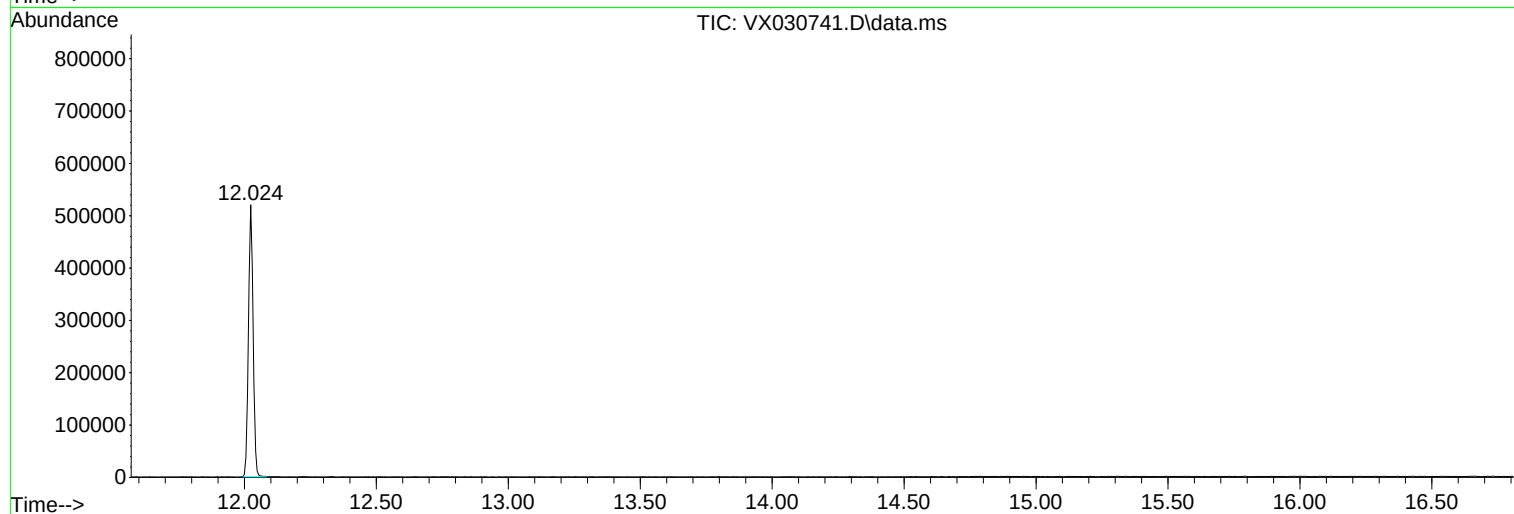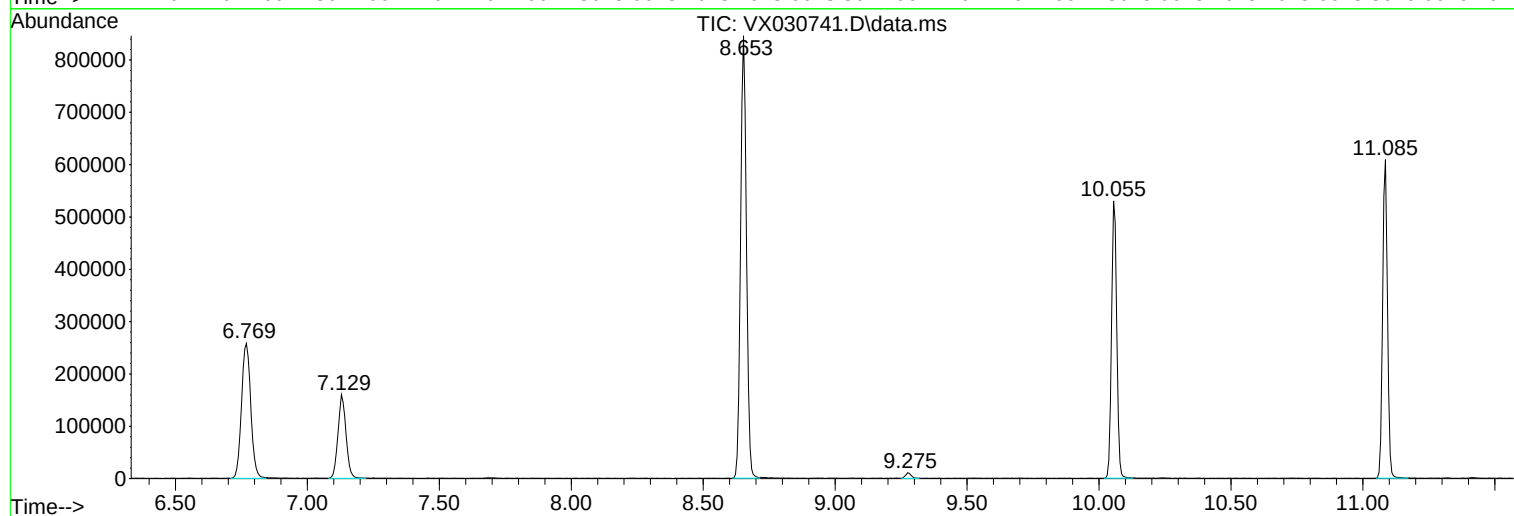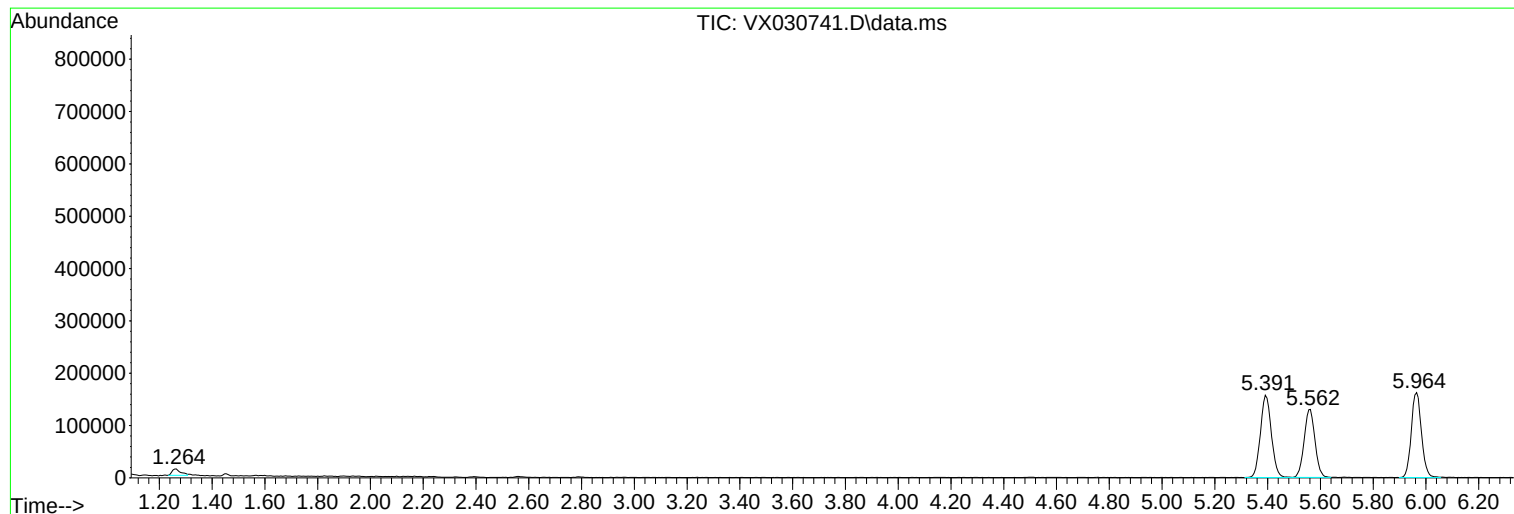

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030741.D
Acq On : 23 Aug 2022 18:49
Operator : JC/MD
Sample : N4245-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE126D1-20220817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082322\
Data File : VX030741.D
Acq On : 23 Aug 2022 18:49
Operator : JC/MD
Sample : N4245-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE126D1-20220817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------