
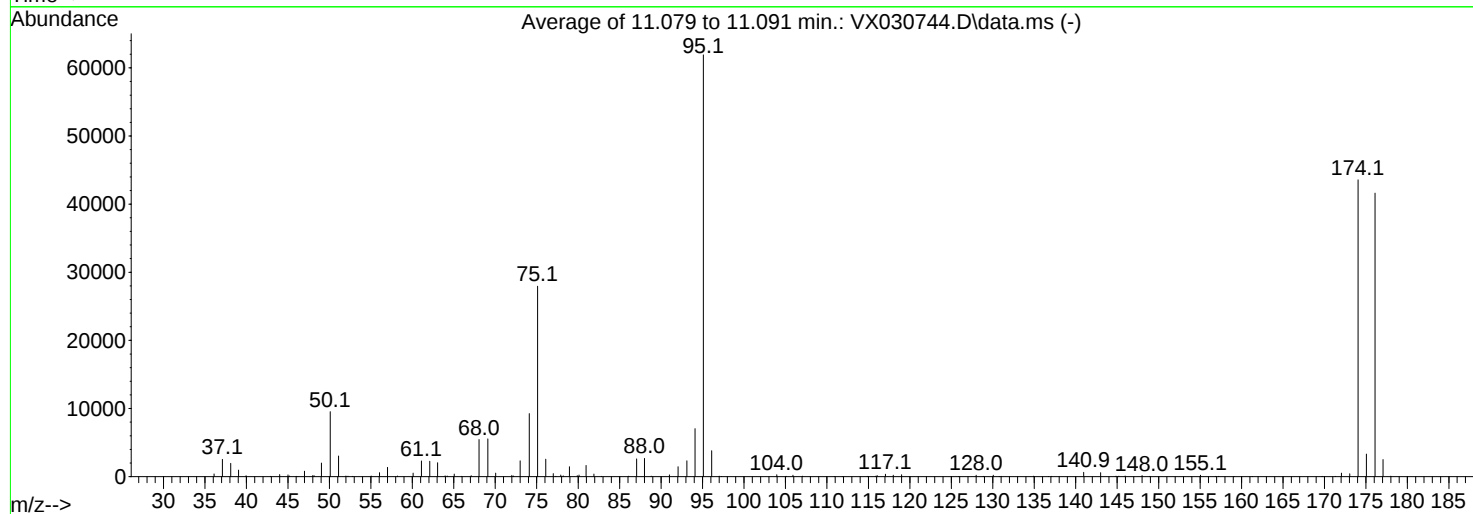


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082322\  
Data File : VX030744.D  
Acq On : 23 Aug 2022 20:23  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072522W.M  
Title : SW846 8260  
Last Update : Mon Jul 25 16:49:17 2022

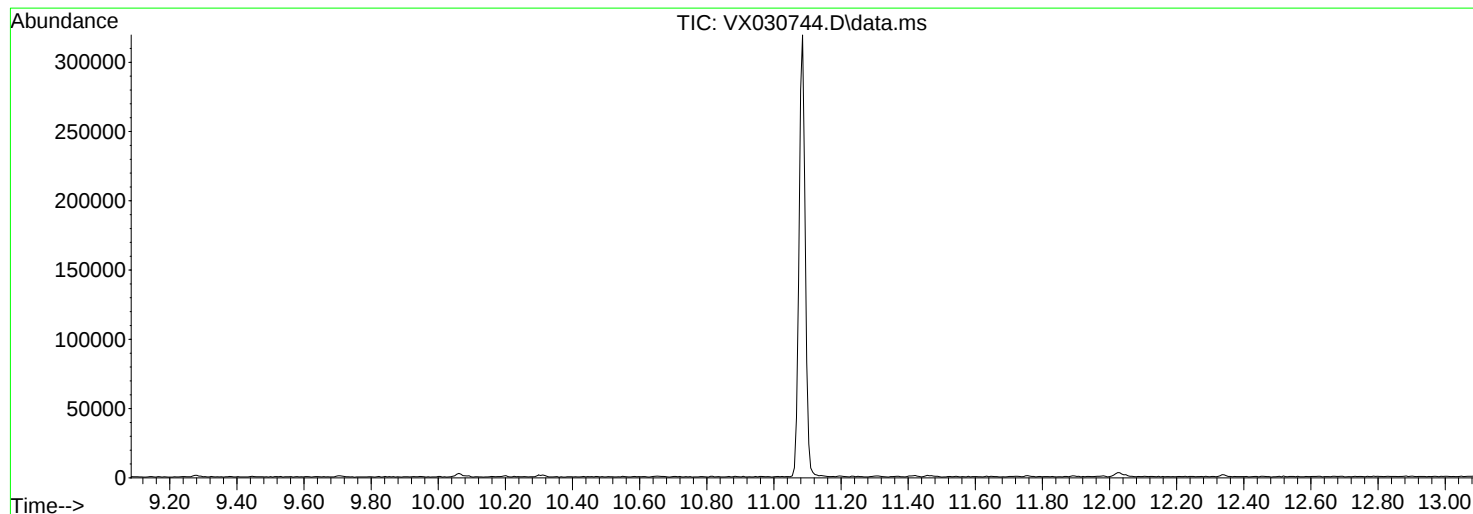

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 15.4  | 9539  | PASS      |
| 75     | 95      | 30     | 60     | 45.2  | 27957 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 61912 | PASS      |
| 96     | 95      | 5      | 9      | 6.1   | 3800  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.0   | 424   | PASS      |
| 174    | 95      | 50     | 100    | 70.4  | 43579 | PASS      |
| 175    | 174     | 5      | 9      | 7.6   | 3302  | PASS      |
| 176    | 174     | 95     | 101    | 95.5  | 41616 | PASS      |
| 177    | 176     | 5      | 9      | 6.0   | 2515  | PASS      |