


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX083119\
Data File : VX011941.D
Acq On : 31 Aug 2019 08:51
Operator : SY/SP
Sample : BFB
Misc : 5.00µ/5.0mL/MSVOA X/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082919S.M
Title : SW846 8260
Last Update : Fri Aug 30 01:59:05 2019

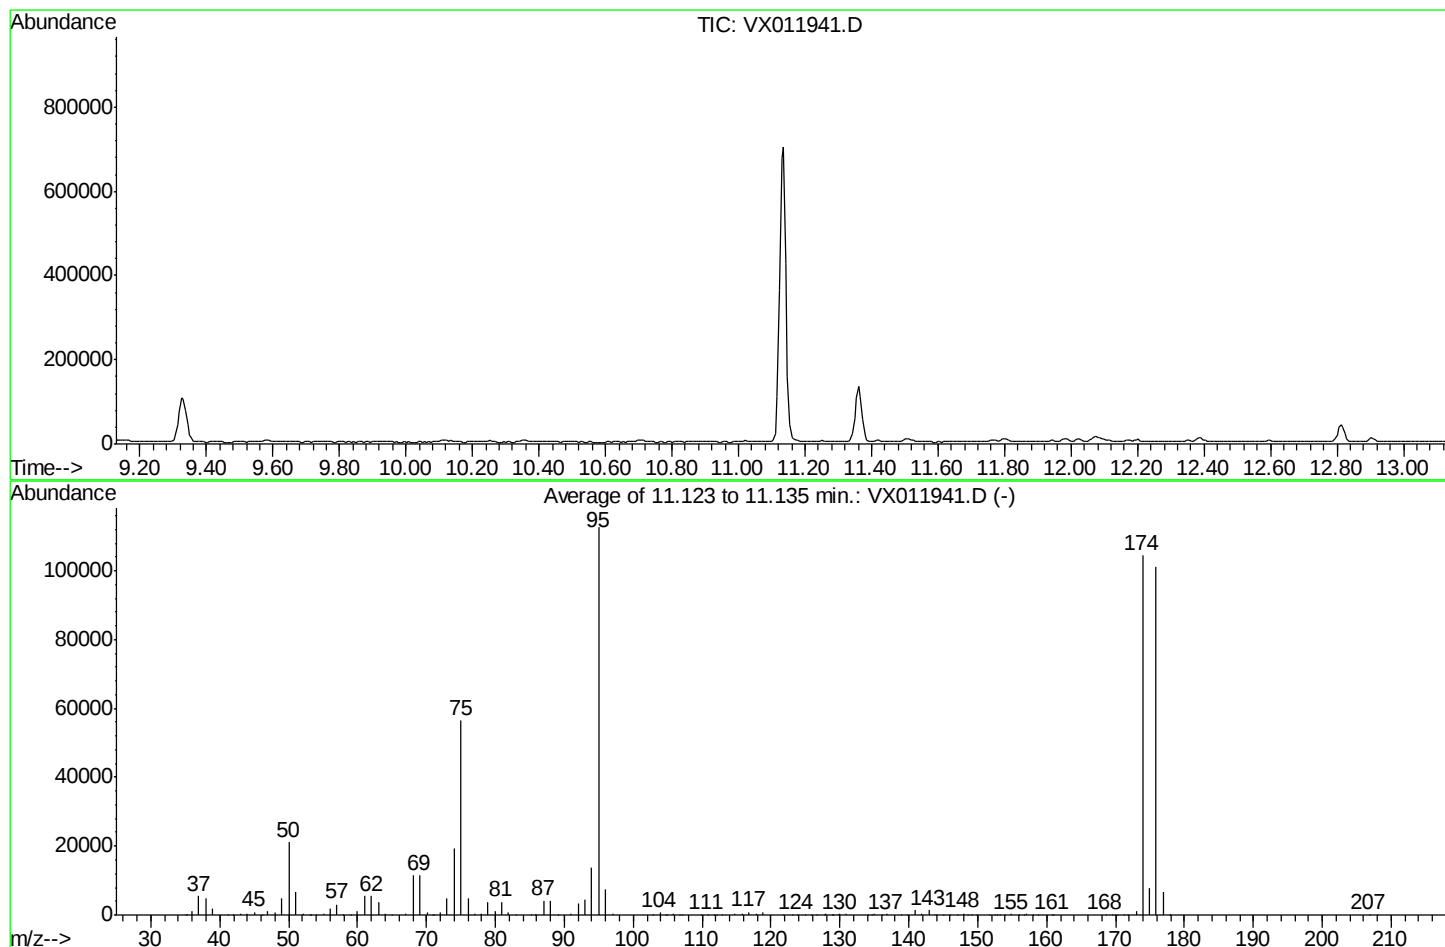

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1669

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	21169	PASS
75	95	30	60	50.1	56455	PASS
95	95	100	100	100.0	112632	PASS
96	95	5	9	6.6	7451	PASS
173	174	0.00	2	1.2	1263	PASS
174	95	50	100	92.8	104496	PASS
175	174	5	9	7.6	7903	PASS
176	174	95	101	96.9	101298	PASS
177	176	5	9	6.7	6784	PASS