


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX083119\
Data File : VX011963.D
Acq On : 31 Aug 2019 21:32
Operator : SY/SP
Sample : BFB
Misc : 5.00µ/5.0mL/MSVOA X/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082919S.M
Title : SW846 8260
Last Update : Fri Aug 30 01:59:05 2019

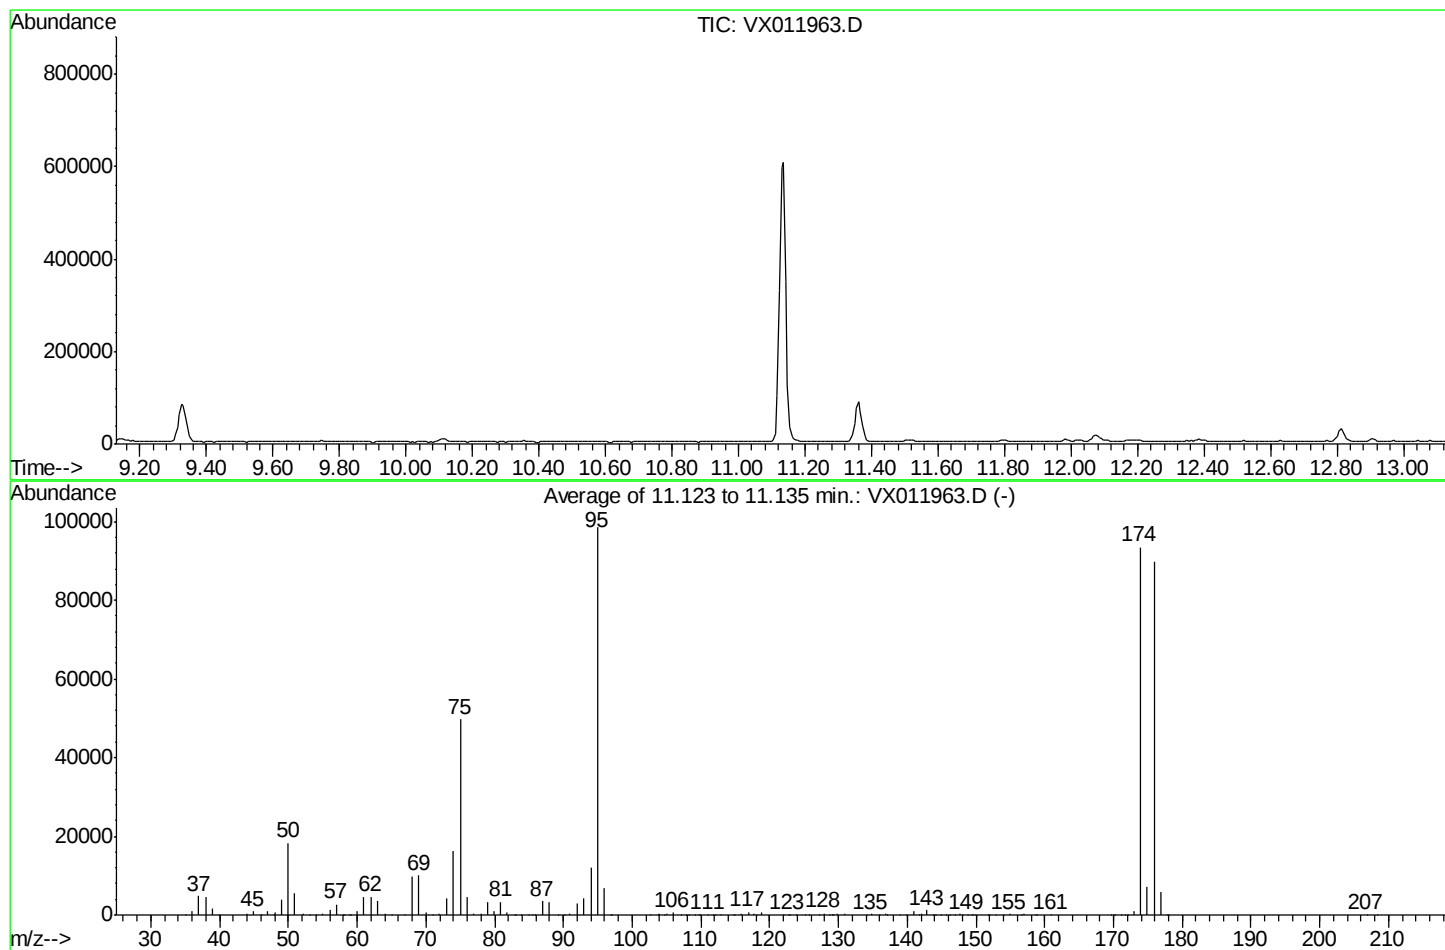

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	18377	PASS
75	95	30	60	50.4	49685	PASS
95	95	100	100	100.0	98524	PASS
96	95	5	9	6.9	6802	PASS
173	174	0.00	2	1.2	1109	PASS
174	95	50	100	94.9	93472	PASS
175	174	5	9	7.6	7083	PASS
176	174	95	101	95.9	89653	PASS
177	176	5	9	6.5	5859	PASS