
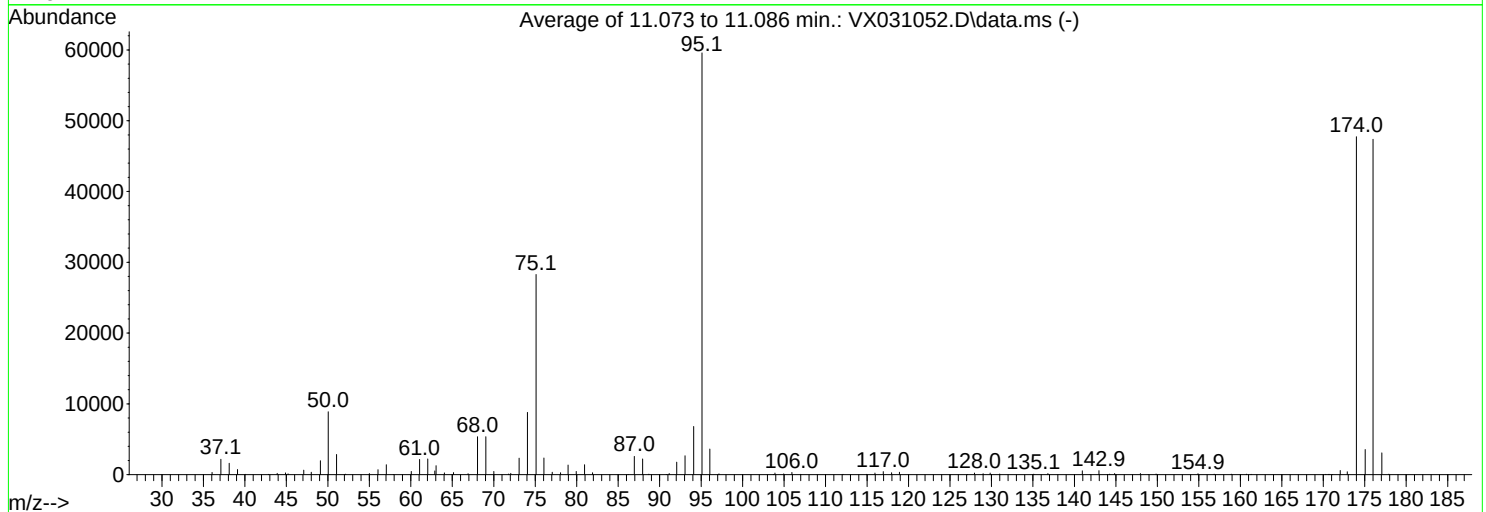


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090222\
 Data File : VX031052.D
 Acq On : 02 Sep 2022 08:53
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
 Title : SW846 8260
 Last Update : Fri Sep 02 02:49:21 2022

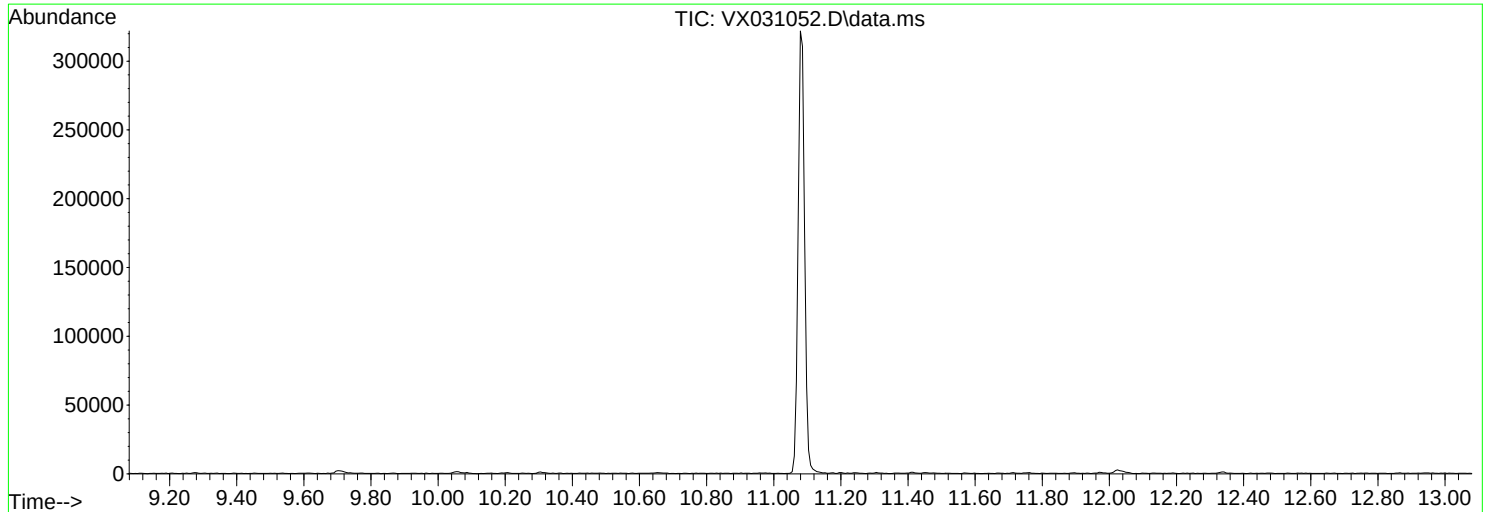

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	14.9	8889	FAIL*
75	95	30	60	47.4	28272	PASS
95	95	100	100	100.0	59589	PASS
96	95	5	9	6.1	3612	PASS
173	174	0.00	2	0.9	416	PASS
174	95	50	100	80.1	47736	PASS
175	174	5	9	7.4	3547	PASS
176	174	95	101	99.3	47384	PASS
177	176	5	9	6.5	3071	PASS