

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091423\
 Data File : VX037726.D
 Acq On : 14 Sep 2023 13:42
 Operator : JC/MD
 Sample : 04374-06 20X
 Misc : 2.71g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Sep 15 01:33:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 10:10:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	257036	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	426844	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	396953	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	184033	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	163930	39.419	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	78.840%		
35) Dibromofluoromethane	5.385	113	134413	44.426	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	88.860%		
50) Toluene-d8	8.647	98	513370	44.991	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	89.980%#		
62) 4-Bromofluorobenzene	11.079	95	186224	45.237	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.480%		
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.940	59	1243	Below Cal	#	78
13) Acrolein	2.245	56	272	0.400	ug/l #	31
16) Acetone	2.386	43	1172	0.697	ug/l	97
20) Methylene Chloride	2.788	84	1821	Below Cal		94
31) Cyclohexane	5.544	56	7011	1.464	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	19620	4.767	ug/l #	51
38) Carbon Tetrachloride	5.550	117	25343	6.027	ug/l #	15
39) Methylcyclohexane	7.379	83	4093	0.840	ug/l	89
48) Methyl methacrylate	7.659	41	967	0.266	ug/l #	57
51) 4-Methyl-2-Pentanone	8.616	43	3730	0.756	ug/l #	37
55) 1,1,2-Trichloroethane	9.104	97	3186	0.943	ug/l #	21
56) Ethyl methacrylate	9.104	69	1075	0.208	ug/l #	8
59) 2-Hexanone	9.384	43	3842	1.009	ug/l #	32
68) m/p-Xylenes	10.305	106	2589	0.451	ug/l	80
73) Isopropylbenzene	10.963	105	3159	0.229	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	93618	23.139	ug/l #	39
77) Bromobenzene	11.201	156	2030	0.622	ug/l #	16
78) n-propylbenzene	11.305	91	11475	0.724	ug/l	94
79) 2-Chlorotoluene	11.457	91	3433	0.352	ug/l	76
80) 1,3,5-Trimethylbenzene	11.451	105	20113	1.737	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	93618	70.336	ug/l #	5
82) 4-Chlorotoluene	11.457	91	3433	0.308	ug/l	83
84) 1,2,4-Trimethylbenzene	11.750	105	91067	7.800	ug/l	97
85) sec-Butylbenzene	11.890	105	7375	0.514	ug/l	98
86) p-Isopropyltoluene	12.012	119	9330	0.793	ug/l	92
89) n-Butylbenzene	12.317	91	34398	3.227	ug/l #	1
90) Hexachloroethane	12.530	117	11205	5.642	ug/l #	18
92) 1,2-Dibromo-3-Chloropr...	12.920	75	1116	1.054	ug/l #	11
93) 1,2,4-Trichlorobenzene	13.591	180	1332	0.357	ug/l #	24
94) Hexachlorobutadiene	13.725	225	345	0.221	ug/l	83
95) Naphthalene	13.780	128	12782	0.945	ug/l #	90
96) 1,2,3-Trichlorobenzene	13.963	180	1215	0.317	ug/l #	22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091423\
Data File : VX037726.D
Acq On : 14 Sep 2023 13:42
Operator : JC/MD
Sample : 04374-06 20X
Misc : 2.71g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Sep 15 01:33:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 10:10:04 2023
Response via : Initial Calibration




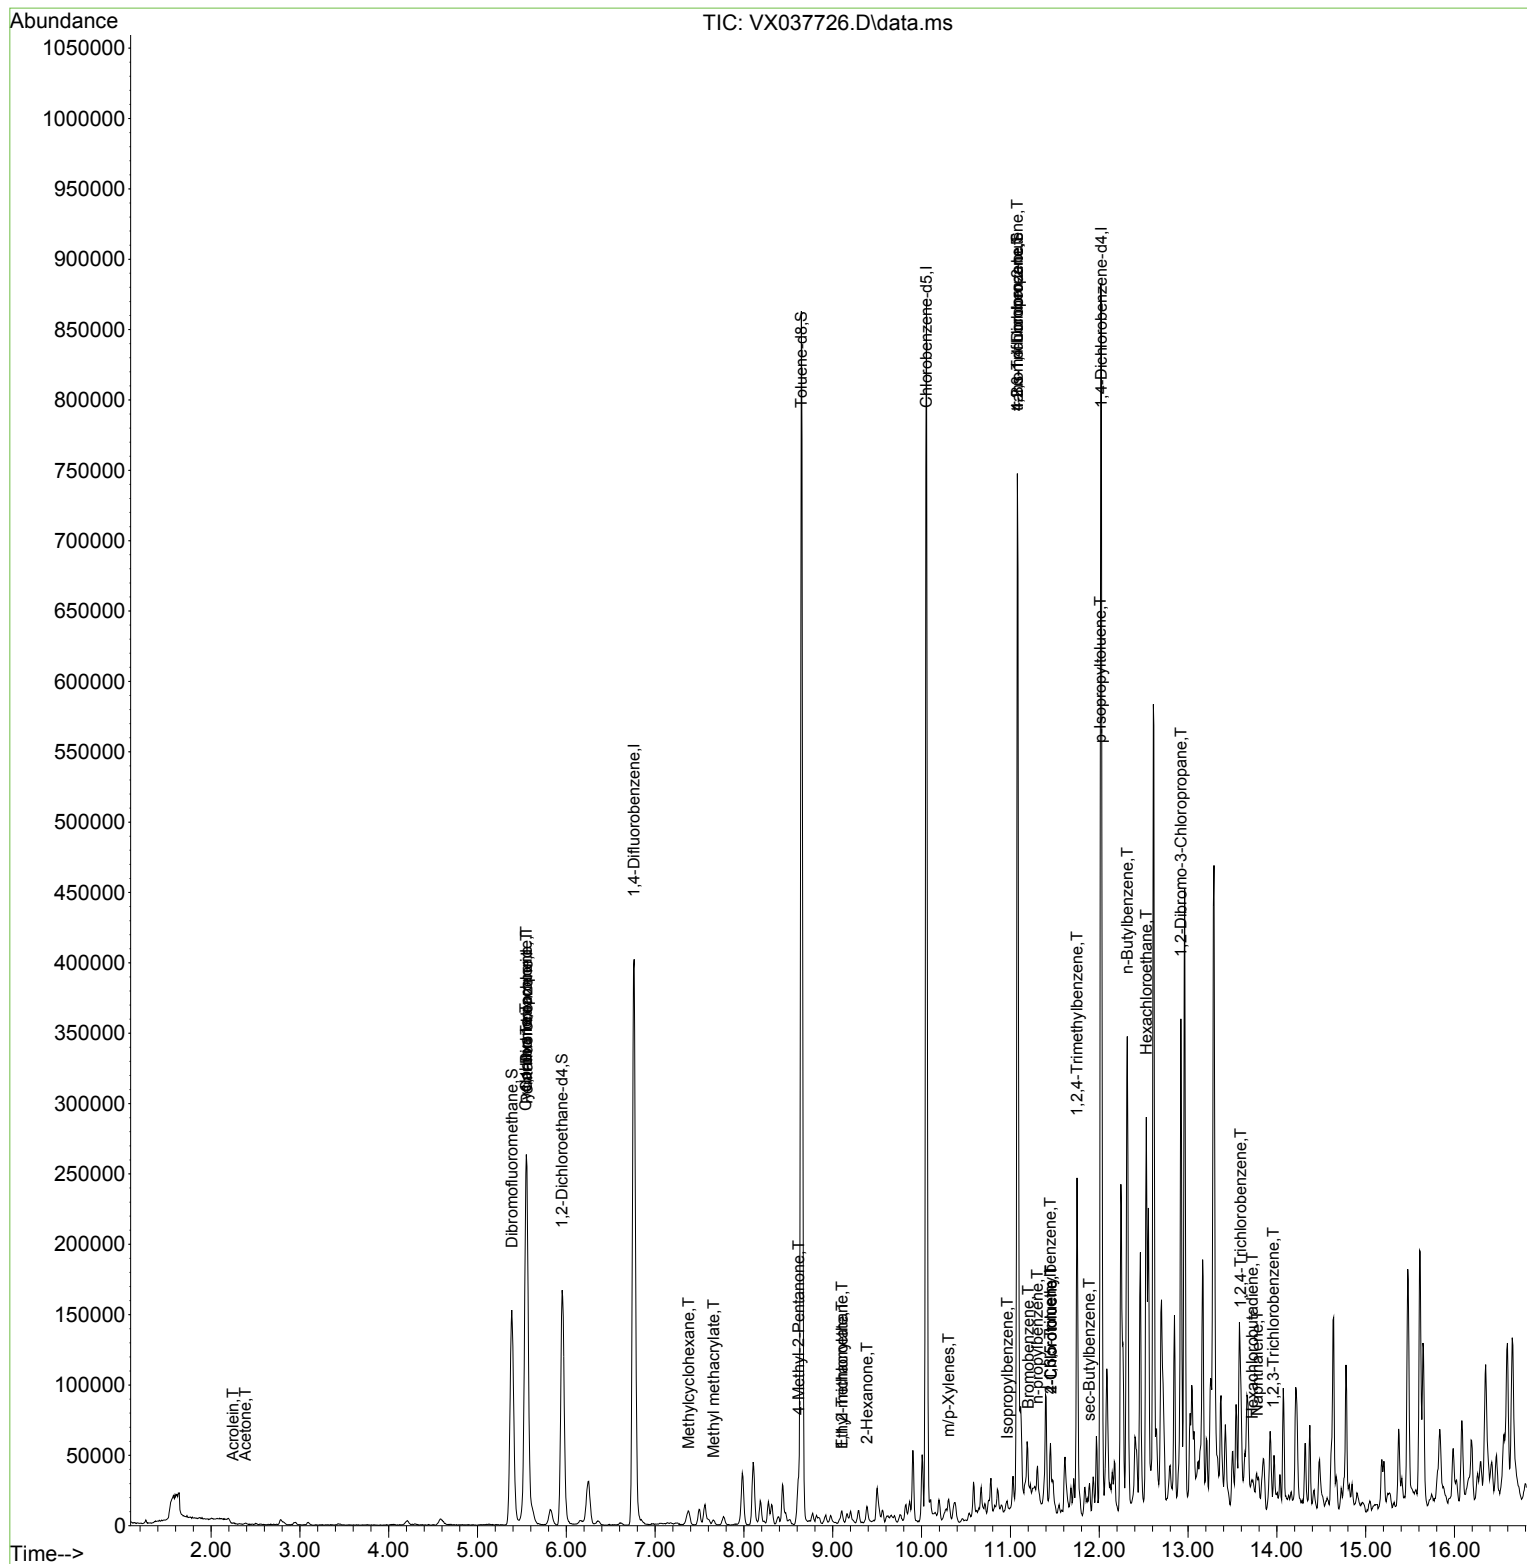


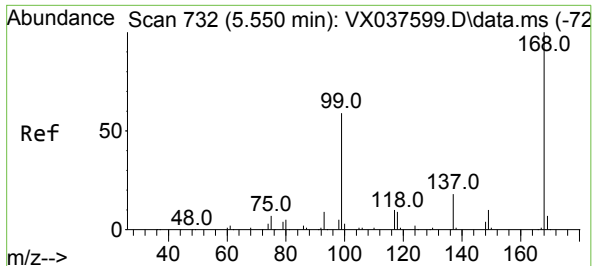

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 257036
Ion Ratio Lower Upper
168 100
99 54.3 56.6 85.0#

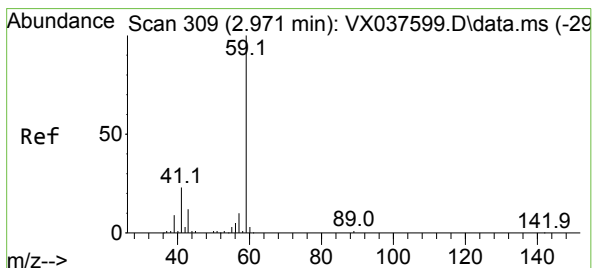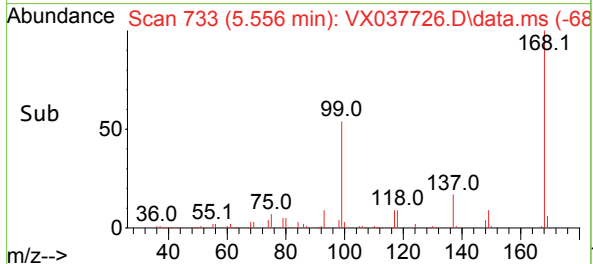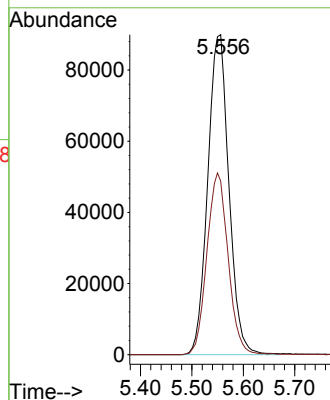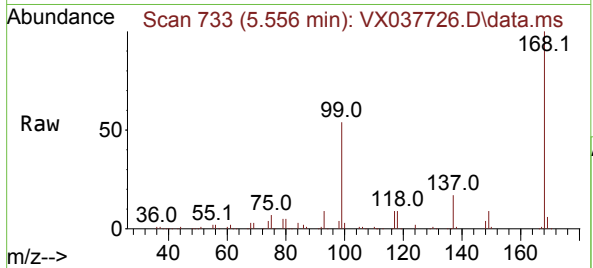

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.940 min Scan# 304
Delta R.T. -0.031 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Tgt Ion: 59 Resp: 1243
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#


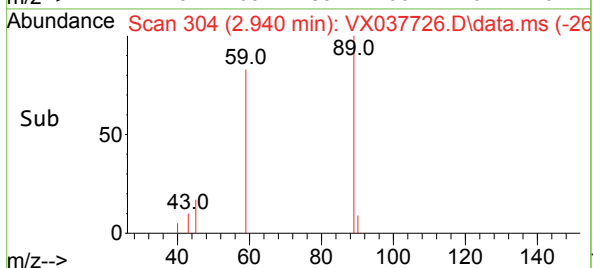
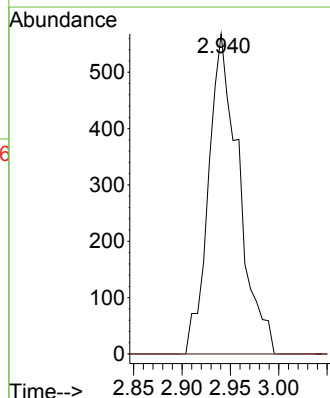
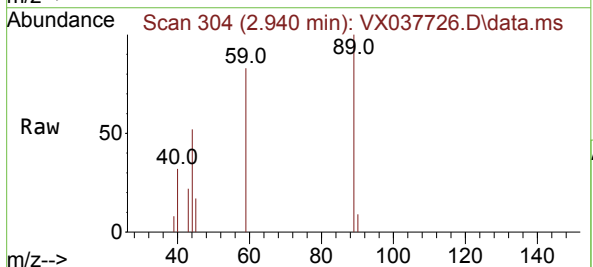




#13
Acrolein
Concen: 0.400 ug/l
RT: 2.245 min Scan# 190
Delta R.T. 0.006 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 56 Resp: 272
Ion Ratio Lower Upper
56 100
55 14.3 57.1 85.7#

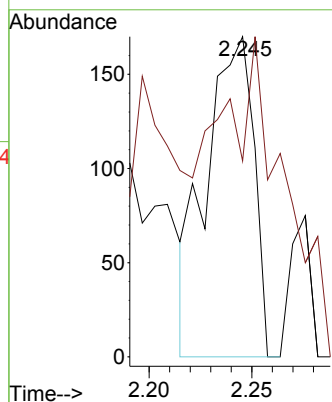

#16
Acetone
Concen: 0.697 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42


Tgt Ion: 43 Resp: 1172
Ion Ratio Lower Upper
43 100
58 28.9 21.9 32.9

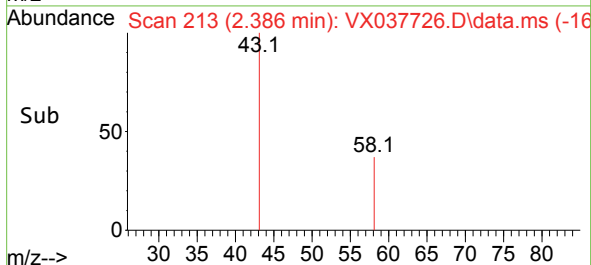






#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion: 84 Resp: 1821




Ion	Ratio	Lower	Upper
84	100		
49	122.1	103.6	155.4
51	37.4	33.8	50.6
86	59.8	49.4	74.0




#31
Cyclohexane
Concen: 1.464 ug/l
RT: 5.544 min Scan# 731
Delta R.T. 0.073 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Tgt Ion: 56 Resp: 7011

Ion	Ratio	Lower	Upper
56	100		
69	173.7	23.4	35.2#
84	130.8	65.9	98.9#





#33

1,2-Dichloroethane-d4

Concen: 39.419 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 163930

Ion Ratio Lower Upper

65 100

67 52.2 0.0 100.2

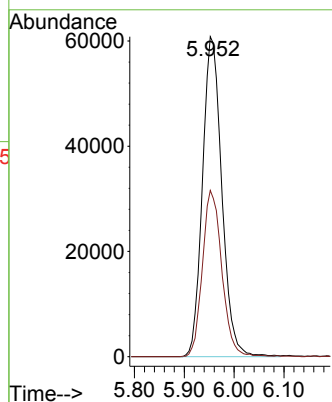

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42




Tgt Ion: 114 Resp: 426844


Ion Ratio Lower Upper

114 100

63 19.1 0.0 45.0


88 15.7 0.0 36.6

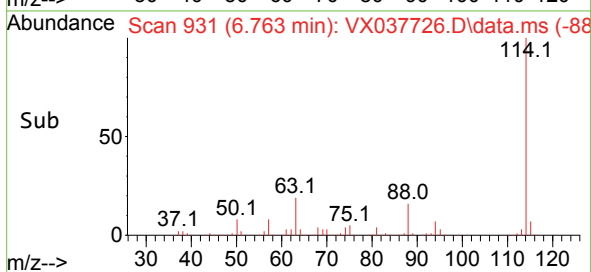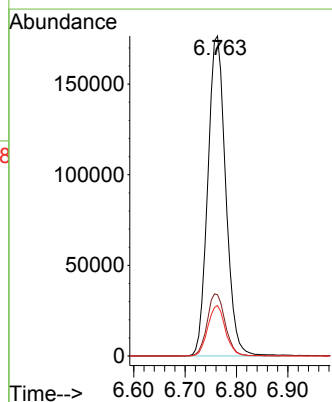



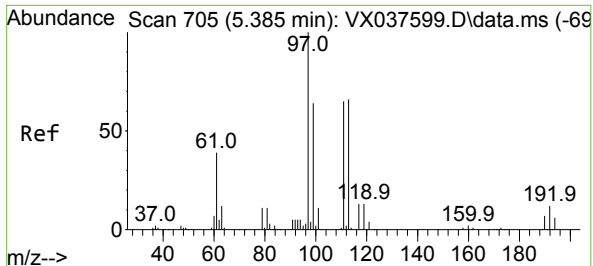


#35
Dibromofluoromethane
Concen: 44.426 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Instrument :
MSVOA_X
ClientSampleId :



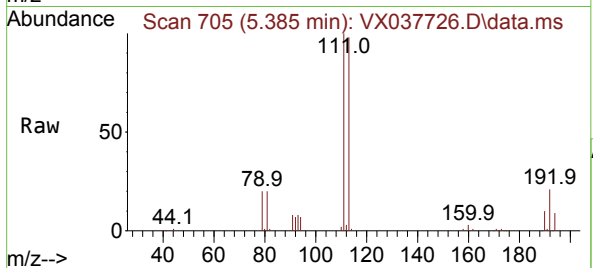



Tgt Ion:113 Resp: 134413
Ion Ratio Lower Upper
113 100
111 102.3 82.9 124.3
192 19.5 13.3 19.9

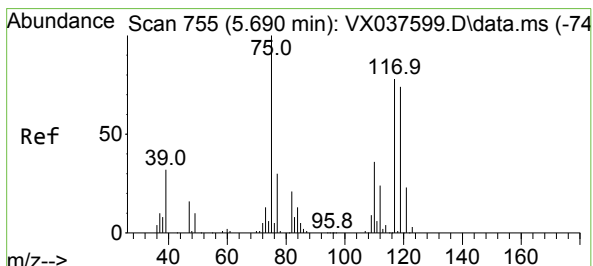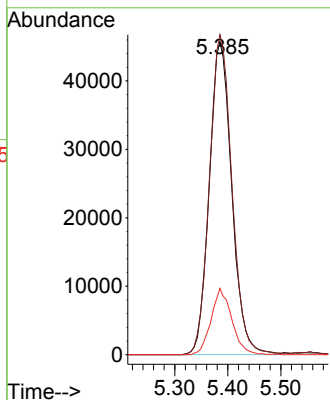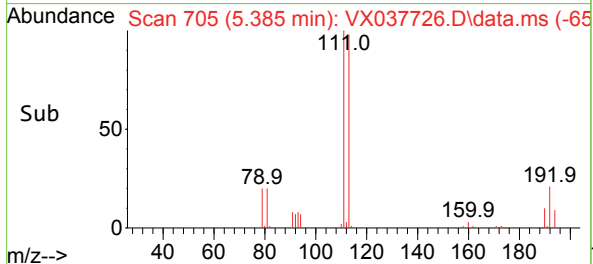

#36
1,1-Dichloropropene
Concen: 4.767 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42


Tgt Ion: 75 Resp: 19620
Ion Ratio Lower Upper
75 100
110 9.5 17.0 50.9#
77 0.0 24.7 37.1#

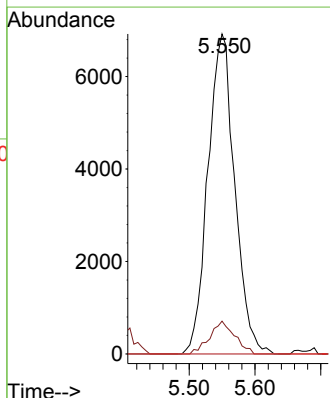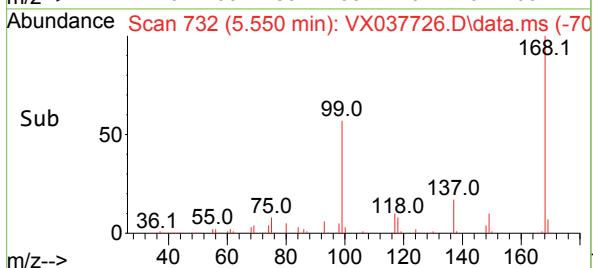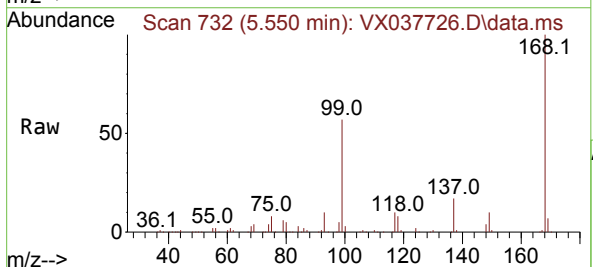






#38
Carbon Tetrachloride
Concen: 6.027 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 25343
Ion Ratio Lower Upper
117 100
119 5.4 78.2 117.2#
121 0.0 24.4 36.6#



#39
Methylcyclohexane
Concen: 0.840 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.000 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Tgt Ion: 83 Resp: 4093
Ion Ratio Lower Upper
83 100
55 67.1 64.6 97.0
98 43.1 36.7 55.1





#48

Methyl methacrylate

Concen: 0.266 ug/l

RT: 7.659 min Scan# 1084

Delta R.T. -0.037 min

Lab File: VX037726.D





Acq: 14 Sep 2023 13:42

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 41	Resp: 967
Ion Ratio	Lower Upper
41	100
69	136.2 59.2 88.8#
39	63.5 47.7 71.5

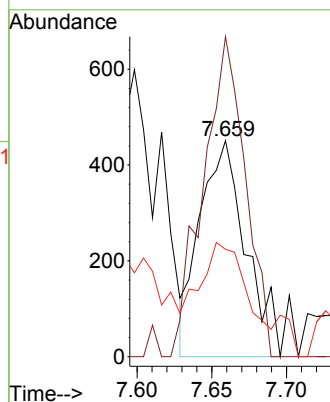

#50

Toluene-d8

Concen: 44.991 ug/l




RT: 8.647 min Scan# 1240


Delta R.T. -0.006 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42

Tgt Ion: 98	Resp: 513370
Ion Ratio	Lower Upper
98	100
100	64.3 53.1 79.7


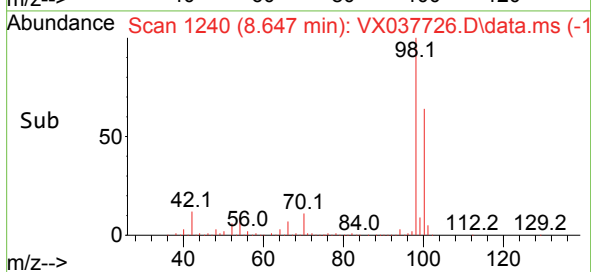
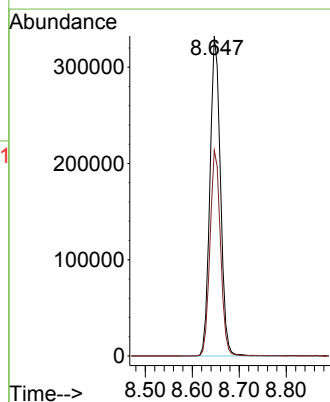





#51
4-Methyl-2-Pentanone
Concen: 0.756 ug/l
RT: 8.616 min Scan# 11
Delta R.T. 0.042 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 3730
Ion Ratio Lower Upper
43 100
58 0.0 30.4 45.6#

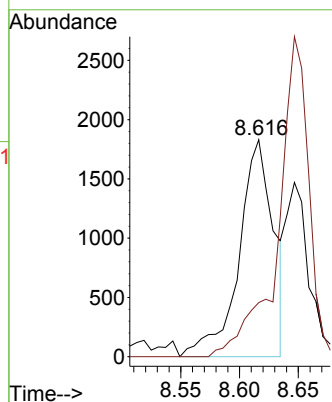

#55
1,1,2-Trichloroethane
Concen: 0.943 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.049 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Tgt Ion: 97 Resp: 3186
Ion Ratio Lower Upper
97 100
83 8.3 65.8 98.8#
85 0.0 41.6 62.4#
99 0.0 47.8 71.8#




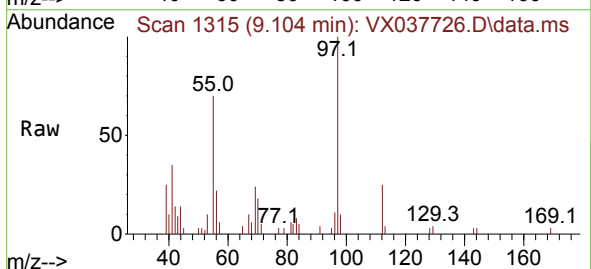




#56
Ethyl methacrylate
Concen: 0.208 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.012 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 69 Resp: 1075
Ion Ratio Lower Upper
69 100
41 166.4 56.8 85.2#
39 70.6 32.0 48.0#

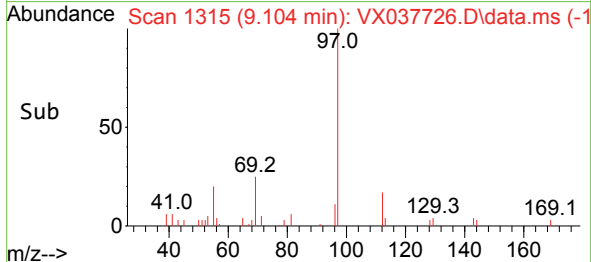

#59
2-Hexanone
Concen: 1.009 ug/l
RT: 9.384 min Scan# 1361
Delta R.T. -0.049 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Tgt Ion: 43 Resp: 3842
Ion Ratio Lower Upper
43 100
58 4.3 26.2 78.5#




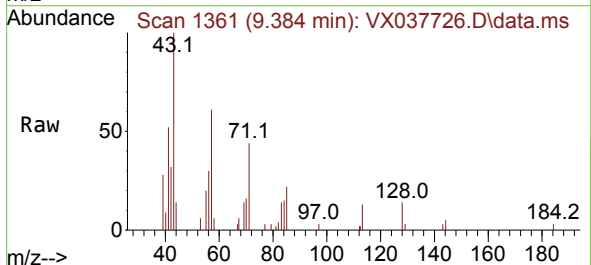




#62
4-Bromofluorobenzene
Concen: 45.237 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 186224
Ion Ratio Lower Upper
95 100
174 81.5 0.0 135.6
176 78.5 0.0 131.0

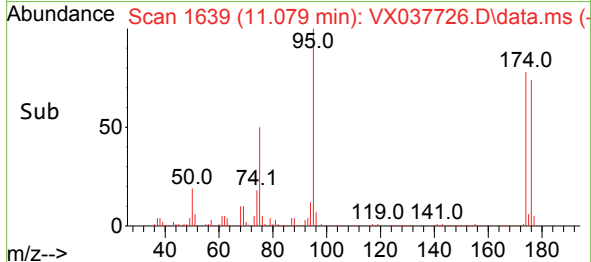

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Tgt Ion: 117 Resp: 396953
Ion Ratio Lower Upper
117 100
82 55.0 46.2 69.4
119 32.2 25.5 38.3




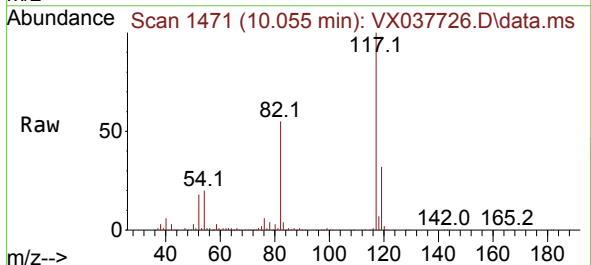


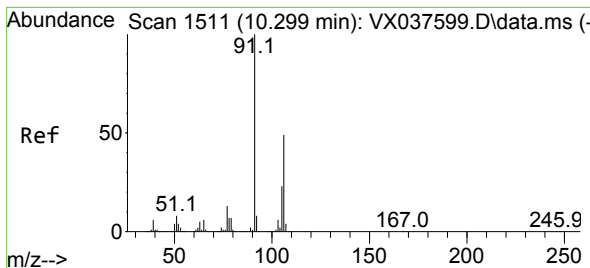

#68
m/p-Xylenes
Concen: 0.451 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 2589
Ion Ratio Lower Upper
106 100
91 238.0 165.5 248.3

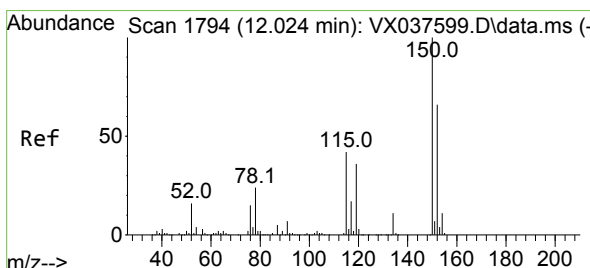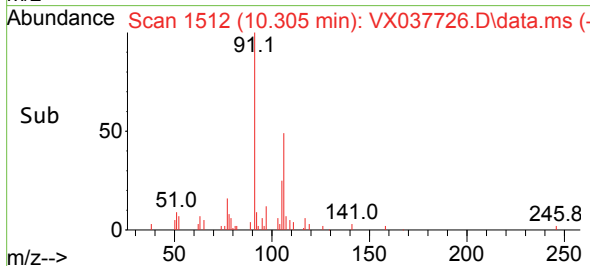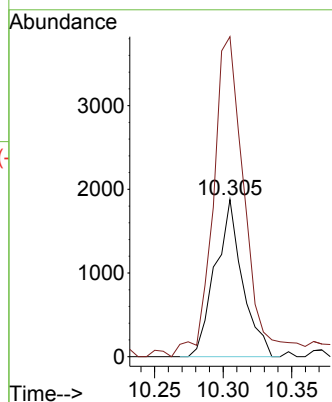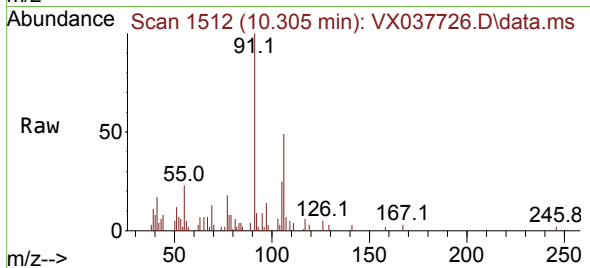

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Tgt Ion:152 Resp: 184033
Ion Ratio Lower Upper
152 100
115 58.9 43.3 129.9
150 157.3 0.0 345.0

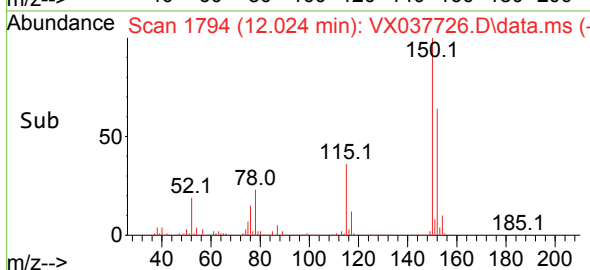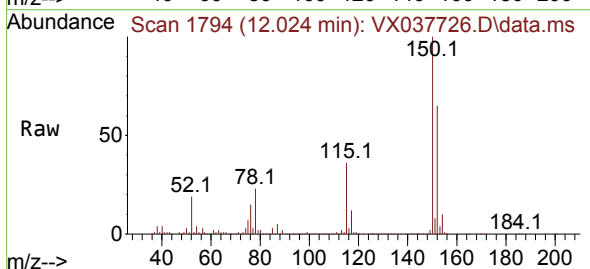



#73

Isopropylbenzene

Concen: 0.229 ug/l

RT: 10.963 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 3159

Ion Ratio Lower Upper

105 100

120 25.4 12.9 38.6

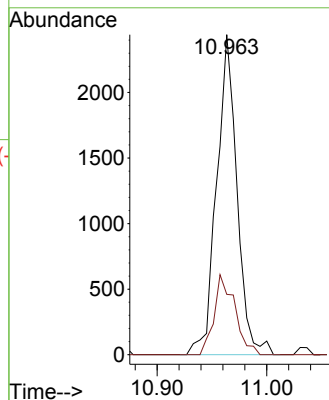

#76

1,2,3-Trichloropropane

Concen: 23.139 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX037726.D




Acq: 14 Sep 2023 13:42


Tgt Ion: 75 Resp: 93618

Ion Ratio Lower Upper

75 100

77 1.5 19.1 57.5#

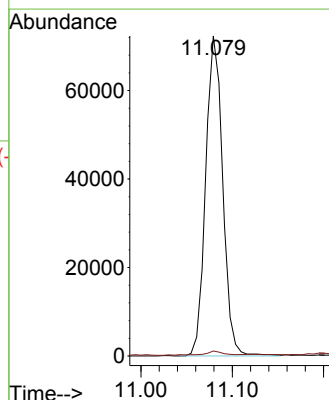



#77

Bromobenzene

Concen: 0.622 ug/l

RT: 11.201 min Scan# 1659

Delta R.T. -0.000 min

Lab File: VX037726.D





Acq: 14 Sep 2023 13:42

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:	156	Resp:	2030
Ion Ratio	Lower	Upper	
156	100		
77	52.7	88.4	265.3#
158	21.5	48.0	144.0#

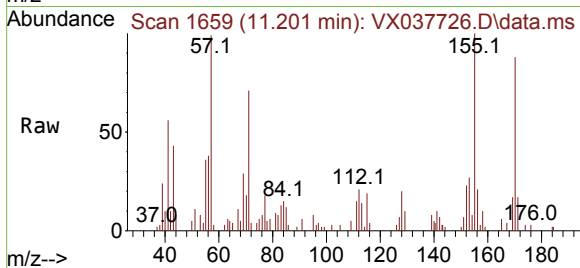

#78

n-propylbenzene

Concen: 0.724 ug/l




RT: 11.305 min Scan# 1676


Delta R.T. -0.000 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42

Tgt Ion:	91	Resp:	11475
Ion Ratio	Lower	Upper	
91	100		
120	25.8	11.5	34.4

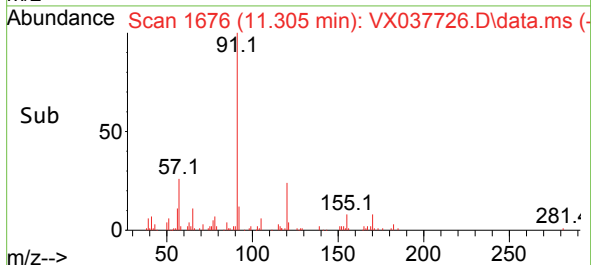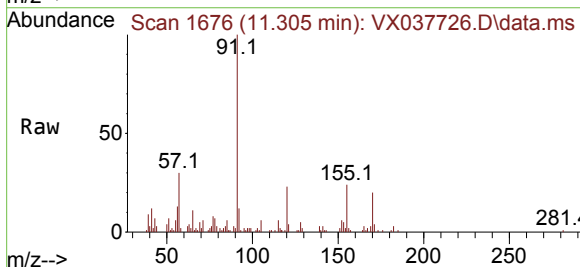



#79

2-Chlorotoluene

Concen: 0.352 ug/l

RT: 11.457 min Scan# 1

Delta R.T. 0.091 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 3433

Ion Ratio Lower Upper

91 100

126 19.2 16.3 48.8

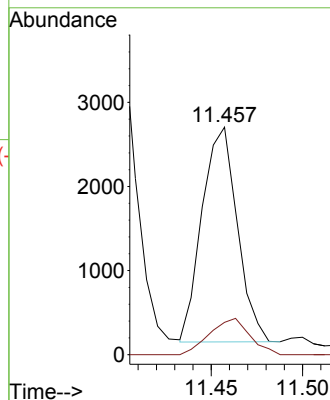

#80

1,3,5-Trimethylbenzene

Concen: 1.737 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX037726.D




Acq: 14 Sep 2023 13:42


Tgt Ion: 105 Resp: 20113

Ion Ratio Lower Upper

105 100

120 48.5 24.1 72.3


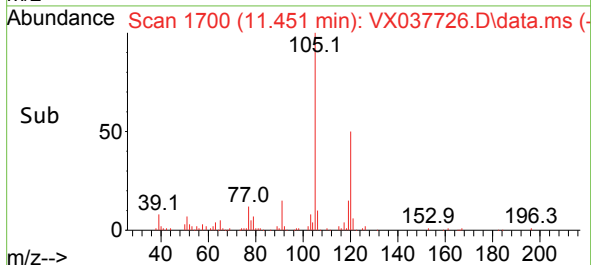
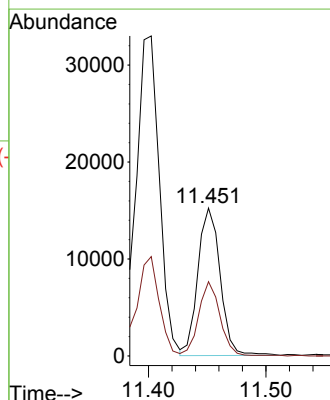





#81
trans-1,4-Dichloro-2-butene
Concen: 70.336 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 93618
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

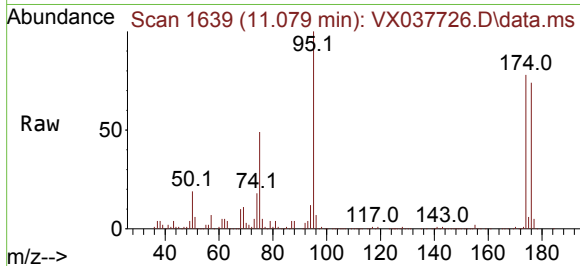

#82
4-Chlorotoluene
Concen: 0.308 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. -0.000 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Tgt Ion: 91 Resp: 3433
Ion Ratio Lower Upper
91 100
126 19.2 14.2 42.6

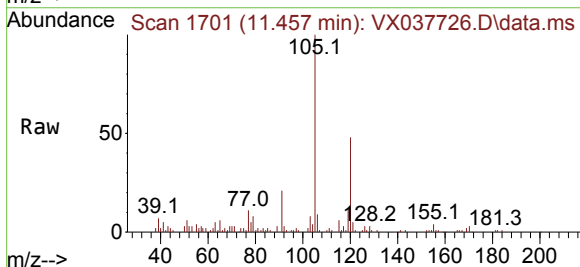



#84

1,2,4-Trimethylbenzene

Concen: 7.800 ug/l

RT: 11.750 min Scan# 1750

Delta R.T. -0.006 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 91067

Ion Ratio Lower Upper

105 100

120 44.2 21.2 63.6



#85

sec-Butylbenzene

Concen: 0.514 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. -0.000 min

Lab File: VX037726.D




Acq: 14 Sep 2023 13:42


Tgt Ion:105 Resp: 7375

Ion Ratio Lower Upper

105 100

134 18.8 9.8 29.4

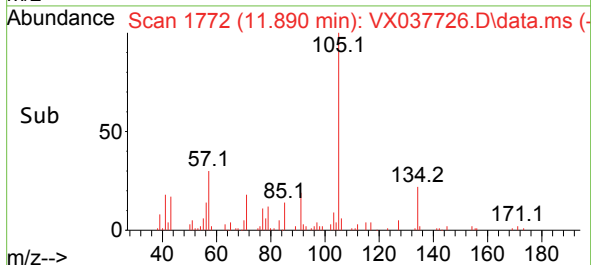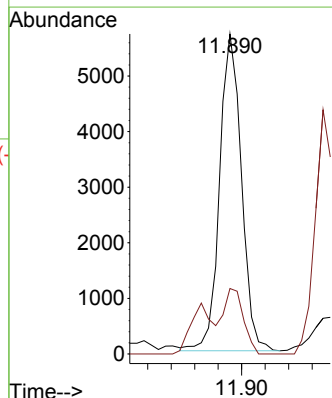



#86

p-Isopropyltoluene

Concen: 0.793 ug/l

RT: 12.012 min Scan# 119

Delta R.T. -0.000 min

Lab File: VX037726.D





Acq: 14 Sep 2023 13:42

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:119	Resp:	9330
Ion	Ratio	Lower Upper
119	100	
134	28.5	12.8 38.3
91	31.3	13.1 39.3

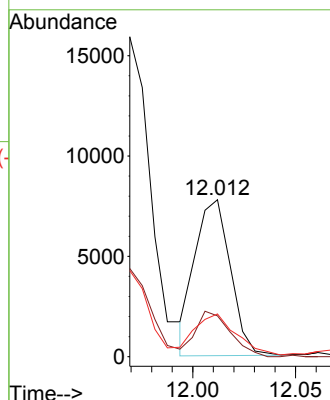

#89

n-Butylbenzene

Concen: 3.227 ug/l




RT: 12.317 min Scan# 1842


Delta R.T. -0.018 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42

Tgt Ion: 91	Resp:	34398
Ion	Ratio	Lower Upper
91	100	
92	19.7	27.4 82.0#
134	151.8	12.6 37.8#



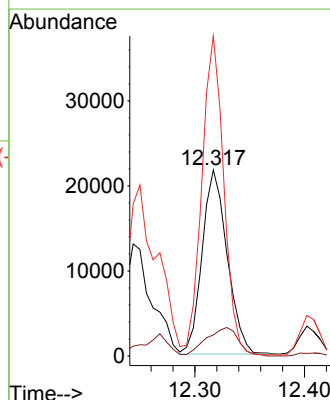





#90
Hexachloroethane
Concen: 5.642 ug/l
RT: 12.530 min Scan# 1117
Delta R.T. -0.012 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 11205
Ion Ratio Lower Upper
117 100
201 1.0 32.9 98.6#

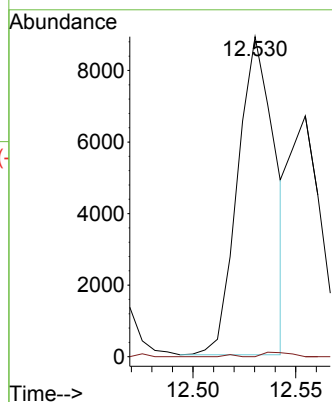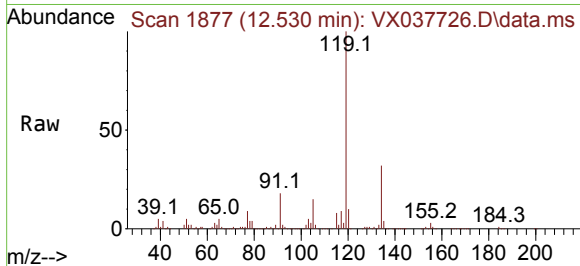

#92
1,2-Dibromo-3-Chloropropane
Concen: 1.054 ug/l
RT: 12.920 min Scan# 1941
Delta R.T. -0.024 min
Lab File: VX037726.D
Acq: 14 Sep 2023 13:42

Tgt Ion: 75 Resp: 1116
Ion Ratio Lower Upper
75 100
155 0.0 36.1 108.5#
157 4.8 44.9 134.7#





#93

1,2,4-Trichlorobenzene

Concen: 0.357 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. -0.000 min

Lab File: VX037726.D





Acq: 14 Sep 2023 13:42

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:180	Resp:	1332
Ion Ratio	Lower	Upper
180	100	
182	100.5	48.3 144.8
145	194.3	18.0 54.0#

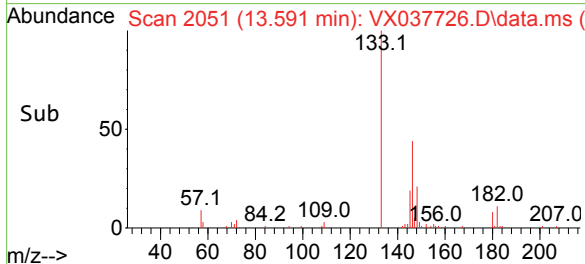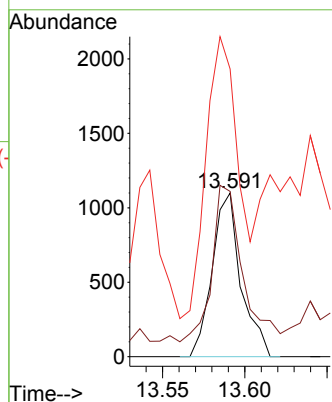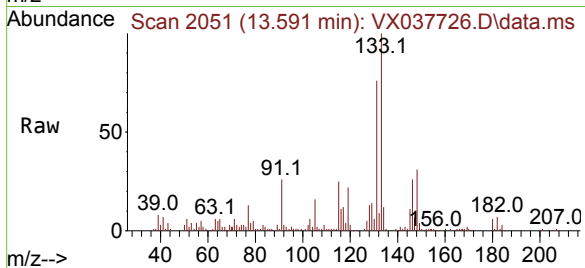

#94

Hexachlorobutadiene

Concen: 0.221 ug/l




RT: 13.725 min Scan# 2073


Delta R.T. -0.000 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42

Tgt Ion:225	Resp:	345
Ion Ratio	Lower	Upper
225	100	
223	69.0	31.1 93.2
227	83.8	32.5 97.5

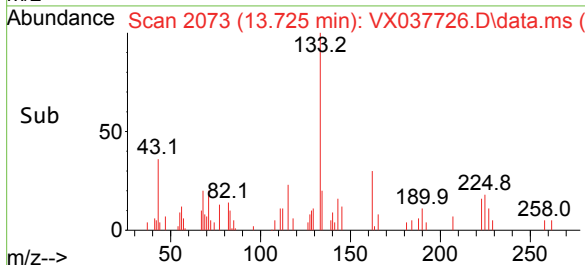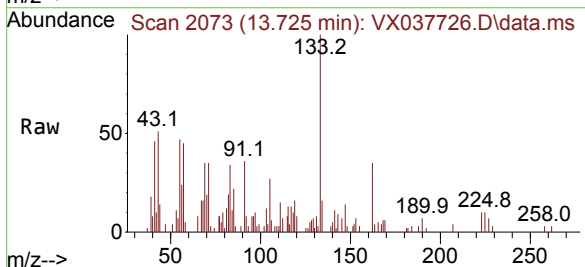

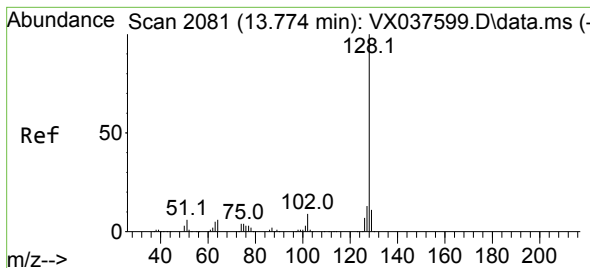

#95

Naphthalene

Concen: 0.945 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX037726.D





Acq: 14 Sep 2023 13:42

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:128	Resp:	12782
Ion Ratio	Lower	Upper
128	100	
127	15.3	10.3 15.5
129	16.7	8.8 13.2#

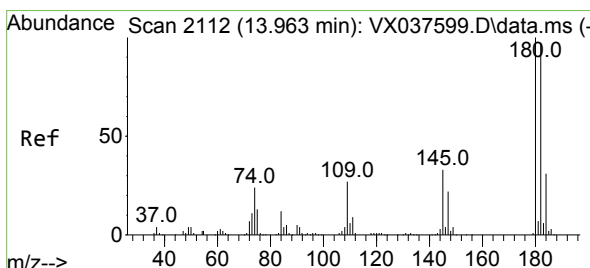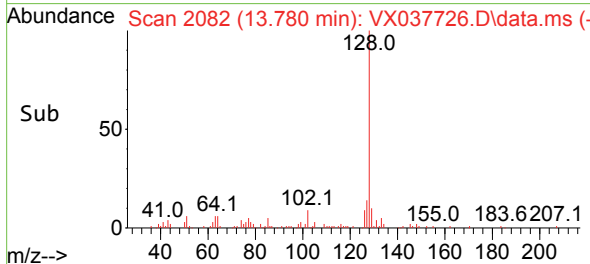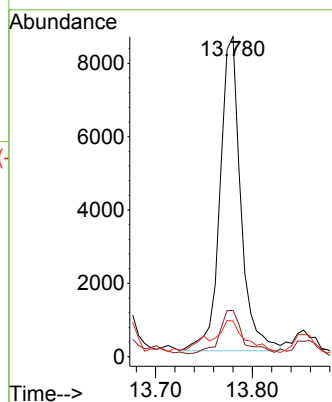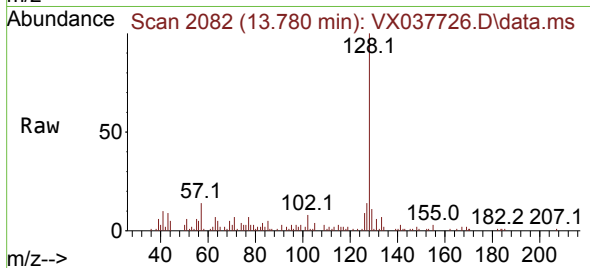

#96

1,2,3-Trichlorobenzene

Concen: 0.317 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX037726.D

Acq: 14 Sep 2023 13:42

Tgt Ion:180	Resp:	1215
Ion Ratio	Lower	Upper
180	100	
182	106.4	46.9 140.6
145	180.7	17.8 53.5#

