



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091423\
Data File : VX037719.D
Acq On : 14 Sep 2023 09:04
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 10:10:04 2023

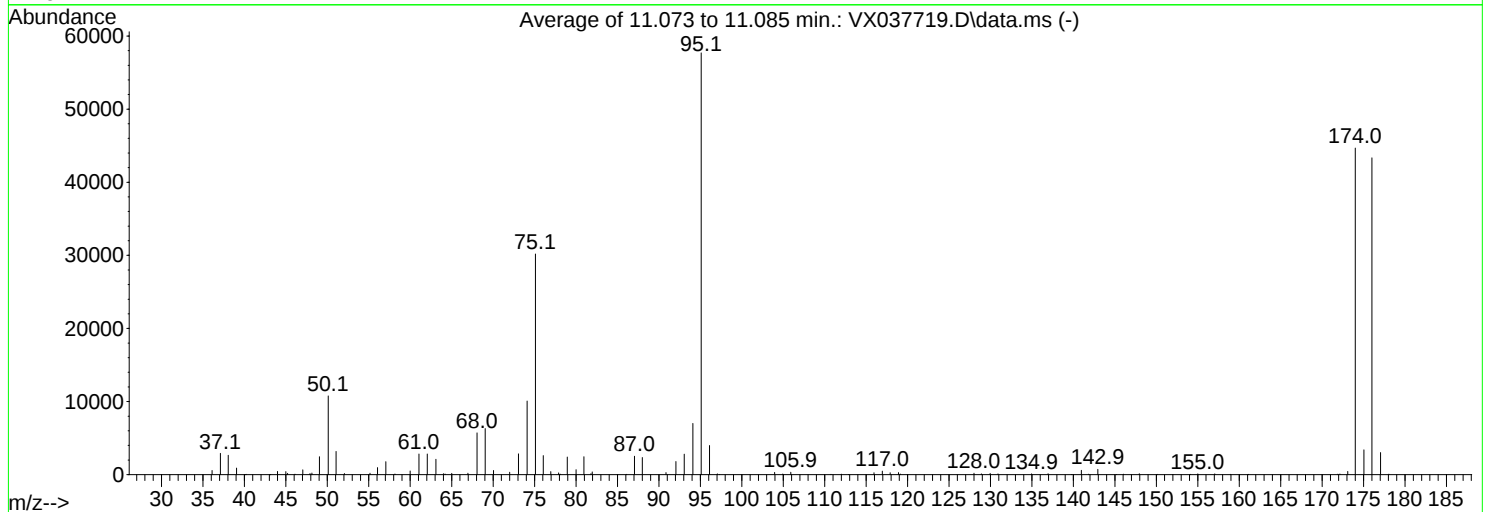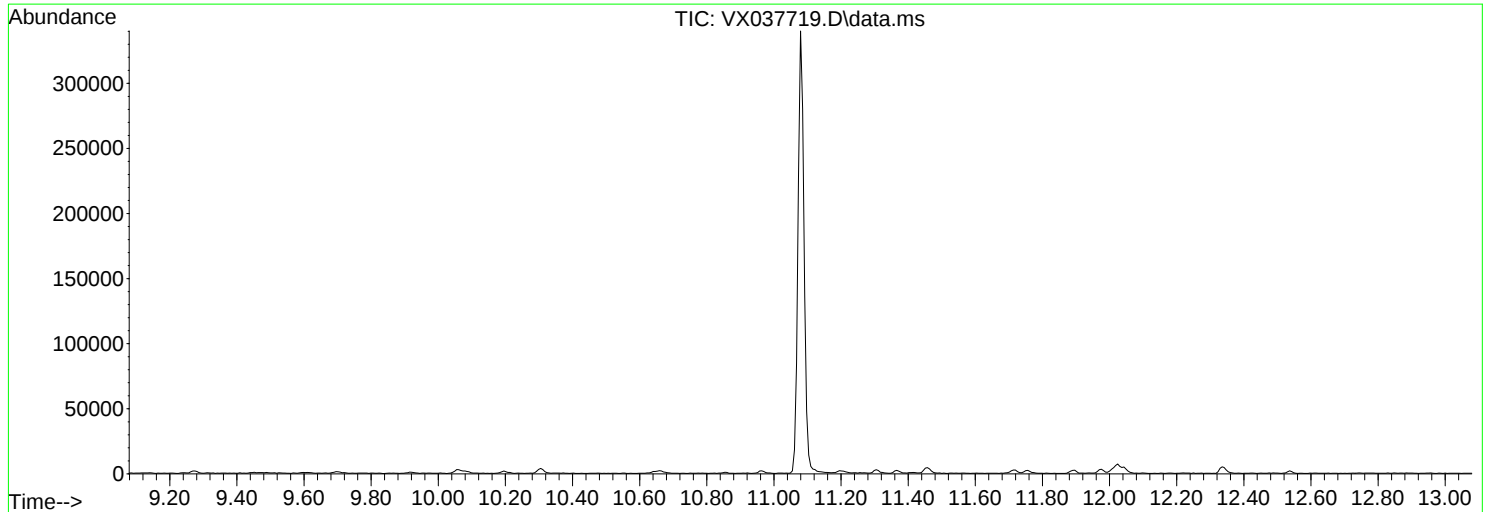

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	10771	PASS
75	95	30	60	52.3	30179	PASS
95	95	100	100	100.0	57704	PASS
96	95	5	9	6.9	3982	PASS
173	174	0.00	2	1.0	444	PASS
174	95	50	100	77.4	44675	PASS
175	174	5	9	7.6	3393	PASS
176	174	95	101	97.0	43341	PASS
177	176	5	9	7.0	3015	PASS