

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092022\
 Data File : VX031498.D
 Acq On : 20 Sep 2022 16:10
 Operator : JC/MD
 Sample : N4665-01ME
 Misc : 5.07G/10mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-1ME

Quant Time: Sep 20 17:55:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 09:45:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	62330	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.763	114	95086	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	97823	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	66348	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	61927	54.164	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 108.320%			
35) Dibromofluoromethane	5.391	113	49724	50.602	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.200%			
50) Toluene-d8	8.647	98	193334	51.034	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 102.060%			
62) 4-Bromofluorobenzene	11.085	95	57271	44.631	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 89.260%			
Target Compounds						Qvalue
5) Bromomethane	1.612	94	1547	0.801	ug/l #	70
6) Chloroethane	1.697	64	93	Below Cal	#	43
10) Methyl Iodide	2.428	142	321	0.331	ug/l #	67
11) Tert butyl alcohol	2.953	59	3996	Below Cal	#	73
13) Acrolein	2.209	56	38	Below Cal	#	1
16) Acetone	2.428	43	1049	Below Cal	#	57
18) Methyl Acetate	2.733	43	430	0.252	ug/l #	70
20) Methylene Chloride	2.776	84	1449	Below Cal	#	80
25) 2-Butanone	4.617	43	8546	9.684	ug/l	95
29) Tetrahydrofuran	5.062	42	578	1.004	ug/l #	66
31) Cyclohexane	5.544	56	1619	0.955	ug/l #	38
36) 1,1-Dichloropropene	5.544	75	5146	3.405	ug/l #	48
37) Ethyl Acetate	4.617	43	8546	4.740	ug/l #	68
38) Carbon Tetrachloride	5.544	117	6318	3.771	ug/l #	16
40) Benzene	6.038	78	2248	0.499	ug/l	92
41) Methacrylonitrile	5.050	41	323	0.360	ug/l #	44
43) Isopropyl Acetate	6.367	43	1842	0.665	ug/l #	61
51) 4-Methyl-2-Pentanone	8.647	43	986	0.553	ug/l #	1
52) Toluene	8.720	92	9828	3.342	ug/l	100
67) Ethyl Benzene	10.195	91	37858	7.108	ug/l	98
68) m/p-Xylenes	10.299	106	18267	8.534	ug/l	99
69) o-Xylene	10.647	106	10134	4.960	ug/l	100
70) Styrene	10.653	104	1281	0.381	ug/l #	1
73) Isopropylbenzene	10.964	105	6050	1.221	ug/l	97
75) 1,1,2,2-Tetrachloroethane	11.079	83	144	Below Cal	#	15
76) 1,2,3-Trichloropropane	11.085	75	33577	22.675	ug/l #	37
78) n-propylbenzene	11.305	91	2731	0.479	ug/l	94
79) 2-Chlorotoluene	11.616	91	890	0.262	ug/l	78
80) 1,3,5-Trimethylbenzene	11.451	105	13479	3.206	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.085	75	33577	73.009	ug/l #	11
82) 4-Chlorotoluene	11.616	91	1047	0.263	ug/l	84
83) tert-Butylbenzene	11.756	119	5685	1.395	ug/l #	48
84) 1,2,4-Trimethylbenzene	11.756	105	43727	10.560	ug/l	97
85) sec-Butylbenzene	11.756	105	43727	8.478	ug/l #	56
86) p-Isopropyltoluene	12.012	119	3826	0.879	ug/l	88
89) n-Butylbenzene	12.323	91	2450	0.660	ug/l #	20

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092022\
Data File : VX031498.D
Acq On : 20 Sep 2022 16:10
Operator : JC/MD
Sample : N4665-01ME
Misc : 5.07G/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME

Quant Time: Sep 20 17:55:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
90) Hexachloroethane	12.414	117	6444	8.611	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	12.969	75	217	0.637	ug/l #	3
95) Naphthalene	13.780	128	2977853	626.077	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092022\
Data File : VX031498.D
Acq On : 20 Sep 2022 16:10
Operator : JC/MD
Sample : N4665-01ME
Misc : 5.07G/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME

Quant Time: Sep 20 17:55:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration




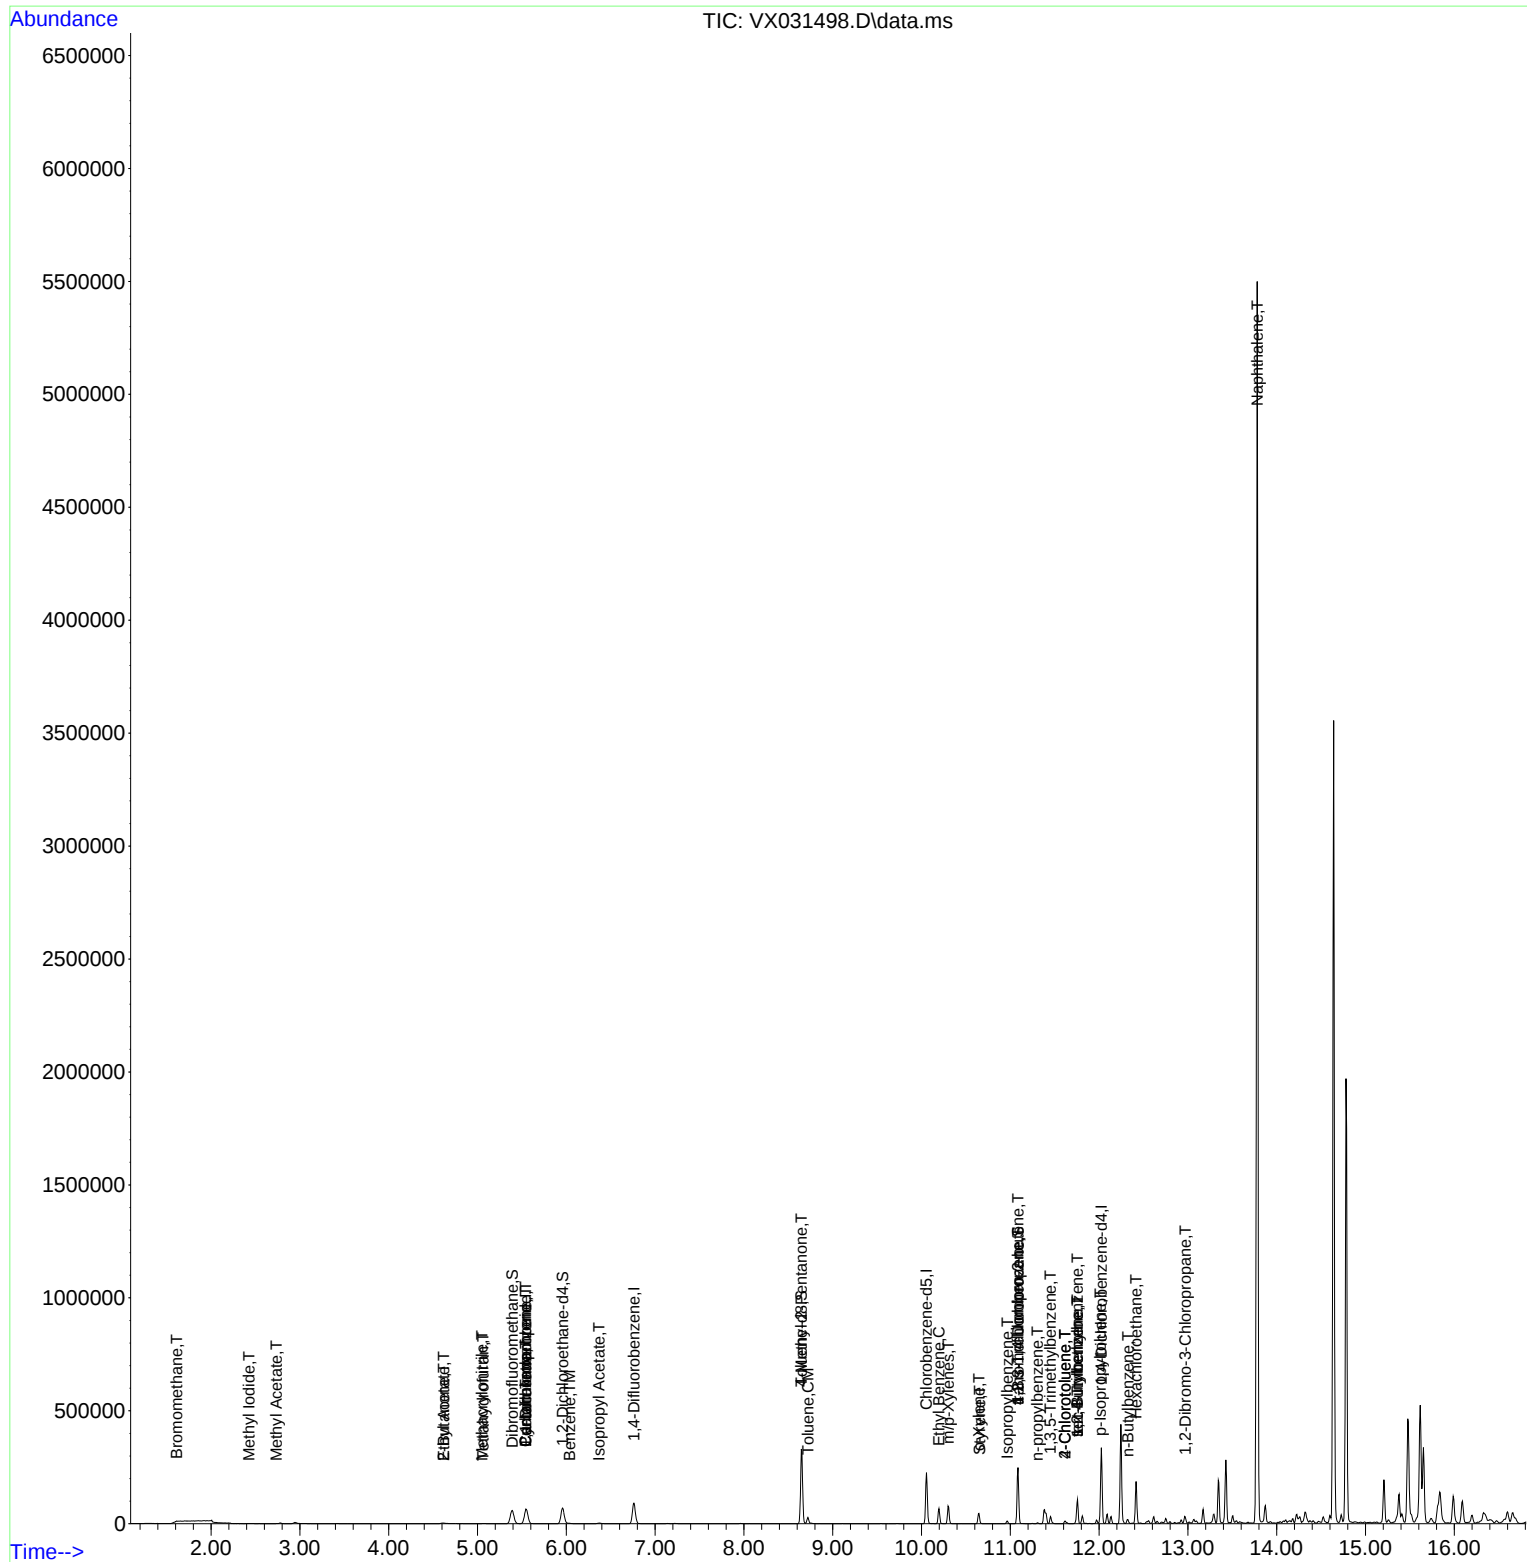




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.012 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion:168 Resp: 62330
Ion Ratio Lower Upper
168 100
99 57.0 48.8 73.2



#5
Bromomethane
Concen: 0.801 ug/l
RT: 1.612 min Scan# 86
Delta R.T. 0.001 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 94 Resp: 1547
Ion Ratio Lower Upper
94 100
96 121.9 74.4 111.6#



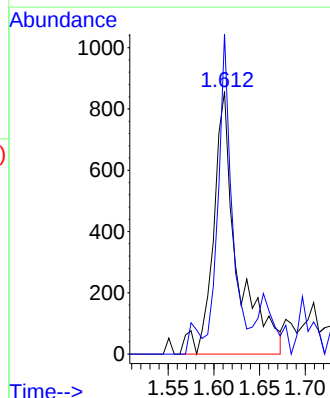



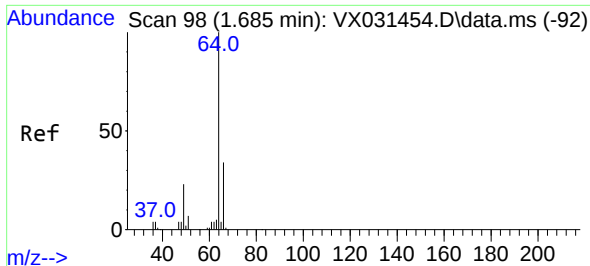

#6
Chloroethane
Concen: Below Cal
RT: 1.697 min Scan# 10
Delta R.T. 0.012 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 64 Resp: 93
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.4#

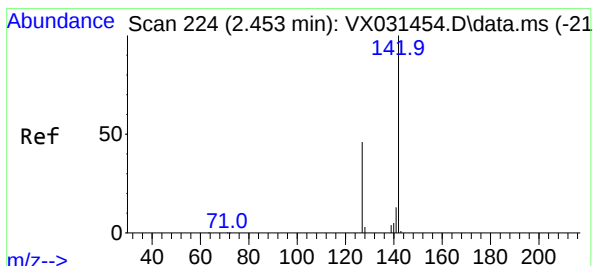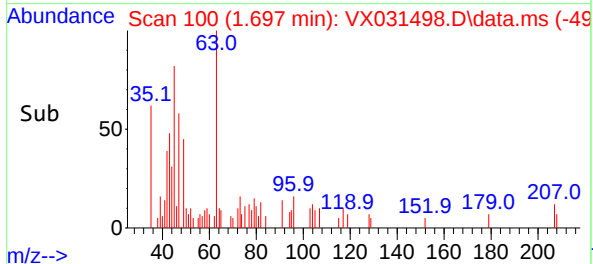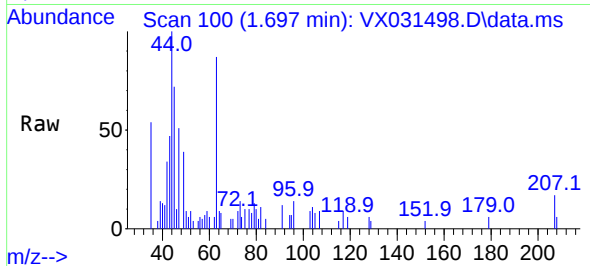

#10
Methyl Iodide
Concen: 0.331 ug/l
RT: 2.428 min Scan# 220
Delta R.T. -0.025 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 142 Resp: 321
Ion Ratio Lower Upper
142 100
127 25.5 37.4 56.0#
141 0.0 11.6 17.4#

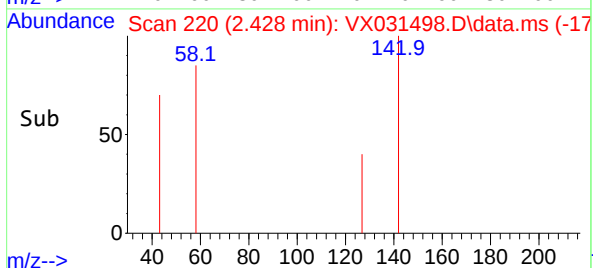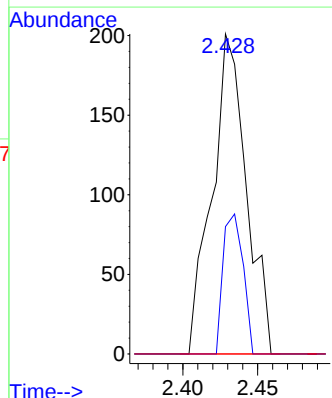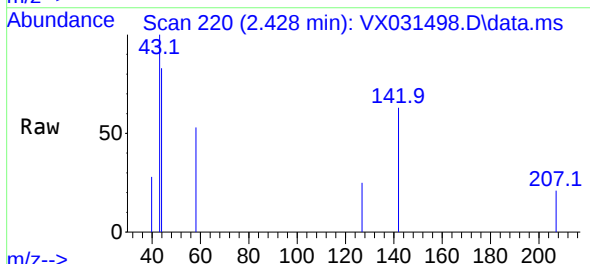



#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.953 min Scan# 306

Delta R.T. -0.036 min

Lab File: VX031498.D

Acq: 20 Sep 2022 16:10

Instrument :

MSVOA_X

ClientSampleId :





COMP-1ME

Tgt Ion: 59 Resp: 3996

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

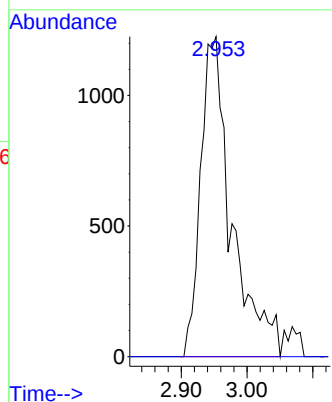

#13

Acrolein

Concen: Below Cal

RT: 2.209 min Scan# 184

Delta R.T. -0.030 min

Lab File: VX031498.D




Acq: 20 Sep 2022 16:10


Tgt Ion: 56 Resp: 38

Ion Ratio Lower Upper

56 100

55 310.5 56.0 84.0#


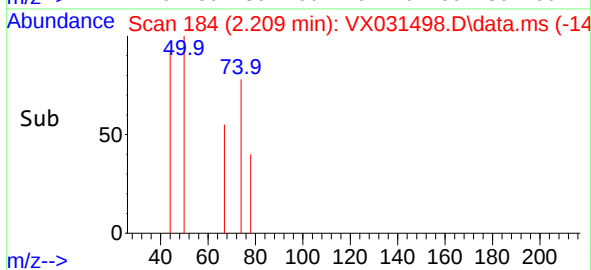






#16
Acetone
Concen: Below Cal
RT: 2.428 min Scan# 21
Delta R.T. 0.042 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 43 Resp: 1049
Ion Ratio Lower Upper
43 100
58 53.3 23.8 35.8#



#18
Methyl Acetate
Concen: 0.252 ug/l
RT: 2.733 min Scan# 270
Delta R.T. 0.024 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 43 Resp: 430
Ion Ratio Lower Upper
43 100
74 8.8 18.6 27.8#

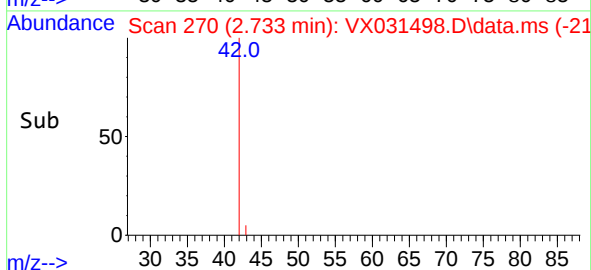



#20

Methylene Chloride

Concen: Below Cal

RT: 2.776 min Scan# 21

Delta R.T. -0.012 min

Lab File: VX031498.D

Acq: 20 Sep 2022 16:10

Instrument :

MSVOA_X

ClientSampleId :

COMP-1ME

Tgt Ion: 84 Resp: 1449


Ion Ratio Lower Upper

84 100



49 99.6 105.9 158.9#

51 46.0 32.2 48.2


86 54.9 50.8 76.2



Abundance

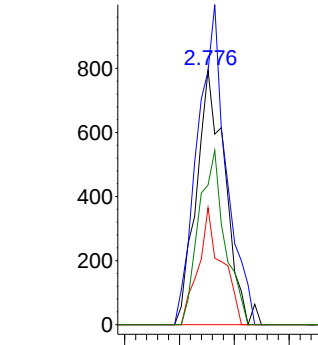

Time-->



#25

2-Butanone

Concen: 9.684 ug/l

RT: 4.617 min Scan# 579

Delta R.T. 0.055 min

Lab File: VX031498.D


Acq: 20 Sep 2022 16:10

Tgt Ion: 43 Resp: 8546



Ion Ratio Lower Upper

43 100


72 23.9 21.1 31.7



Abundance

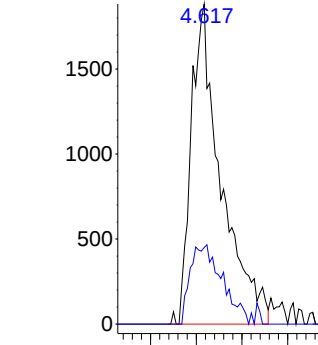

Time-->



#29

Tetrahydrofuran

Concen: 1.004 ug/l

RT: 5.062 min Scan# 61

Delta R.T. 0.049 min

Lab File: VX031498.D

Acq: 20 Sep 2022 16:10

Instrument :

MSVOA_X

ClientSampleId :

COMP-1ME





Tgt Ion: 42 Resp: 578

Ion Ratio Lower Upper

42 100

72 35.3 36.4 54.6#

71 8.0 33.5 50.3#

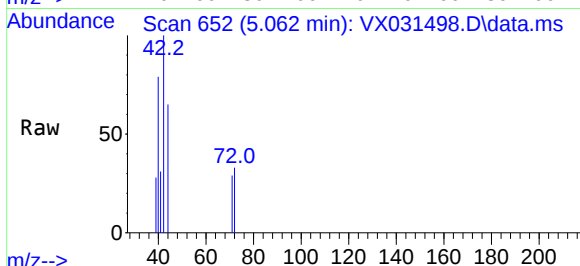

#31

Cyclohexane

Concen: 0.955 ug/l

RT: 5.544 min Scan# 731

Delta R.T. 0.073 min

Lab File: VX031498.D

Acq: 20 Sep 2022 16:10




Tgt Ion: 56 Resp: 1619


Ion Ratio Lower Upper

56 100

69 106.8 25.1 37.7#

84 120.2 70.2 105.4#


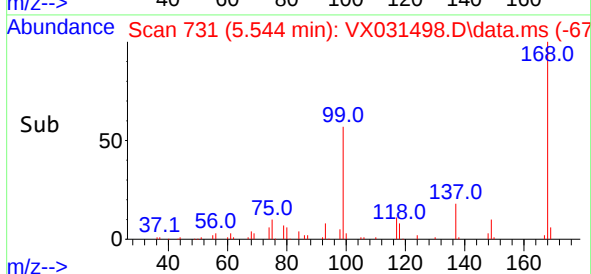

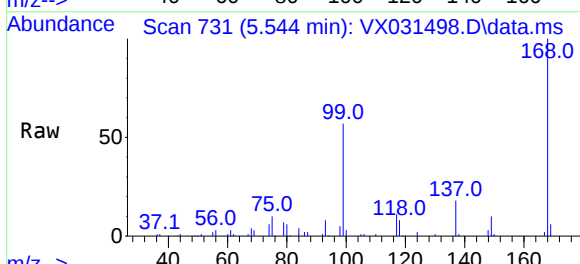


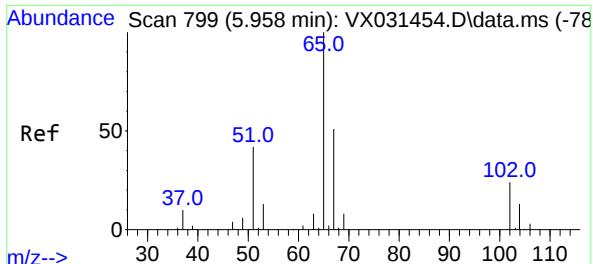

#33
1,2-Dichloroethane-d4
Concen: 54.164 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 65 Resp: 61927
Ion Ratio Lower Upper
65 100
67 52.3 0.0 102.4

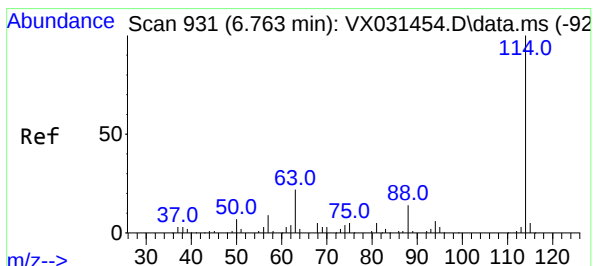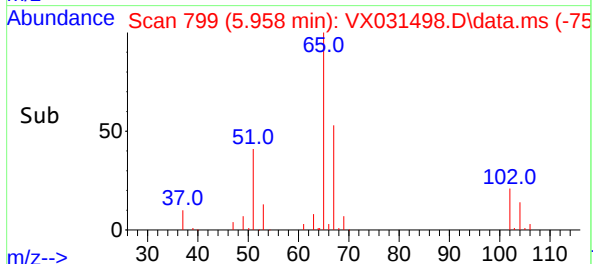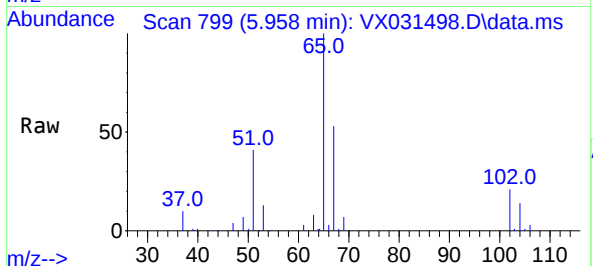

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 114 Resp: 95086
Ion Ratio Lower Upper
114 100
63 18.7 0.0 42.6
88 14.1 0.0 33.0

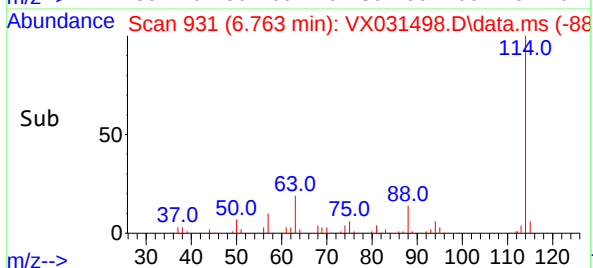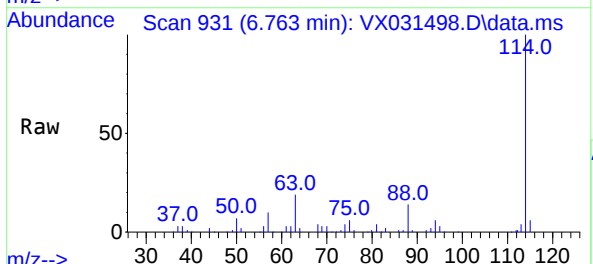

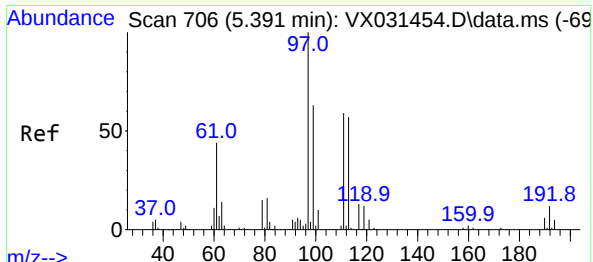

#35

Dibromofluoromethane

Concen: 50.602 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX031498.D


Acq: 20 Sep 2022 16:10

Instrument :

MSVOA_X

ClientSampleId :

COMP-1ME

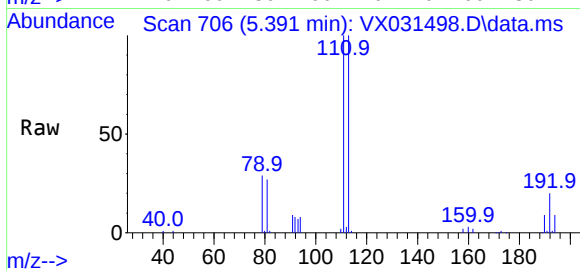




Tgt Ion:113 Resp: 49724

Ion Ratio Lower Upper

113 100

111 100.9 82.4 123.6

192 19.3 14.1 21.1

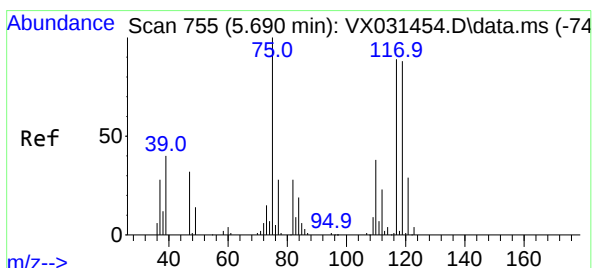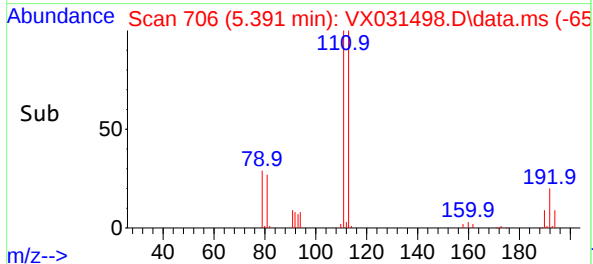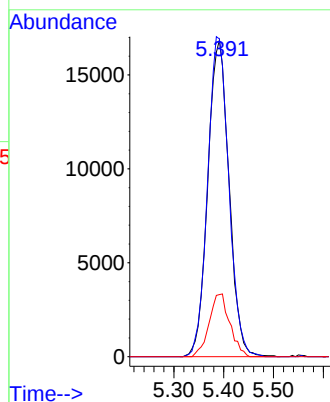

#36

1,1-Dichloropropene

Concen: 3.405 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.146 min

Lab File: VX031498.D

Acq: 20 Sep 2022 16:10




Tgt Ion: 75 Resp: 5146


Ion Ratio Lower Upper

75 100

110 7.3 17.5 52.5#

77 0.0 24.9 37.3#


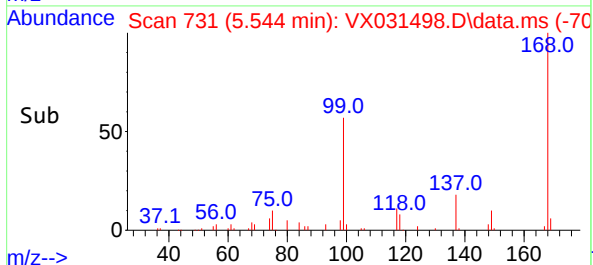

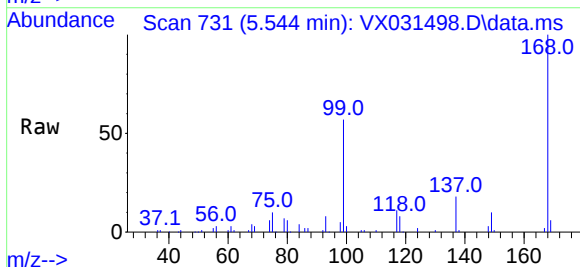




#37
Ethyl Acetate
Concen: 4.740 ug/l
RT: 4.617 min Scan# 51
Delta R.T. -0.104 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 43 Resp: 8546
Ion Ratio Lower Upper
43 100
61 0.0 11.1 16.7#
70 0.0 8.6 13.0#



#38
Carbon Tetrachloride
Concen: 3.771 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.134 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 117 Resp: 6318
Ion Ratio Lower Upper
117 100
119 3.5 74.6 112.0#
121 0.0 25.3 37.9#


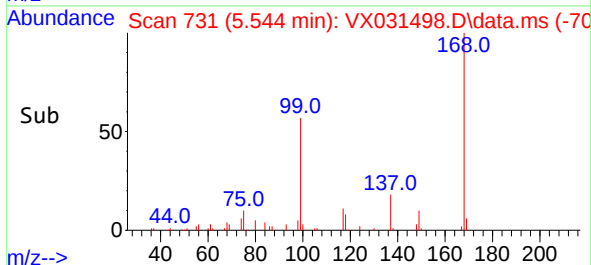

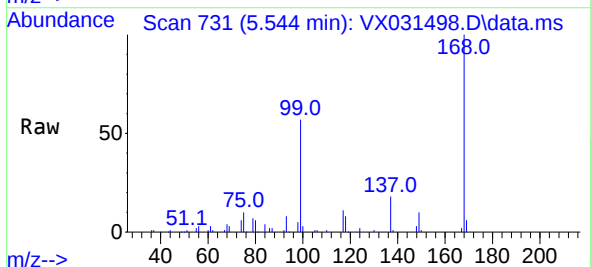




#40
Benzene
Concen: 0.499 ug/l
RT: 6.038 min Scan# 81
Delta R.T. -0.006 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 78 Resp: 2248
Ion Ratio Lower Upper
78 100
77 19.7 18.7 28.1



#41
Methacrylonitrile
Concen: 0.360 ug/l
RT: 5.050 min Scan# 650
Delta R.T. 0.122 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 41 Resp: 323
Ion Ratio Lower Upper
41 100
39 67.2 45.0 67.6
67 0.0 58.2 87.4#
52 0.0 25.0 37.6#


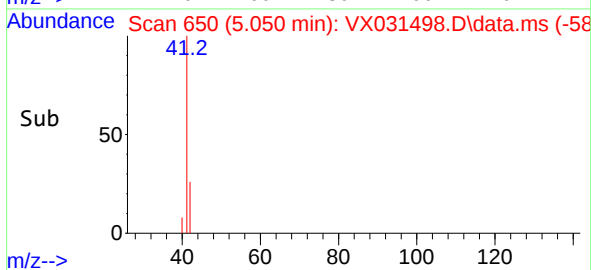






#43
Isopropyl Acetate
Concen: 0.665 ug/l
RT: 6.367 min Scan# 866
Delta R.T. 0.025 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 43 Resp: 1842
Ion Ratio Lower Upper
43 100
61 0.0 15.3 22.9#
87 0.0 10.6 15.8#

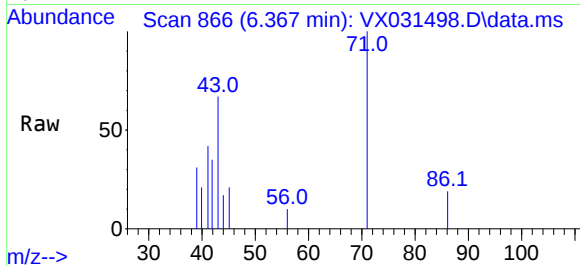

#50
Toluene-d8
Concen: 51.034 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 98 Resp: 193334
Ion Ratio Lower Upper
98 100
100 63.8 52.5 78.7

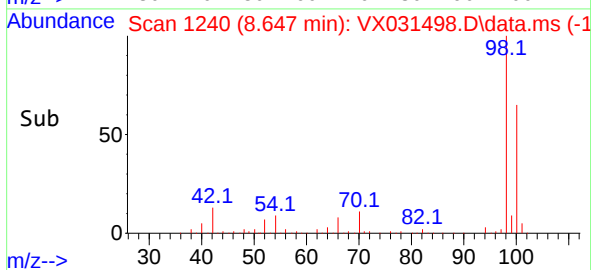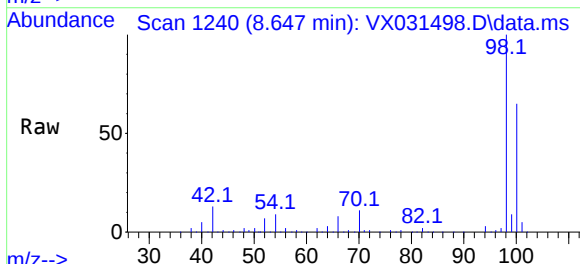

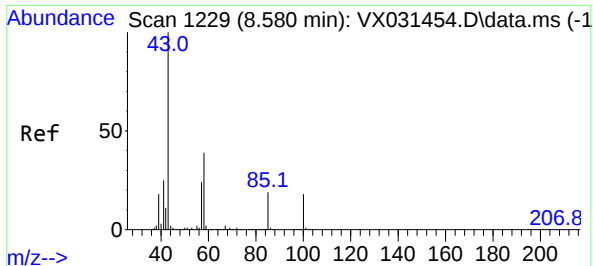

#51

4-Methyl-2-Pentanone

Concen: 0.553 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.067 min

Lab File: VX031498.D

Acq: 20 Sep 2022 16:10

Instrument :

MSVOA_X

ClientSampleId :


COMP-1ME

Tgt Ion: 43 Resp: 986




Ion Ratio Lower Upper

43 100

58 150.9 30.6 46.0#

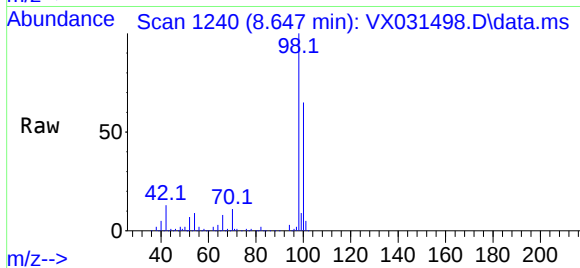

Abundance

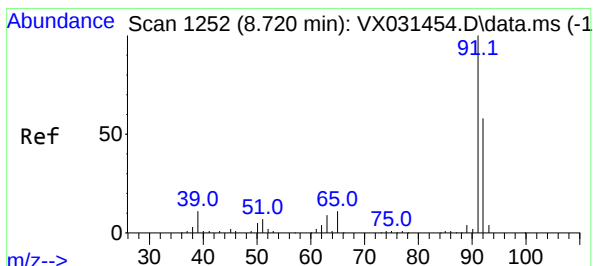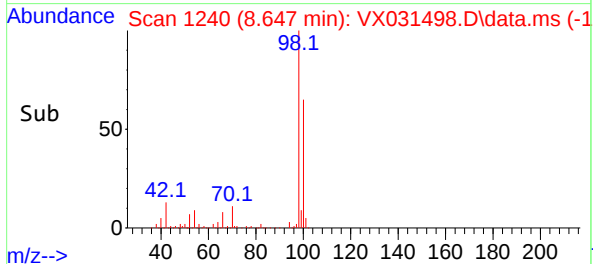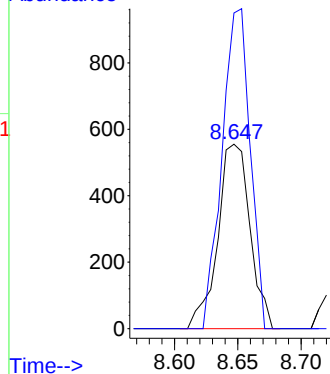

#52

Toluene

Concen: 3.342 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX031498.D


Acq: 20 Sep 2022 16:10

Tgt Ion: 92 Resp: 9828



Ion Ratio Lower Upper


92 100

91 171.1 137.1 205.7

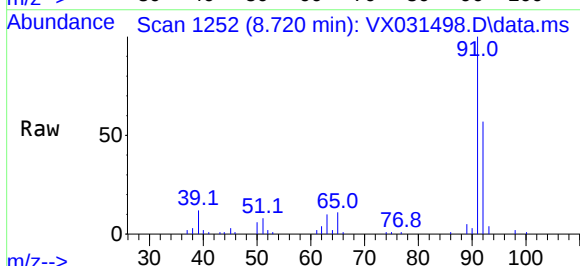

Abundance



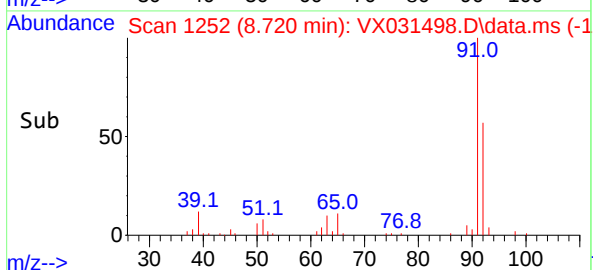
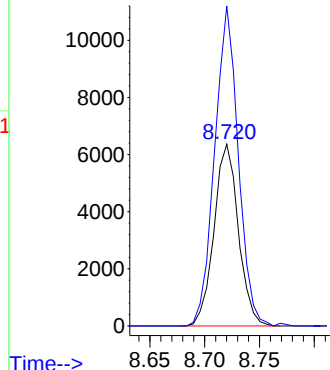




#62
4-Bromofluorobenzene
Concen: 44.631 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 95 Resp: 57271
Ion Ratio Lower Upper
95 100
174 87.6 0.0 153.2
176 86.5 0.0 144.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 117 Resp: 97823
Ion Ratio Lower Upper
117 100
82 53.5 46.8 70.2
119 32.0 26.4 39.6



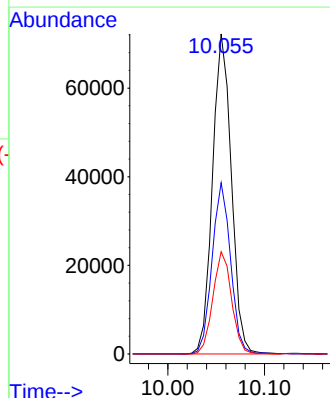





#67
Ethyl Benzene
Concen: 7.108 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument : MSVOA_X
ClientSampleId : COMP-1ME


Tgt Ion: 91 Resp: 37858
Ion Ratio Lower Upper
91 100
106 30.6 25.2 37.8

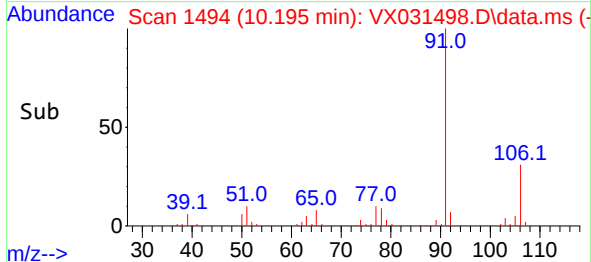

#68
m/p-Xylenes
Concen: 8.534 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 106 Resp: 18267
Ion Ratio Lower Upper
106 100
91 200.1 161.0 241.4


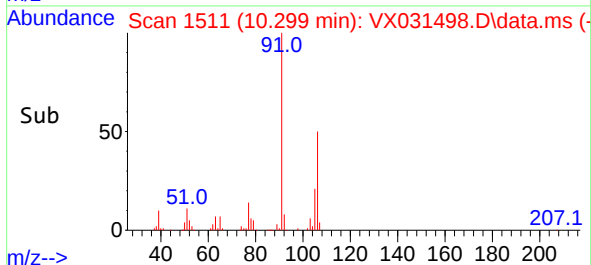
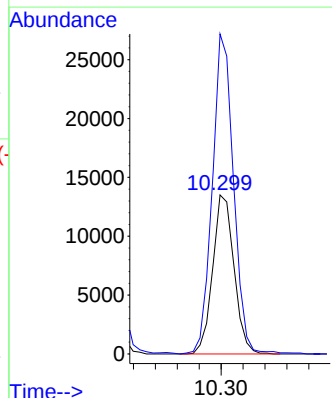
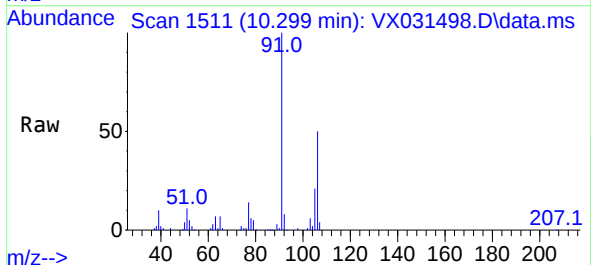




#69
o-Xylene
Concen: 4.960 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.001 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion:106 Resp: 10134
Ion Ratio Lower Upper
106 100
91 215.2 107.2 321.6

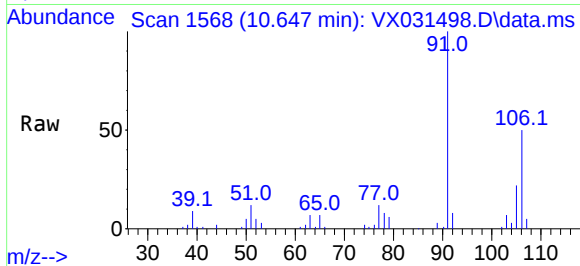

#70
Styrene
Concen: 0.381 ug/l
RT: 10.653 min Scan# 1569
Delta R.T. -0.006 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion:104 Resp: 1281
Ion Ratio Lower Upper
104 100
78 146.4 41.4 62.2#
103 142.7 43.8 65.8#


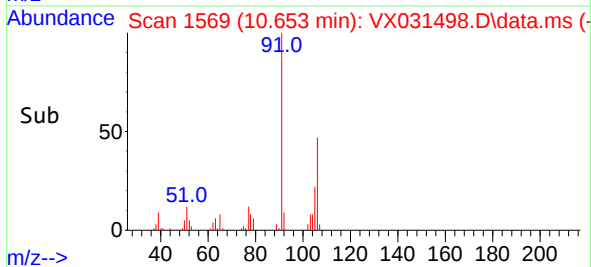

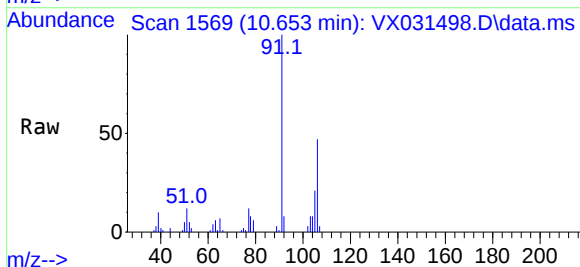




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion:152 Resp: 66348
Ion Ratio Lower Upper
152 100
115 56.0 43.4 130.1
150 157.0 0.0 346.8

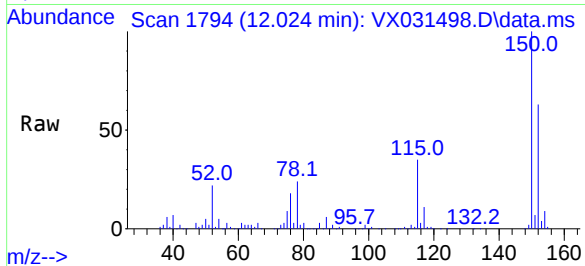

#73
Isopropylbenzene
Concen: 1.221 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.001 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion:105 Resp: 6050
Ion Ratio Lower Upper
105 100
120 25.6 13.7 41.0


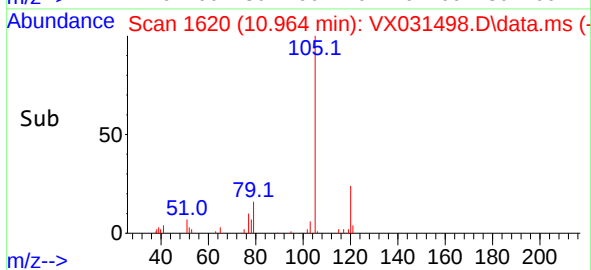

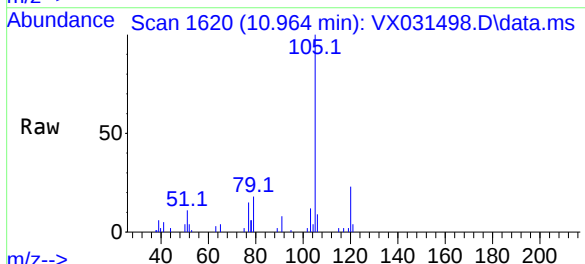




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 11.079 min Scan# 1639
Delta R.T. -0.134 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 83 Resp: 144
Ion Ratio Lower Upper
83 100
131 47.2 5.1 15.4#
85 0.0 32.6 97.8#

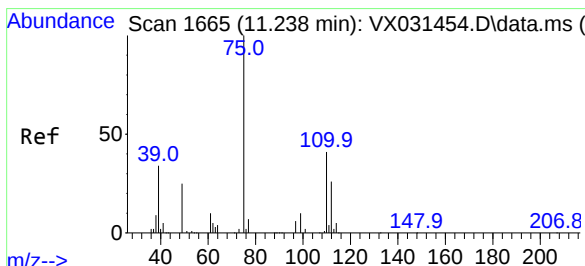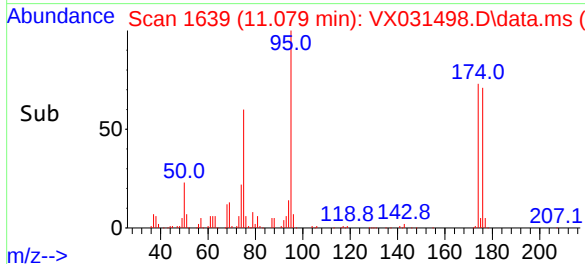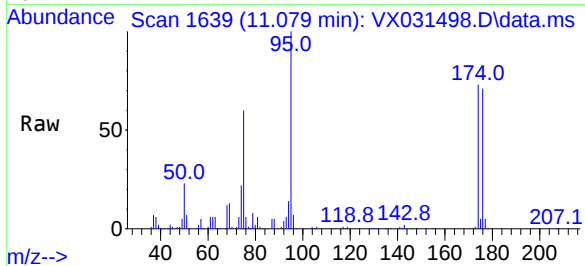

#76
1,2,3-Trichloropropane
Concen: 22.675 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.153 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 75 Resp: 33577
Ion Ratio Lower Upper
75 100
77 1.2 20.3 60.9#


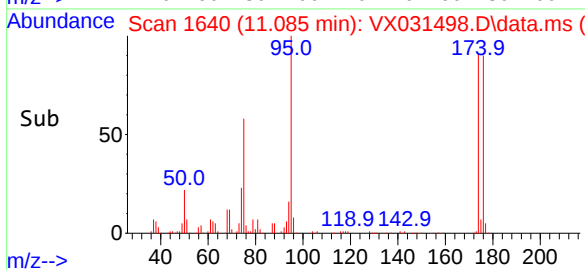

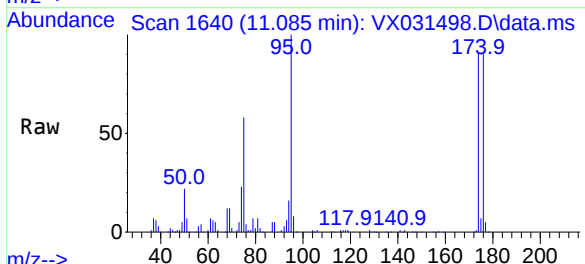




#78
n-propylbenzene
Concen: 0.479 ug/l
RT: 11.305 min Scan# 1727
Delta R.T. -0.000 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 91 Resp: 2731
Ion Ratio Lower Upper
91 100
120 20.6 11.8 35.4

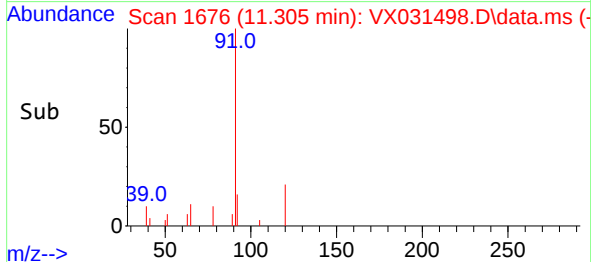

#79
2-Chlorotoluene
Concen: 0.262 ug/l
RT: 11.616 min Scan# 1727
Delta R.T. 0.250 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 91 Resp: 890
Ion Ratio Lower Upper
91 100
126 22.1 17.4 52.3


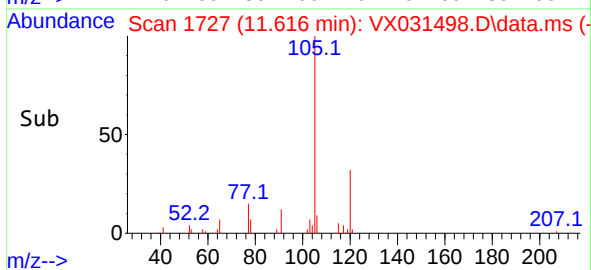






#80
1,3,5-Trimethylbenzene
Concen: 3.206 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion:105 Resp: 13479
Ion Ratio Lower Upper
105 100
120 48.0 24.5 73.5

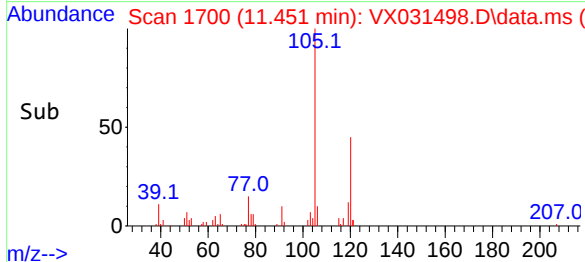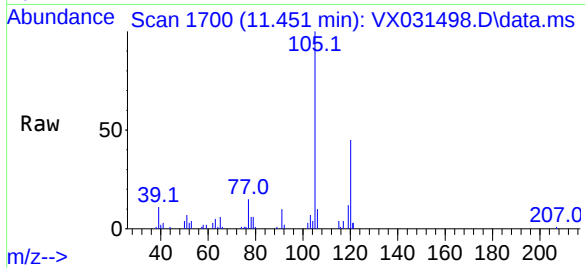

#81
trans-1,4-Dichloro-2-butene
Concen: 73.009 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 75 Resp: 33577
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#


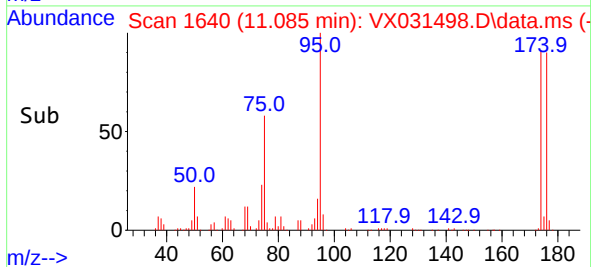

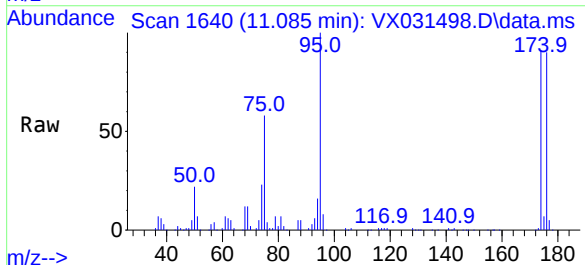




#82
4-Chlorotoluene
Concen: 0.263 ug/l
RT: 11.616 min Scan# 1701
Delta R.T. 0.159 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion: 91 Resp: 1047
Ion Ratio Lower Upper
91 100
126 21.5 15.1 45.3

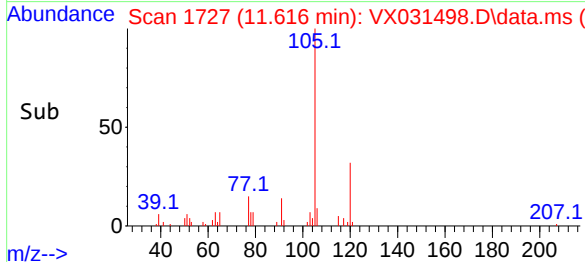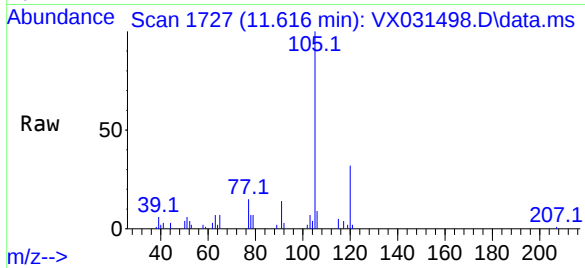

#83
tert-Butylbenzene
Concen: 1.395 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion: 119 Resp: 5685
Ion Ratio Lower Upper
119 100
91 98.1 29.2 87.6#
134 0.0 11.6 34.8#


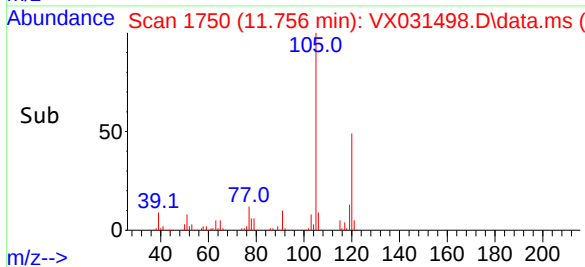

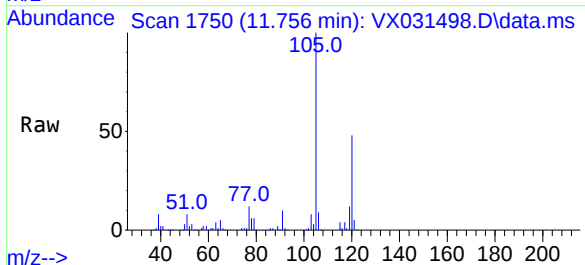




#84
1,2,4-Trimethylbenzene
Concen: 10.560 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion:105 Resp: 43727
Ion Ratio Lower Upper
105 100
120 47.2 22.6 67.8



#85
sec-Butylbenzene
Concen: 8.478 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion:105 Resp: 43727
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#




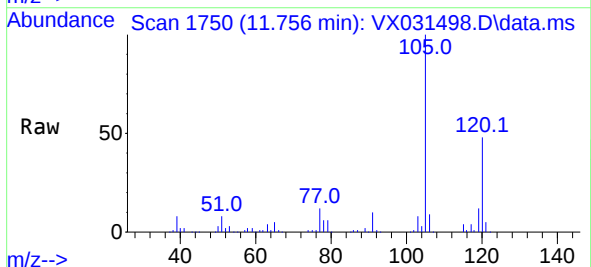




#86
p-Isopropyltoluene
Concen: 0.879 ug/l
RT: 12.012 min Scan# 119
Delta R.T. 0.000 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion:	119	Resp:	3826
Ion	Ratio	Lower	Upper
119	100		
134	29.3	13.4	40.2
91	35.1	12.4	37.2

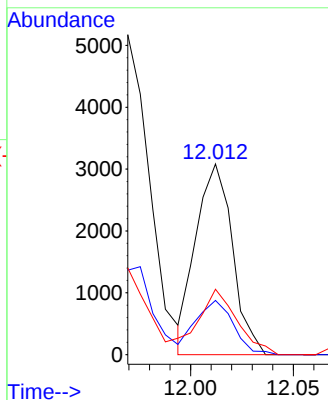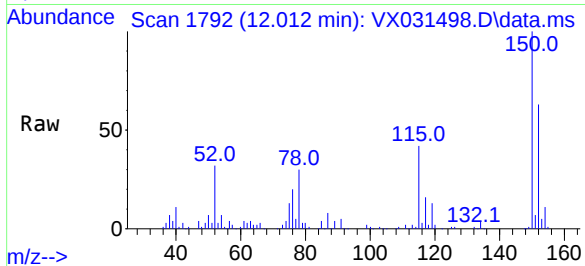

#89
n-Butylbenzene
Concen: 0.660 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Tgt Ion:	91	Resp:	2450
Ion	Ratio	Lower	Upper
91	100		
92	30.4	27.0	81.0
134	117.7	13.3	39.9#



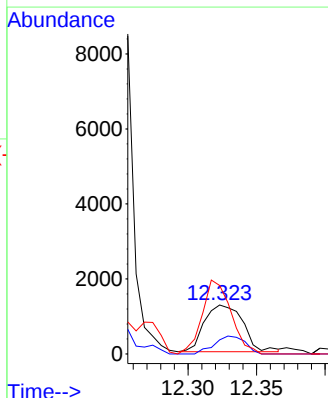
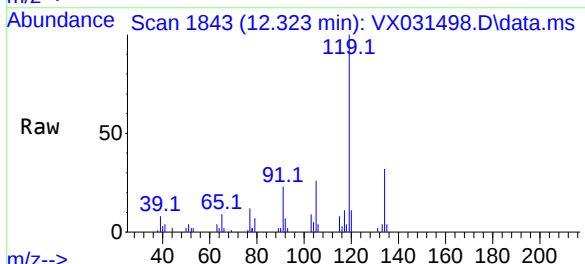




#90
Hexachloroethane
Concen: 8.611 ug/l
RT: 12.414 min Scan# 117
Delta R.T. -0.128 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10




Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME


Tgt Ion:117 Resp: 6444
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

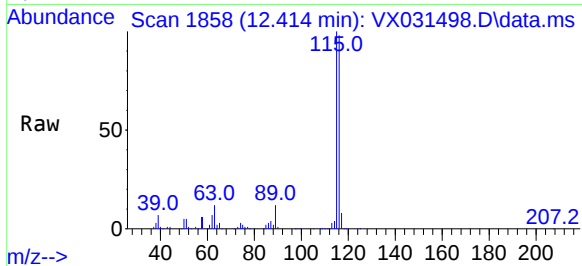

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.637 ug/l
RT: 12.969 min Scan# 1949
Delta R.T. 0.024 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10


Tgt Ion: 75 Resp: 217
Ion Ratio Lower Upper
75 100
155 0.0 40.3 120.8#
157 0.0 51.5 154.5#

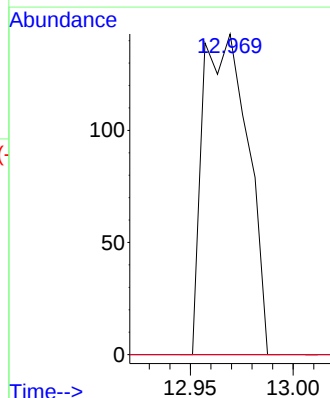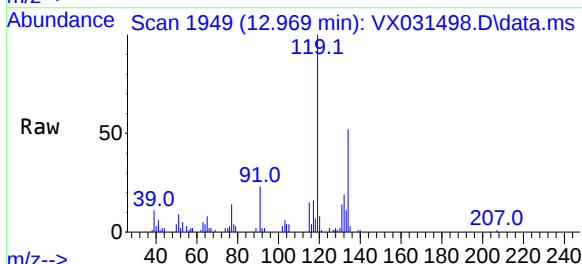



#95
Naphthalene
Concen: 626.077 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX031498.D
Acq: 20 Sep 2022 16:10

Instrument :
MSVOA_X
ClientSampleId :
COMP-1ME



Tgt Ion:128 Resp: 2977853
Ion Ratio Lower Upper
128 100
127 13.7 10.4 15.6
129 11.6 8.8 13.2

