

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092022\
 Data File : VX031499.D
 Acq On : 20 Sep 2022 16:33
 Operator : JC/MD
 Sample : N4665-02ME 2X
 Misc : 5.03G/10mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-2ME

Quant Time: Sep 20 17:55:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 09:45:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	68343	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	105229	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	112384	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	78237	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	61292	48.785	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.560%
35) Dibromofluoromethane	5.391	113	48569	44.576	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	89.160%
50) Toluene-d8	8.647	98	187510	44.726	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.460%
62) 4-Bromofluorobenzene	11.085	95	59297	41.756	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	83.520%
Target Compounds						Qvalue
5) Bromomethane	1.605	94	1209	0.571	ug/l	100
6) Chloroethane	1.691	64	34	Below Cal	#	1
10) Methyl Iodide	2.440	142	236	0.222	ug/l	# 48
11) Tert butyl alcohol	2.953	59	6010	Below Cal	#	73
13) Acrolein	2.209	56	44	Below Cal	#	1
16) Acetone	2.404	43	682	Below Cal		94
20) Methylene Chloride	2.782	84	1088	Below Cal	#	86
25) 2-Butanone	4.586	43	4173	4.313	ug/l	96
31) Cyclohexane	5.544	56	1595	0.858	ug/l	# 21
36) 1,1-Dichloropropene	5.550	75	5447	3.257	ug/l	# 45
38) Carbon Tetrachloride	5.550	117	7110	3.835	ug/l	# 17
40) Benzene	6.043	78	1660	0.333	ug/l	# 75
43) Isopropyl Acetate	6.354	43	832	0.271	ug/l	# 61
51) 4-Methyl-2-Pentanone	8.653	43	863	0.437	ug/l	# 1
52) Toluene	8.720	92	17695	5.437	ug/l	99
67) Ethyl Benzene	10.195	91	102075	16.681	ug/l	100
68) m/p-Xylenes	10.305	106	52799	21.471	ug/l	99
69) o-Xylene	10.646	106	33637	14.331	ug/l	97
70) Styrene	10.659	104	4040	1.045	ug/l	# 1
73) Isopropylbenzene	10.963	105	18800	3.218	ug/l	100
75) 1,1,2,2-Tetrachloroethane	11.225	83	151	Below Cal	#	71
76) 1,2,3-Trichloropropane	11.378	75	1820	1.042	ug/l	# 1
78) n-propylbenzene	11.305	91	8178	1.217	ug/l	99
79) 2-Chlorotoluene	11.378	91	23116	5.778	ug/l	# 40
80) 1,3,5-Trimethylbenzene	11.451	105	51228	10.332	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.085	75	33704	62.149	ug/l	# 11
82) 4-Chlorotoluene	11.451	91	6091	1.297	ug/l	# 44
83) tert-Butylbenzene	11.756	119	21491	4.472	ug/l	# 48
84) 1,2,4-Trimethylbenzene	11.756	105	165281	33.848	ug/l	98
85) sec-Butylbenzene	11.756	105	165281	27.177	ug/l	# 56
86) p-Isopropyltoluene	12.012	119	15008	2.922	ug/l	94
89) n-Butylbenzene	12.323	91	11235	2.568	ug/l	# 12
90) Hexachloroethane	12.414	117	24109	27.321	ug/l	# 15
92) 1,2-Dibromo-3-Chloropr...	12.963	75	757	1.886	ug/l	# 11
95) Naphthalene	13.786	128	11763004	2097.291	ug/l	# 84

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092022\
Data File : VX031499.D
Acq On : 20 Sep 2022 16:33
Operator : JC/MD
Sample : N4665-02ME 2X
Misc : 5.03G/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Quant Time: Sep 20 17:55:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 20 17:55:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion:168 Resp: 68343
Ion Ratio Lower Upper
168 100
99 50.2 48.8 73.2

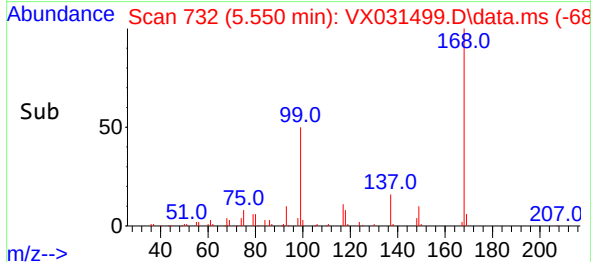

#5
Bromomethane
Concen: 0.571 ug/l
RT: 1.605 min Scan# 85
Delta R.T. -0.006 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 94 Resp: 1209
Ion Ratio Lower Upper
94 100
96 93.1 74.4 111.6


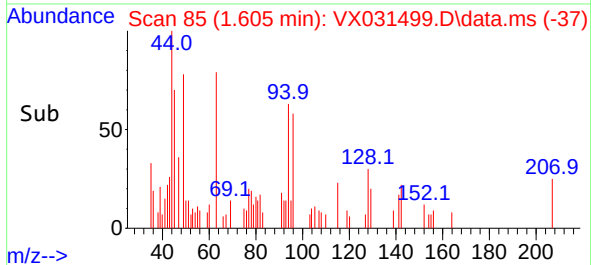

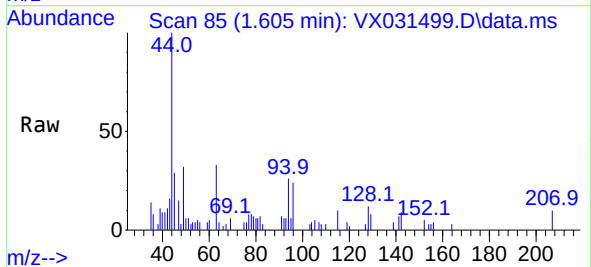


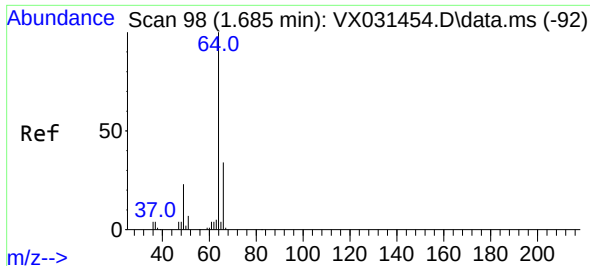

#6
Chloroethane
Concen: Below Cal
RT: 1.691 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 64 Resp: 34
Ion Ratio Lower Upper
64 100
66 226.3 25.0 37.4#

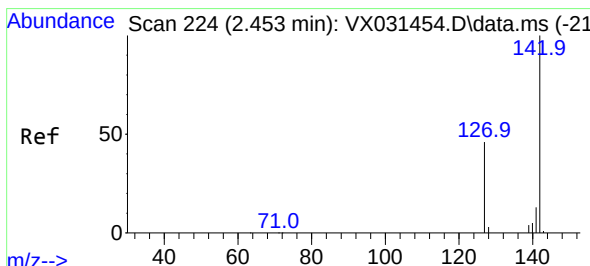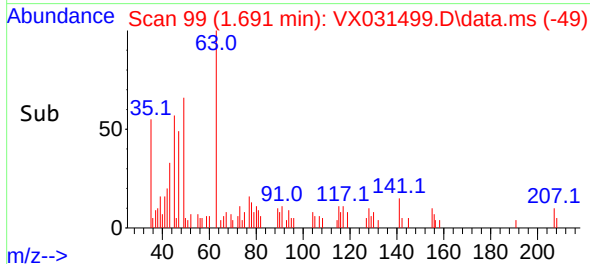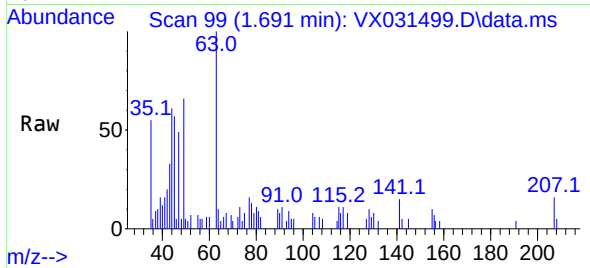

#10
Methyl Iodide
Concen: 0.222 ug/l
RT: 2.440 min Scan# 222
Delta R.T. -0.013 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 142 Resp: 236
Ion Ratio Lower Upper
142 100
127 8.5 37.4 56.0#
141 0.0 11.6 17.4#


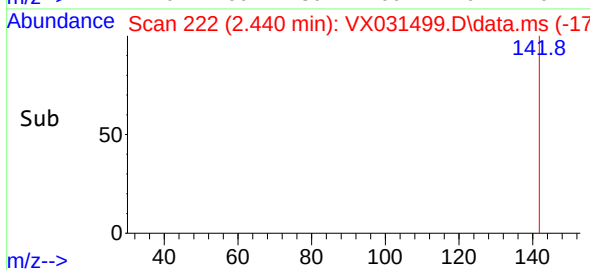

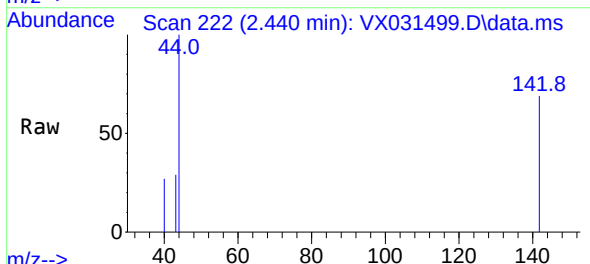




#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.953 min Scan# 306
Delta R.T. -0.036 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 59 Resp: 6010
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

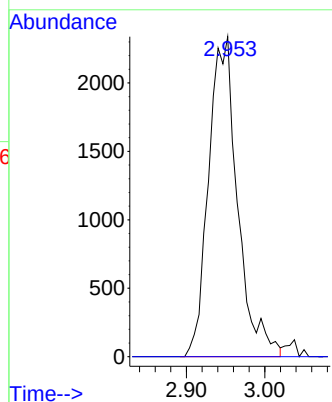

#13
Acrolein
Concen: Below Cal
RT: 2.209 min Scan# 184
Delta R.T. -0.030 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 56 Resp: 44
Ion Ratio Lower Upper
56 100
55 181.8 56.0 84.0#


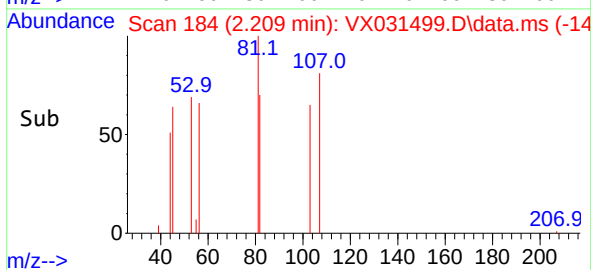






#16
Acetone
Concen: Below Cal
RT: 2.404 min Scan# 21
Delta R.T. 0.018 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 43 Resp: 682
Ion Ratio Lower Upper
43 100
58 26.3 23.8 35.8



#20
Methylene Chloride
Concen: Below Cal
RT: 2.782 min Scan# 278
Delta R.T. -0.006 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 84 Resp: 1088
Ion Ratio Lower Upper
84 100
49 120.1 105.9 158.9
51 25.3 32.2 48.2#
86 52.4 50.8 76.2

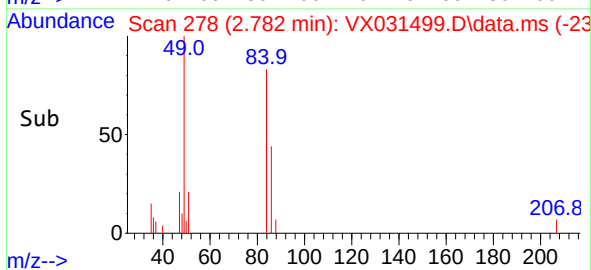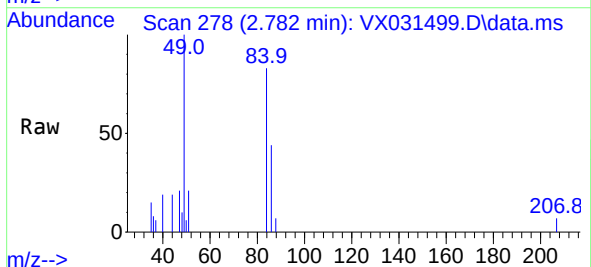

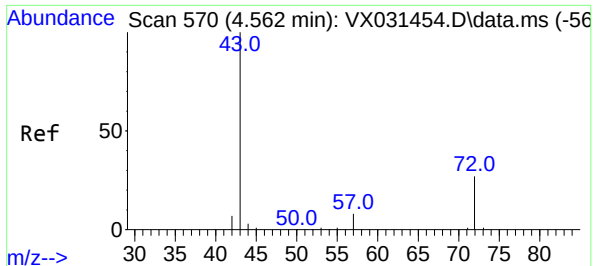

#25

2-Butanone

Concen: 4.313 ug/l

RT: 4.586 min Scan# 51

Delta R.T. 0.024 min

Lab File: VX031499.D

Acq: 20 Sep 2022 16:33

Instrument :

MSVOA_X

ClientSampleId :





COMP-2ME

Tgt Ion: 43 Resp: 4173

Ion Ratio Lower Upper

43 100

72 28.2 21.1 31.7

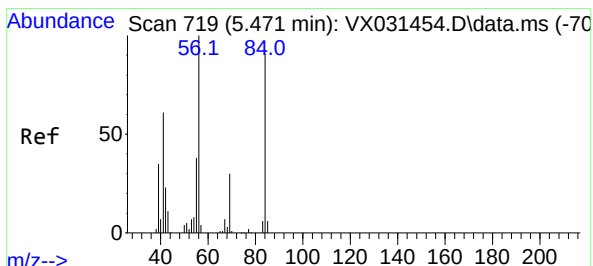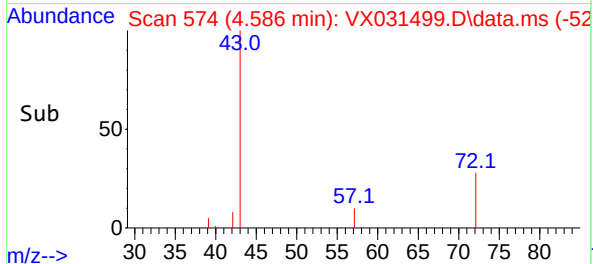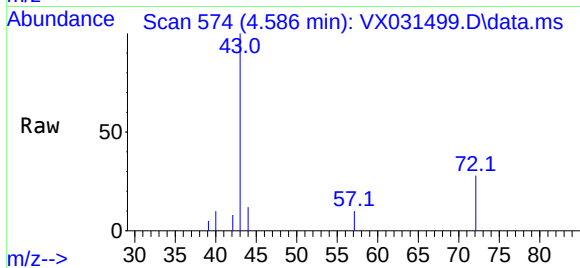

#31

Cyclohexane

Concen: 0.858 ug/l

RT: 5.544 min Scan# 731

Delta R.T. 0.073 min

Lab File: VX031499.D

Acq: 20 Sep 2022 16:33




Tgt Ion: 56 Resp: 1595


Ion Ratio Lower Upper

56 100

69 123.2 25.1 37.7#

84 132.2 70.2 105.4#


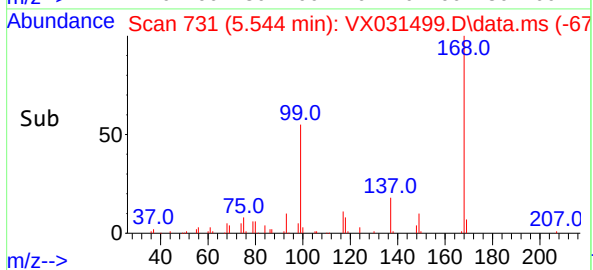

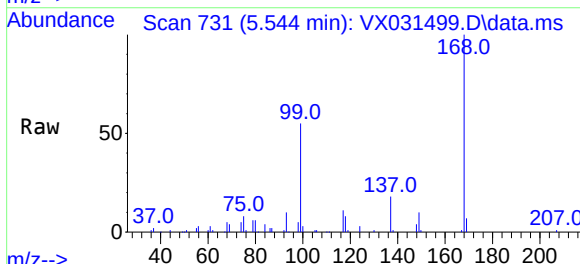


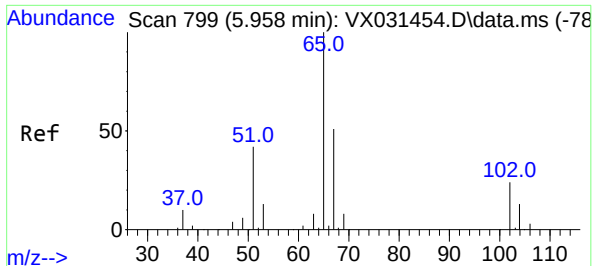

#33
1,2-Dichloroethane-d4
Concen: 48.785 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 65 Resp: 61292
Ion Ratio Lower Upper
65 100
67 50.8 0.0 102.4

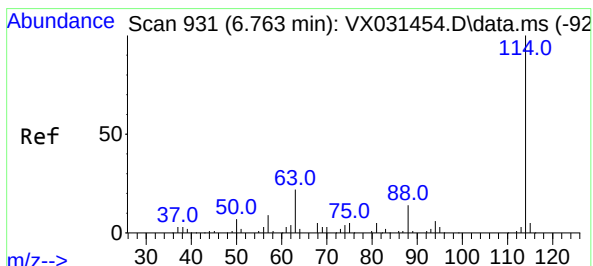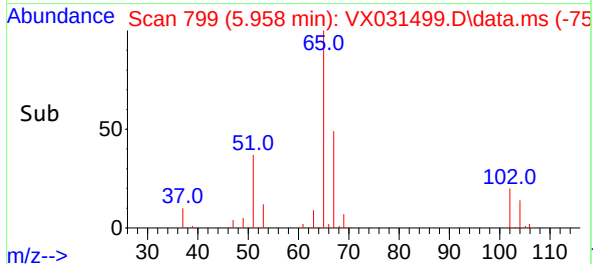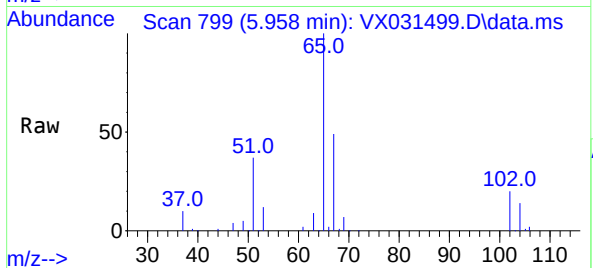

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33


Tgt Ion: 114 Resp: 105229
Ion Ratio Lower Upper
114 100
63 17.3 0.0 42.6
88 13.9 0.0 33.0

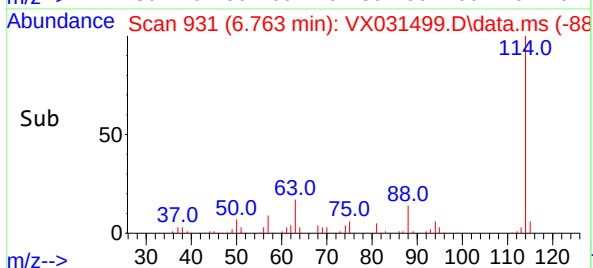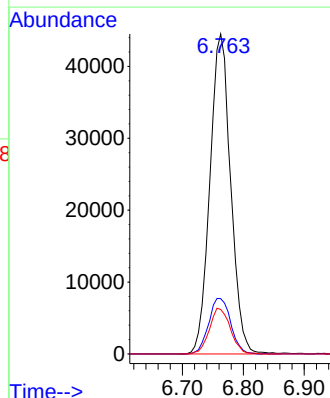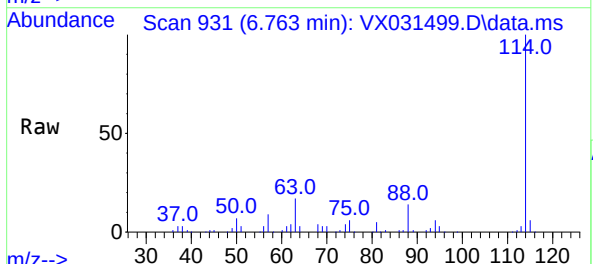



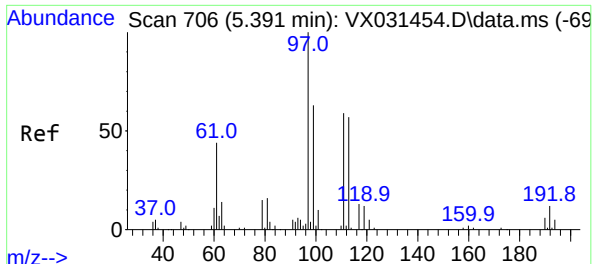


#35
Dibromofluoromethane
Concen: 44.576 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33


Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME

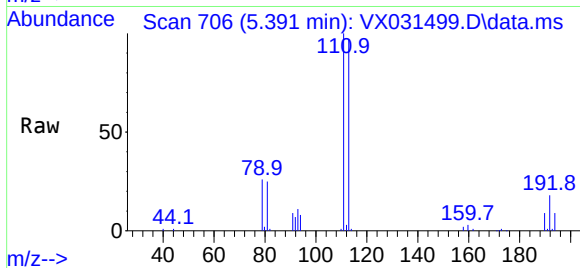



Tgt Ion:113 Resp: 48569
Ion Ratio Lower Upper
113 100
111 103.0 82.4 123.6
192 19.0 14.1 21.1

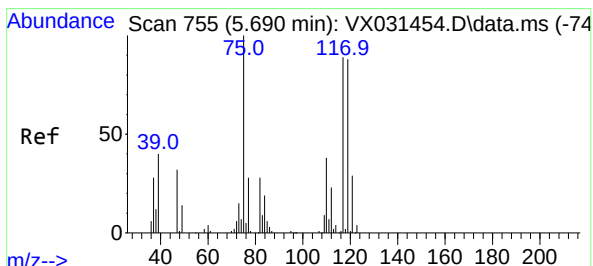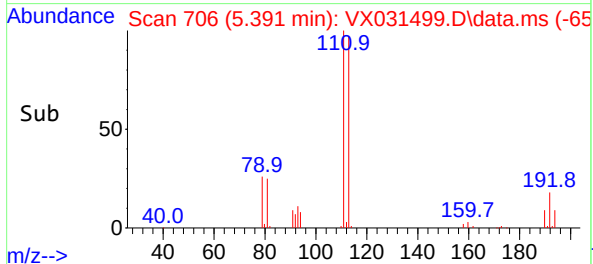


#36
1,1-Dichloropropene
Concen: 3.257 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

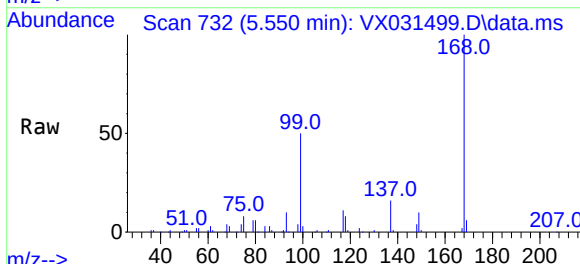

Tgt Ion: 75 Resp: 5447
Ion Ratio Lower Upper
75 100
110 3.4 17.5 52.5#
77 0.0 24.9 37.3#



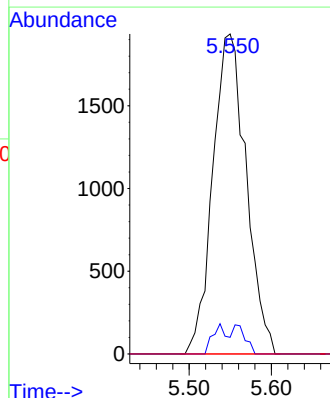
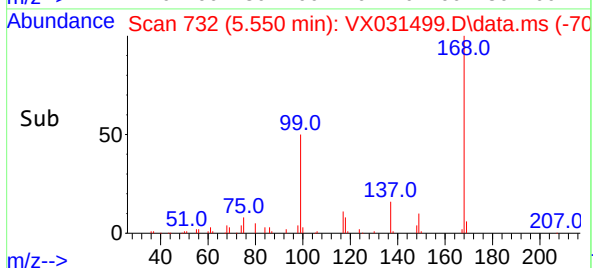




#38
Carbon Tetrachloride
Concen: 3.835 ug/l
RT: 5.550 min Scan# 7110
Delta R.T. -0.128 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion:117 Resp: 7110
Ion Ratio Lower Upper
117 100
119 5.0 74.6 112.0#
121 0.0 25.3 37.9#

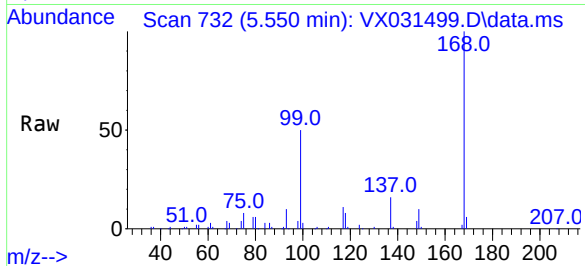

#40
Benzene
Concen: 0.333 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.001 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 78 Resp: 1660
Ion Ratio Lower Upper
78 100
77 35.4 18.7 28.1#


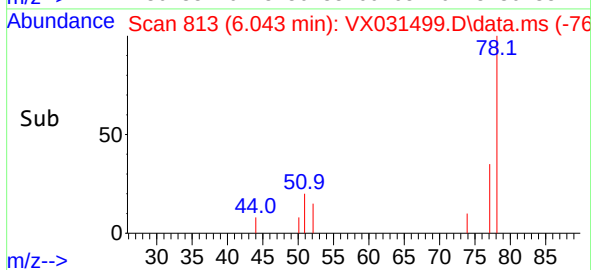

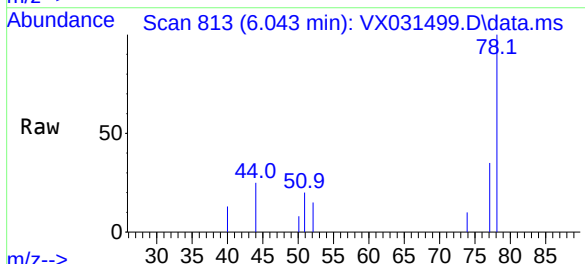


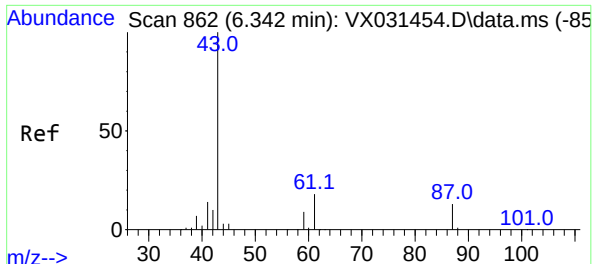

#43
Isopropyl Acetate
Concen: 0.271 ug/l
RT: 6.354 min Scan# 80
Delta R.T. 0.012 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 43 Resp: 832
Ion Ratio Lower Upper
43 100
61 0.0 15.3 22.9#
87 0.0 10.6 15.8#

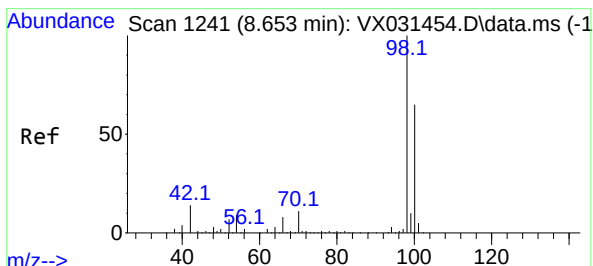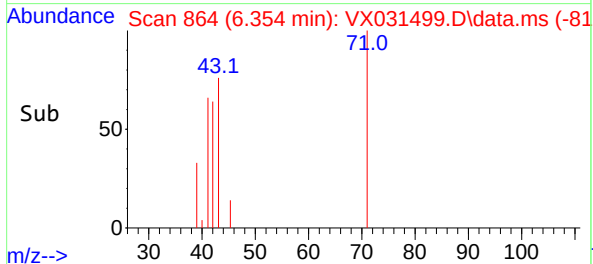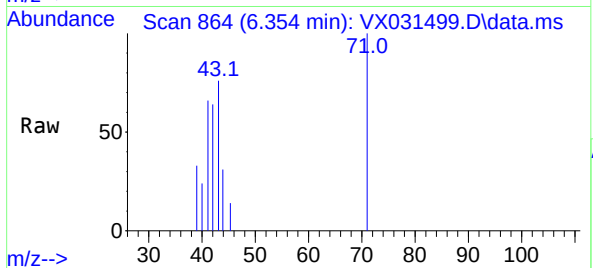

#50
Toluene-d8
Concen: 44.726 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 98 Resp: 187510
Ion Ratio Lower Upper
98 100
100 64.5 52.5 78.7

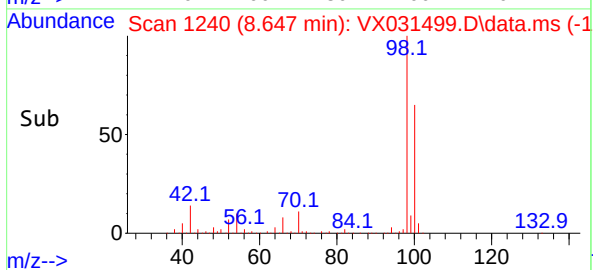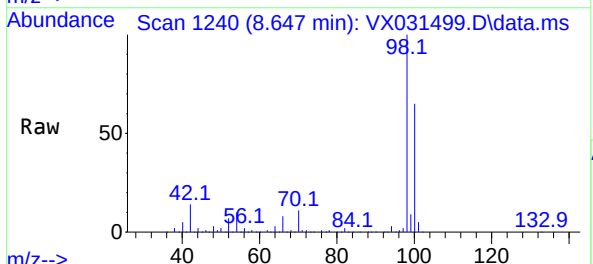



#51

4-Methyl-2-Pentanone

Concen: 0.437 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.073 min

Lab File: VX031499.D

Acq: 20 Sep 2022 16:33

Instrument :

MSVOA_X

ClientSampleId :





COMP-2ME

Tgt Ion: 43 Resp: 863

Ion Ratio Lower Upper

43 100

58 181.9 30.6 46.0#

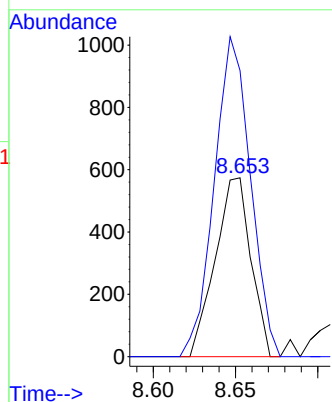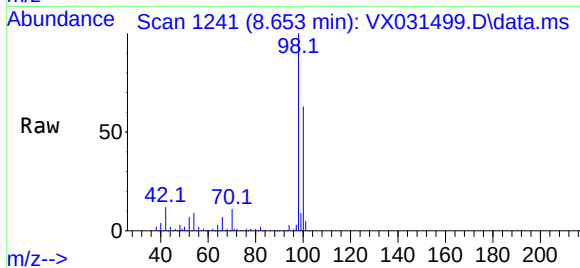

#52

Toluene

Concen: 5.437 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX031499.D




Acq: 20 Sep 2022 16:33


Tgt Ion: 92 Resp: 17695

Ion Ratio Lower Upper

92 100

91 170.5 137.1 205.7


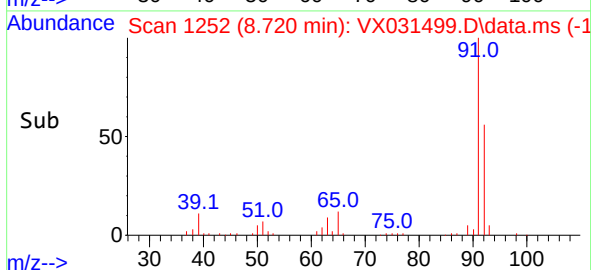

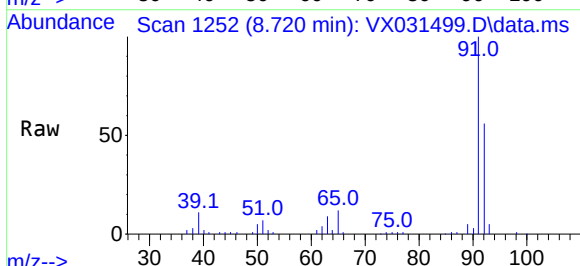




#62
4-Bromofluorobenzene
Concen: 41.756 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 95 Resp: 59297
Ion Ratio Lower Upper
95 100
174 88.7 0.0 153.2
176 85.2 0.0 144.0

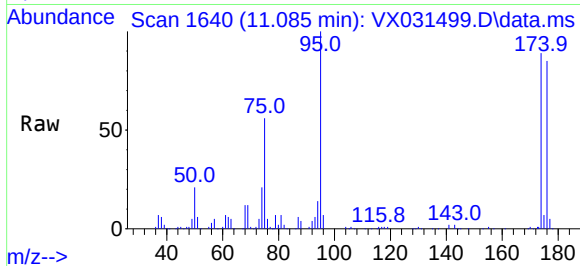

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 117 Resp: 112384
Ion Ratio Lower Upper
117 100
82 52.5 46.8 70.2
119 32.6 26.4 39.6



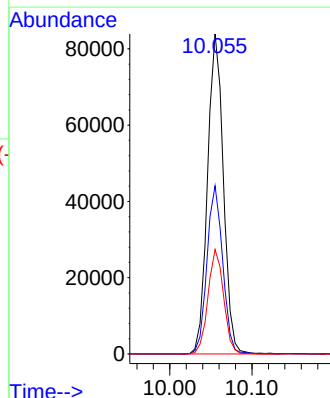
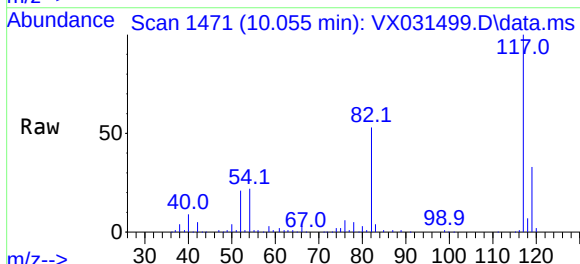




#67
Ethyl Benzene
Concen: 16.681 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 91 Resp: 102075
Ion Ratio Lower Upper
91 100
106 31.8 25.2 37.8

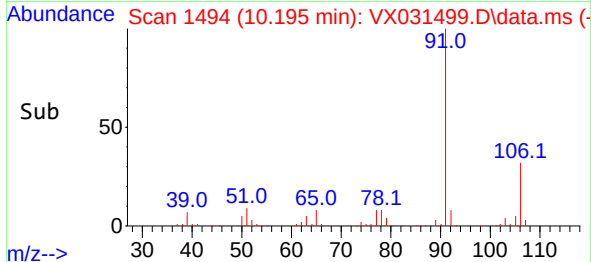

#68
m/p-Xylenes
Concen: 21.471 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 106 Resp: 52799
Ion Ratio Lower Upper
106 100
91 199.7 161.0 241.4


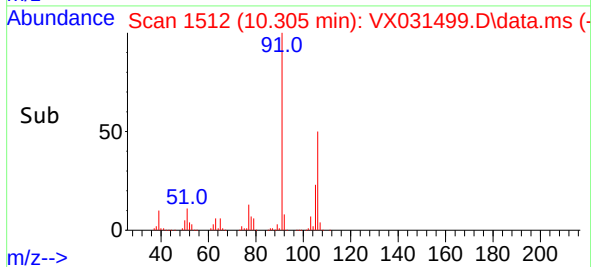

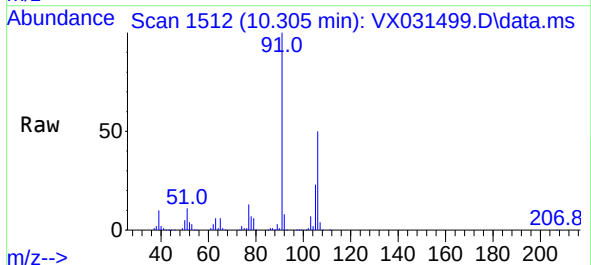




#69
o-Xylene
Concen: 14.331 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion:106 Resp: 33637
Ion Ratio Lower Upper
106 100
91 209.4 107.2 321.6

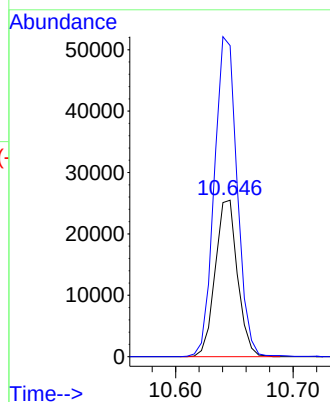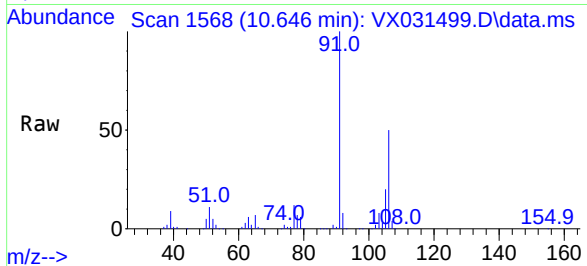

#70
Styrene
Concen: 1.045 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion:104 Resp: 4040
Ion Ratio Lower Upper
104 100
78 149.5 41.4 62.2#
103 142.4 43.8 65.8#


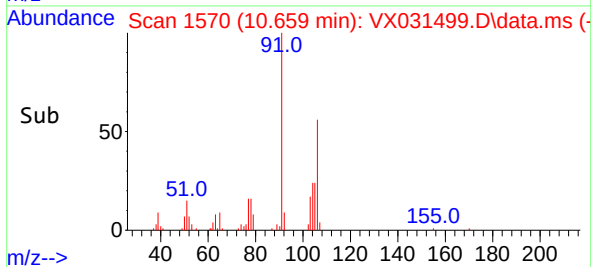

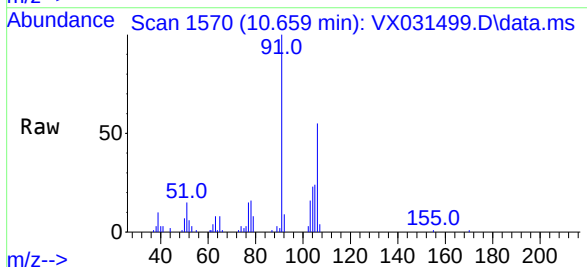




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion:152 Resp: 78237
Ion Ratio Lower Upper
152 100
115 58.7 43.4 130.1
150 154.5 0.0 346.8

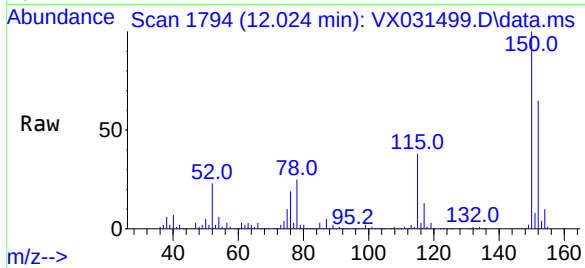

#73
Isopropylbenzene
Concen: 3.218 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion:105 Resp: 18800
Ion Ratio Lower Upper
105 100
120 27.3 13.7 41.0




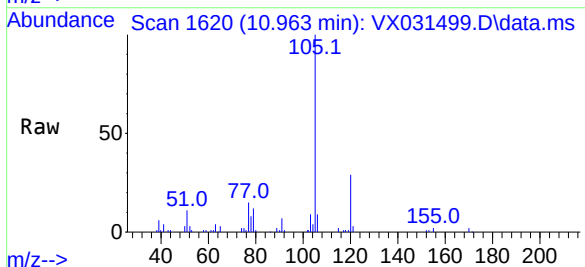




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 11.225 min Scan# 1663
Delta R.T. 0.012 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 83 Resp: 151
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.4#
85 41.7 32.6 97.8

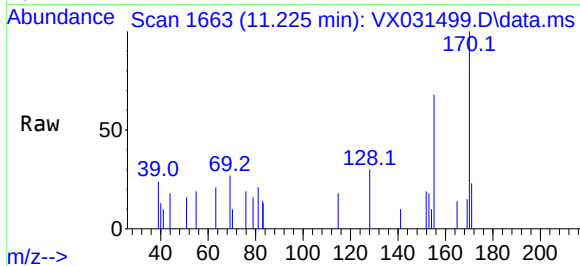

#76
1,2,3-Trichloropropane
Concen: 1.042 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.140 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 75 Resp: 1820
Ion Ratio Lower Upper
75 100
77 1214.5 20.3 60.9#


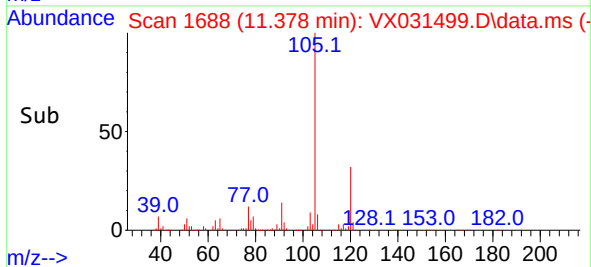

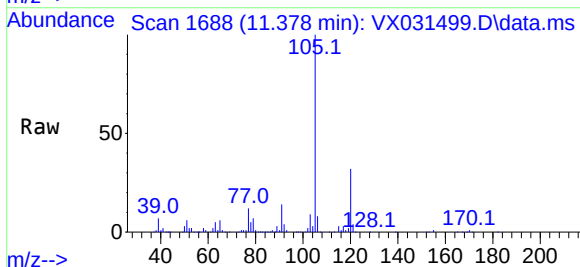




#78
n-propylbenzene
Concen: 1.217 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 91 Resp: 8178
Ion Ratio Lower Upper
91 100
120 23.9 11.8 35.4

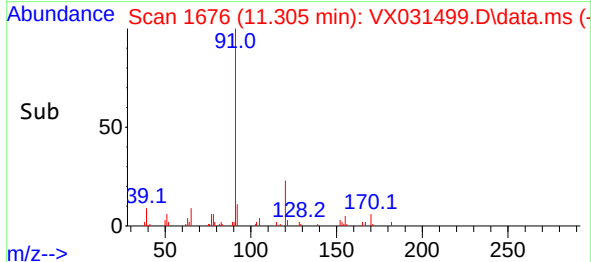

#79
2-Chlorotoluene
Concen: 5.778 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 91 Resp: 23116
Ion Ratio Lower Upper
91 100
126 0.1 17.4 52.3#


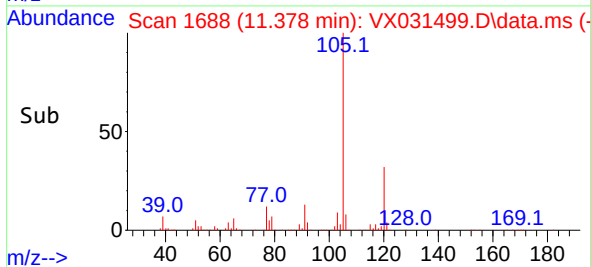

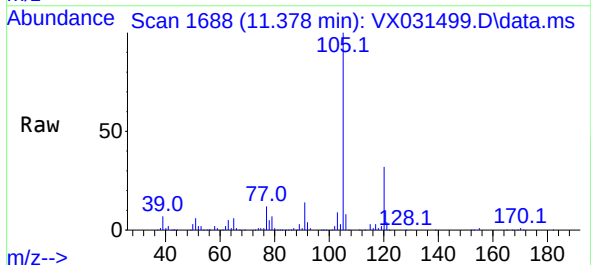




#80
1,3,5-Trimethylbenzene
Concen: 10.332 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion:105 Resp: 51228
Ion Ratio Lower Upper
105 100
120 49.3 24.5 73.5



#81
trans-1,4-Dichloro-2-butene
Concen: 62.149 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 75 Resp: 33704
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.1 37.4 56.0#


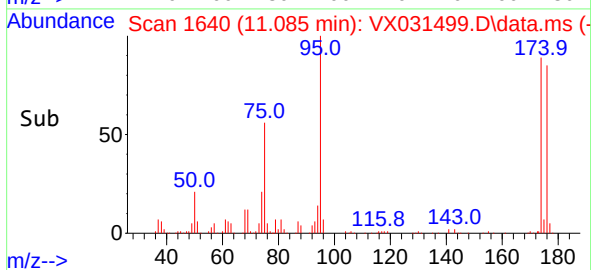






#82
4-Chlorotoluene
Concen: 1.297 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion: 91 Resp: 6091
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#

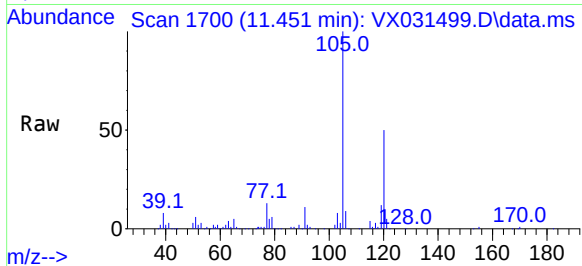

#83
tert-Butylbenzene
Concen: 4.472 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 119 Resp: 21491
Ion Ratio Lower Upper
119 100
91 98.1 29.2 87.6#
134 0.0 11.6 34.8#


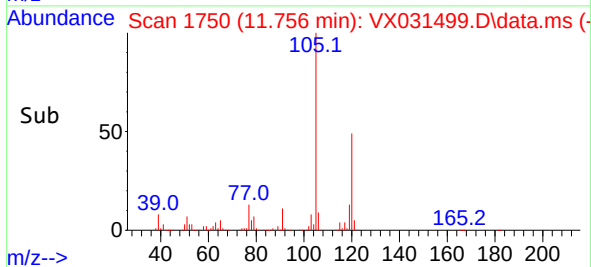

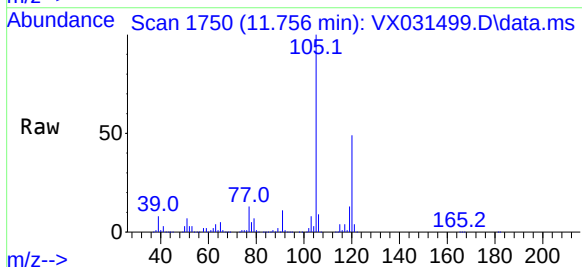




#84
1,2,4-Trimethylbenzene
Concen: 33.848 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion:105 Resp: 165281
Ion Ratio Lower Upper
105 100
120 46.7 22.6 67.8

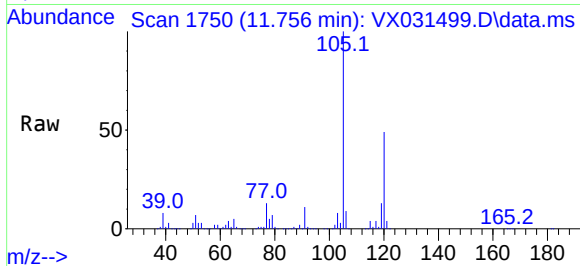

#85
sec-Butylbenzene
Concen: 27.177 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion:105 Resp: 165281
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


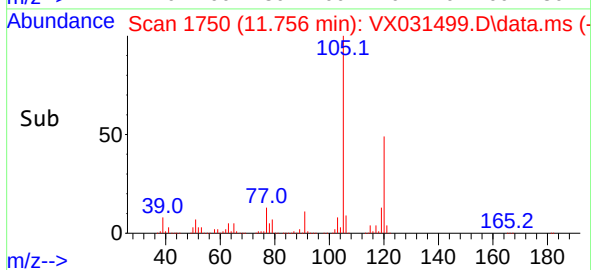

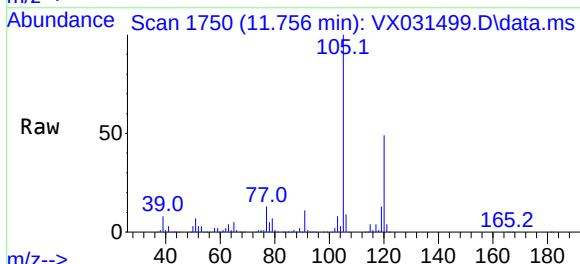




#86
p-Isopropyltoluene
Concen: 2.922 ug/l
RT: 12.012 min Scan# 119
Delta R.T. -0.000 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion:119 Resp: 15008
Ion Ratio Lower Upper
119 100
134 27.1 13.4 40.2
91 30.6 12.4 37.2

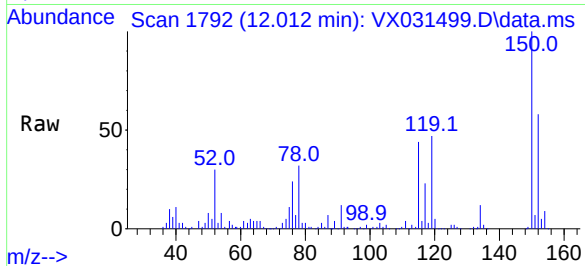

#89
n-Butylbenzene
Concen: 2.568 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Tgt Ion: 91 Resp: 11235
Ion Ratio Lower Upper
91 100
92 28.2 27.0 81.0
134 125.9 13.3 39.9#


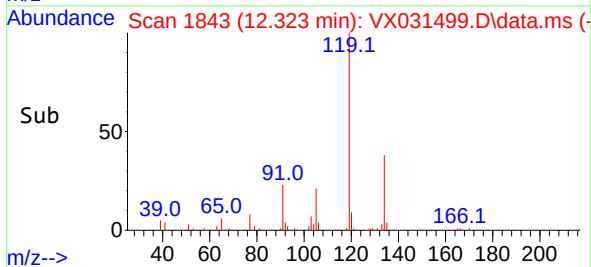

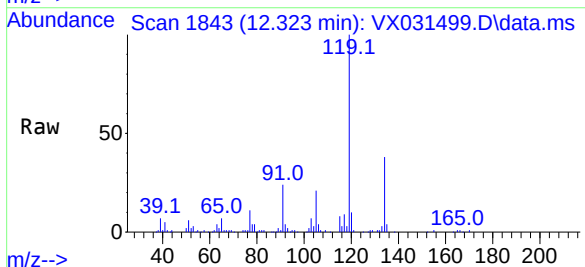




#90
Hexachloroethane
Concen: 27.321 ug/l
RT: 12.414 min Scan# 117
Delta R.T. -0.128 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME


Tgt Ion:117 Resp: 24109
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

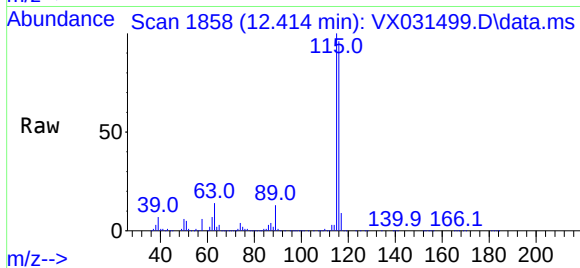

#92
1,2-Dibromo-3-Chloropropane
Concen: 1.886 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33


Tgt Ion: 75 Resp: 757
Ion Ratio Lower Upper
75 100
155 15.7 40.3 120.8#
157 0.0 51.5 154.5#

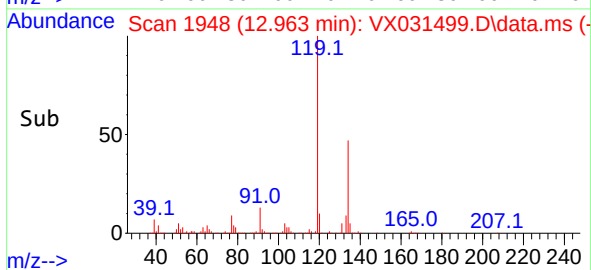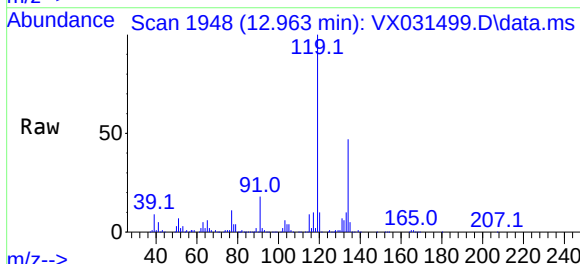



#95
Naphthalene
Concen: 2097.291 ug/l
RT: 13.786 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX031499.D
Acq: 20 Sep 2022 16:33

Instrument :
MSVOA_X
ClientSampleId :
COMP-2ME



Tgt Ion:128 Resp:11763004
Ion Ratio Lower Upper
128 100
127 19.5 10.4 15.6#
129 17.2 8.8 13.2#

