

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092022\
 Data File : VX031495.D
 Acq On : 20 Sep 2022 15:00
 Operator : JC/MD
 Sample : N4608-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TOWER-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M

Title : SW846 8260

Signal : TIC: VX031495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	55	60	64	rBV	4072	5150	1.30%	0.262%
2	1.496	64	67	72	rVV	6808	8665	2.18%	0.441%
3	1.611	76	86	94	rVB8	6051	19990	5.04%	1.017%
4	2.386	207	213	229	rVB	41025	71491	18.03%	3.637%
5	2.563	236	242	251	rBV2	1805	5034	1.27%	0.256%
6	2.941	298	304	312	rVB	2891	6234	1.57%	0.317%
7	5.391	694	706	719	rBV2	46983	136985	34.54%	6.969%
8	5.550	721	732	748	rVV2	51059	143631	36.21%	7.307%
9	5.958	789	799	812	rBV2	58277	143684	36.23%	7.309%
10	6.763	922	931	944	rBV	73525	173723	43.80%	8.838%
11	8.653	1234	1241	1252	rBV	253212	396609	100.00%	20.176%
12	10.055	1465	1471	1481	rBV	184192	247416	62.38%	12.587%
13	11.079	1634	1639	1650	rBV	191663	259511	65.43%	13.202%
14	12.024	1789	1794	1800	rBV	263040	325772	82.14%	16.573%
15	13.469	2025	2031	2032	rBV6	5353	8616	2.17%	0.438%
16	14.085	2127	2132	2139	rBV6	4219	8312	2.10%	0.423%
17	15.091	2291	2297	2300	rBV7	2367	4896	1.23%	0.249%




Sum of corrected areas: 1965719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092022\
Data File : VX031495.D
Acq On : 20 Sep 2022 15:00
Operator : JC/MD
Sample : N4608-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

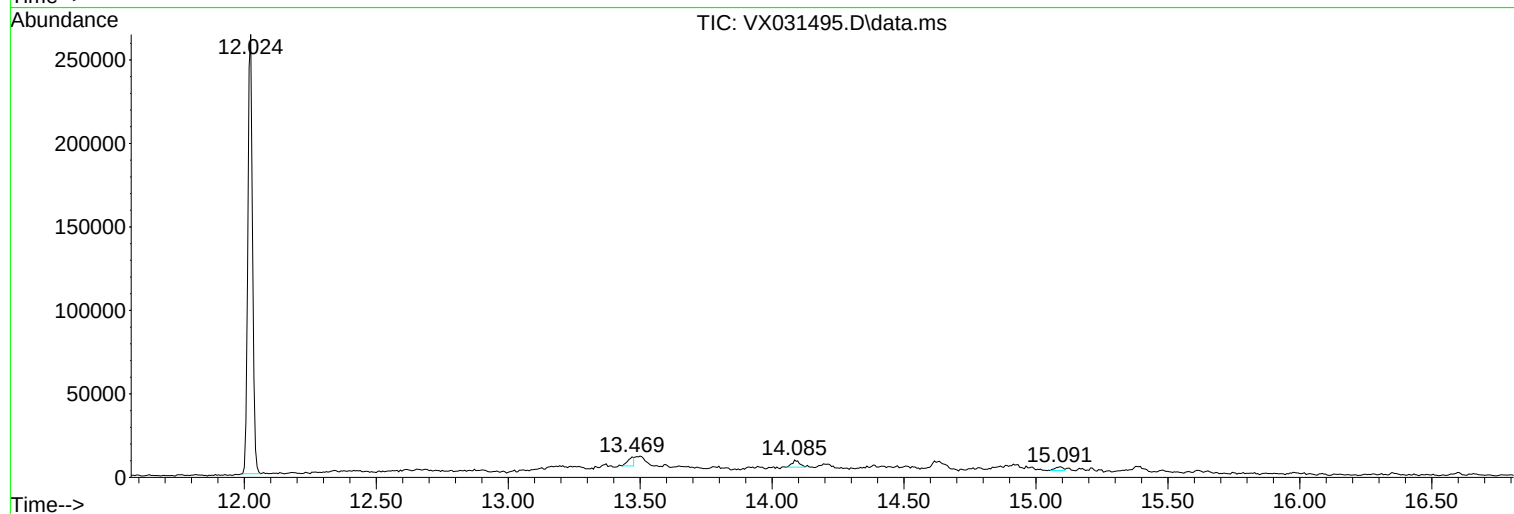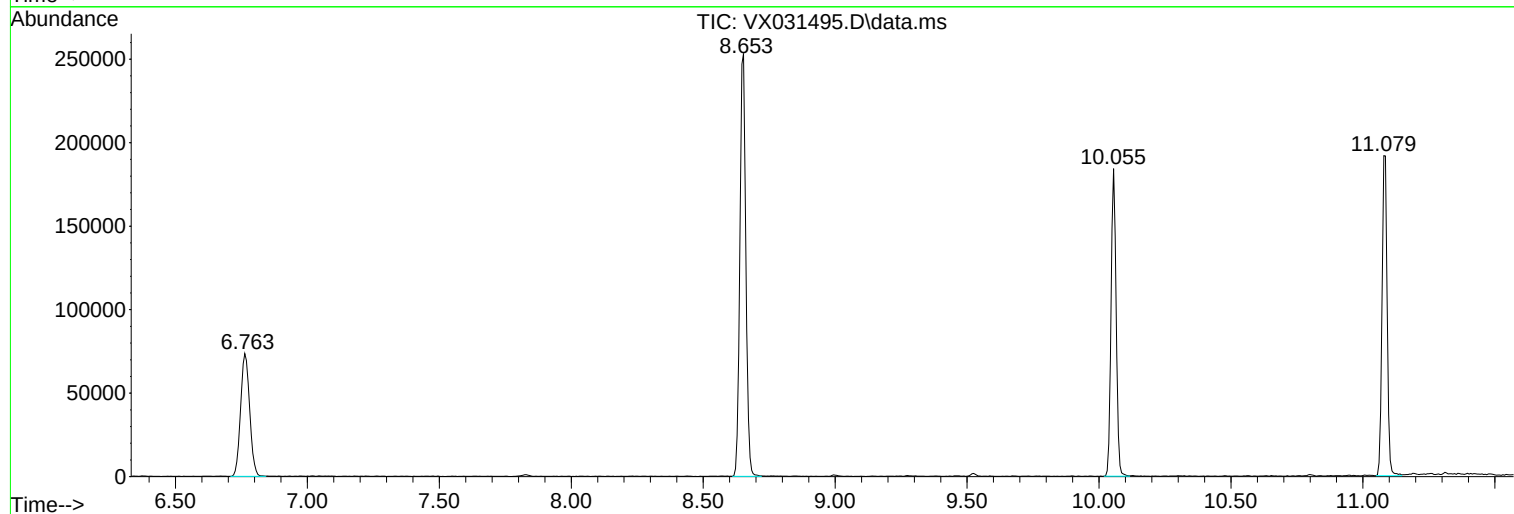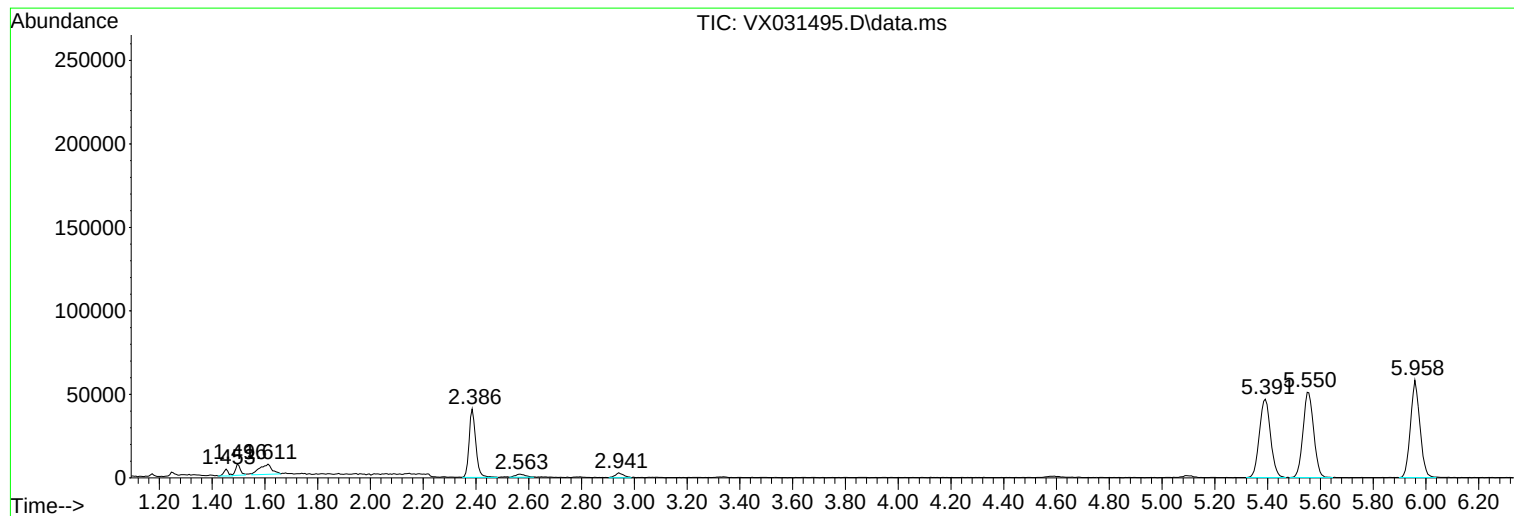

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092022\
Data File : VX031495.D
Acq On : 20 Sep 2022 15:00
Operator : JC/MD
Sample : N4608-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-1










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.611 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.611	6.96 ug/l	19990	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethyl Chloride	64	C2H5Cl	000075-00-3	35
2			2-Chloroethanol	80	C2H5ClO	000107-07-3	33
3			Butanoic acid, 3-oxo-, 2,2,2-tri...	232	C6H7Cl3O3	058547-15-2	17
4			Ethanol, 2,2,2-trichloro-	148	C2H3Cl3O	000115-20-8	17
5			1,2,5-Oxadiazol-3-carboxamide, 4...	284	C6H4N8O6	1000294-17-4	17

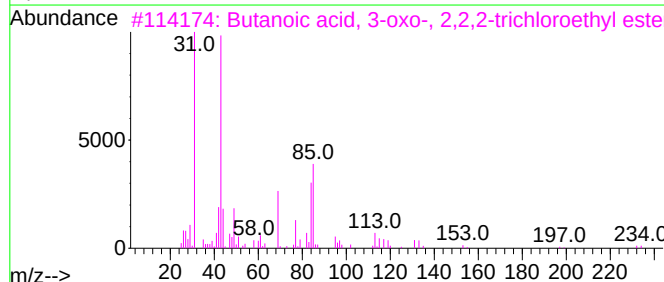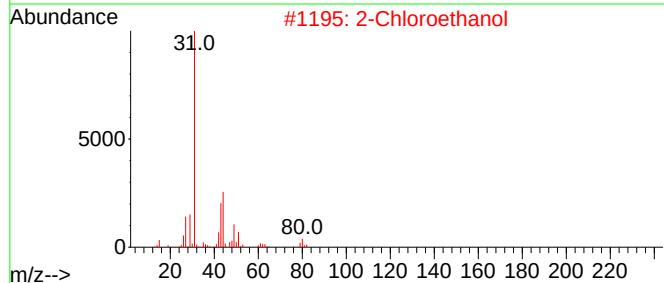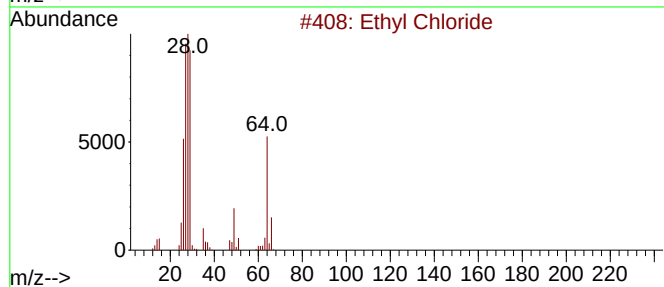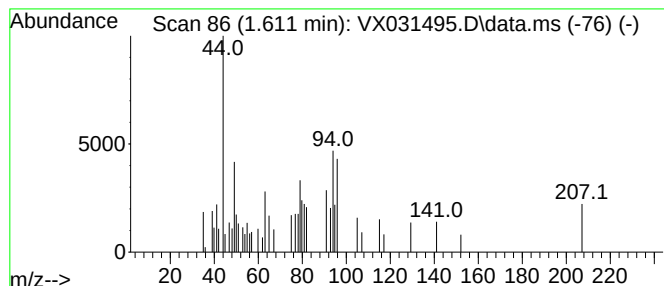

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092022\
Data File : VX031495.D
Acq On : 20 Sep 2022 15:00
Operator : JC/MD
Sample : N4608-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.611	1.611	7.0	ug/l	19990	1	5.556	143631	50.0