

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX092022\  
 Data File : VX031496.D  
 Acq On : 20 Sep 2022 15:23  
 Operator : JC/MD  
 Sample : N4608-02  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 TOWER-2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091922W.M

Title : SW846 8260

Signal : TIC: VX031496.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.496       | 64            | 67          | 71           | rVV      | 5357           | 6460          | 1.50%           | 0.311%        |
| 2         | 1.587       | 71            | 82          | 97           | rVV8     | 6769           | 23679         | 5.49%           | 1.142%        |
| 3         | 2.386       | 206           | 213         | 221          | rBV      | 38620          | 67113         | 15.57%          | 3.236%        |
| 4         | 2.947       | 297           | 305         | 314          | rVB3     | 2315           | 5229          | 1.21%           | 0.252%        |
| 5         | 5.105       | 650           | 659         | 669          | rBV4     | 2032           | 5448          | 1.26%           | 0.263%        |
| 6         | 5.391       | 693           | 706         | 719          | rBV2     | 51258          | 149385        | 34.65%          | 7.202%        |
| 7         | 5.556       | 722           | 733         | 746          | rVV      | 54160          | 149740        | 34.74%          | 7.219%        |
| 8         | 5.958       | 787           | 799         | 813          | rBV2     | 58462          | 153661        | 35.65%          | 7.408%        |
| 9         | 6.763       | 920           | 931         | 941          | rBV      | 78236          | 186427        | 43.25%          | 8.988%        |
| 10        | 8.647       | 1234          | 1240        | 1250         | rBV      | 271709         | 431068        | 100.00%         | 20.783%       |
| 11        | 10.055      | 1465          | 1471        | 1483         | rVB      | 205332         | 266077        | 61.73%          | 12.828%       |
| 12        | 11.079      | 1634          | 1639        | 1652         | rVB      | 214207         | 273352        | 63.41%          | 13.179%       |
| 13        | 12.024      | 1789          | 1794        | 1805         | rVB      | 283639         | 343644        | 79.72%          | 16.568%       |
| 14        | 13.487      | 2027          | 2034        | 2046         | rVB      | 1919           | 7202          | 1.67%           | 0.347%        |
| 15        | 15.390      | 2339          | 2346        | 2353         | rVB7     | 1996           | 5697          | 1.32%           | 0.275%        |




Sum of corrected areas: 2074182

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX092022\  
Data File : VX031496.D  
Acq On : 20 Sep 2022 15:23  
Operator : JC/MD  
Sample : N4608-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TOWER-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

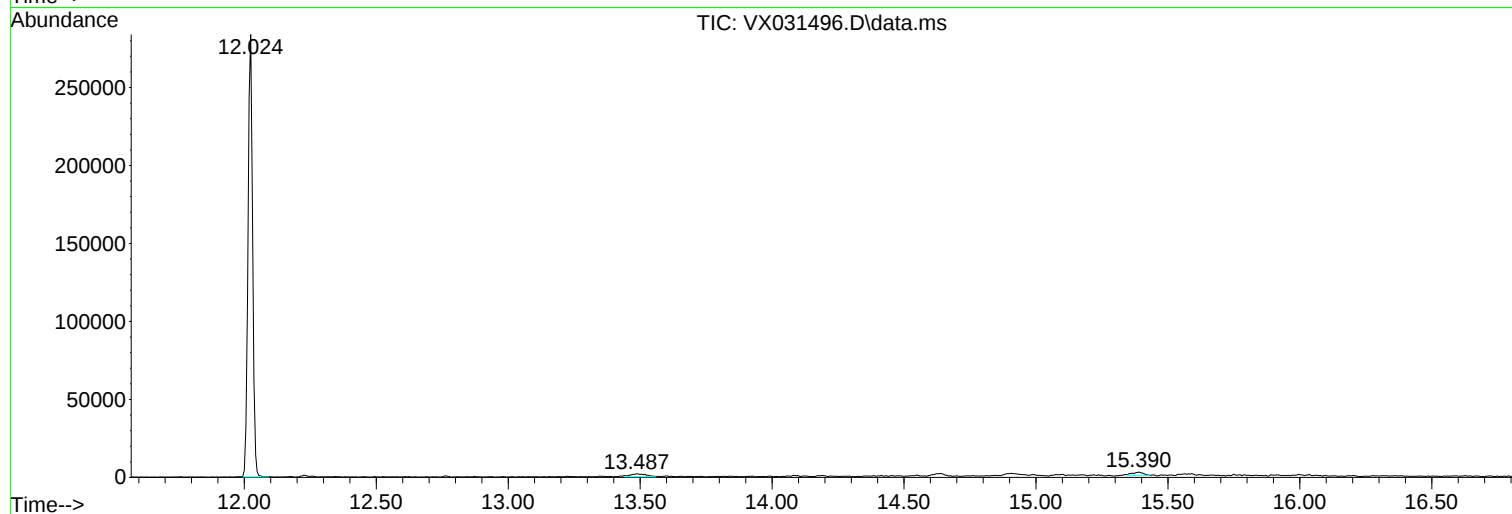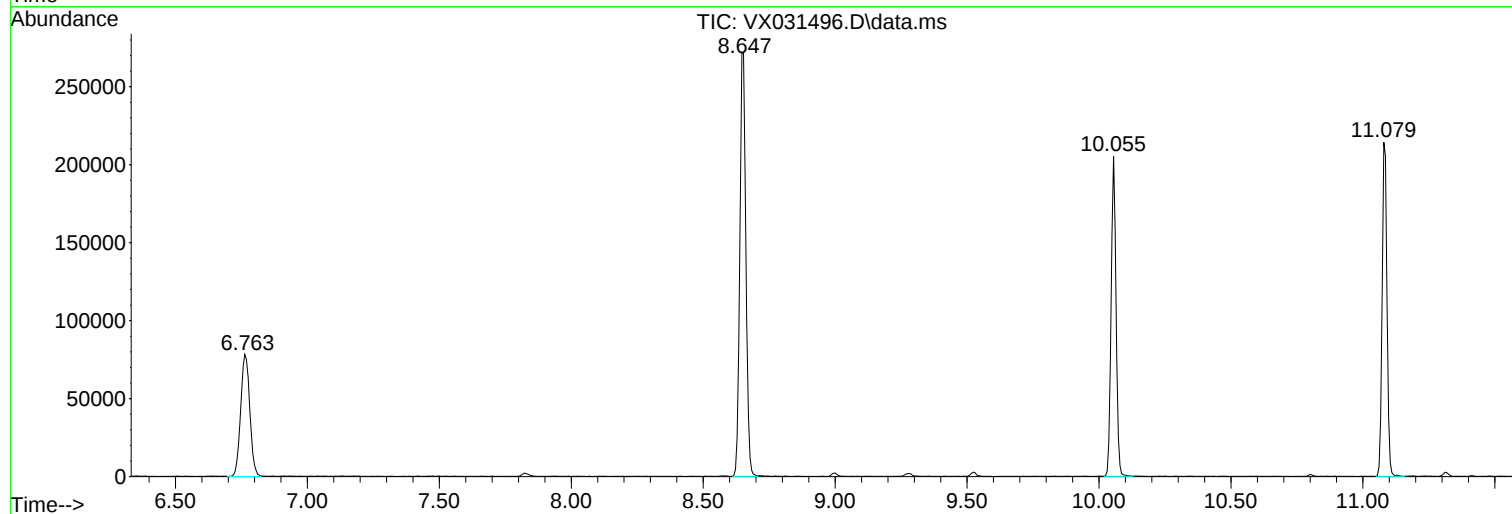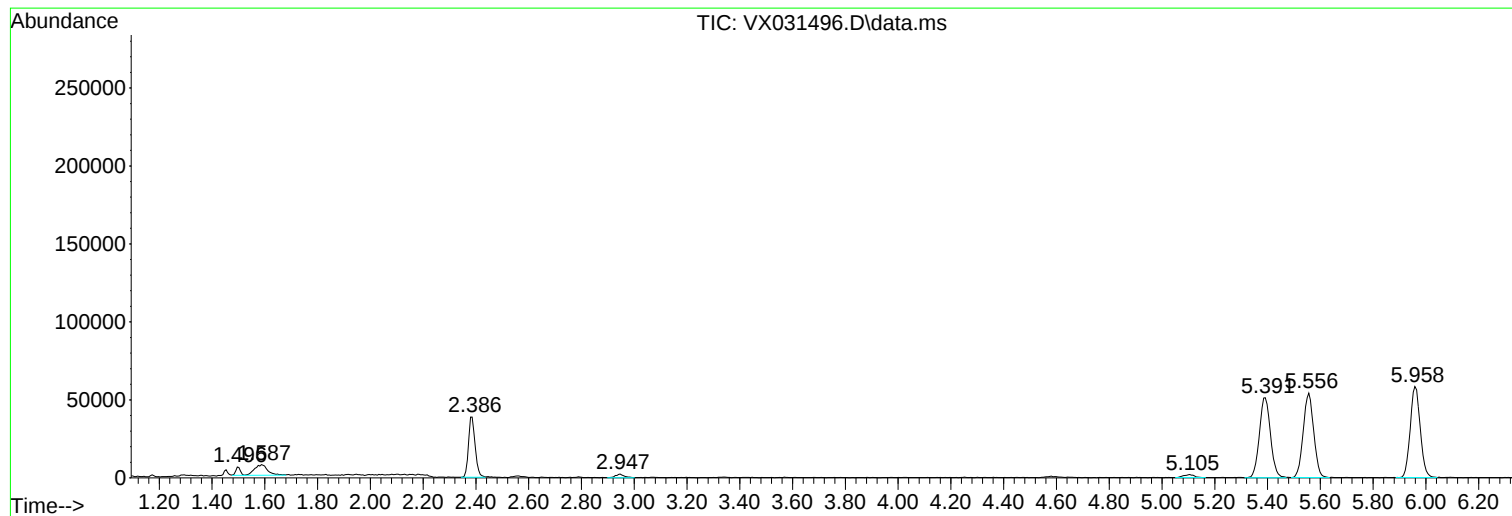

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX092022\  
Data File : VX031496.D  
Acq On : 20 Sep 2022 15:23  
Operator : JC/MD  
Sample : N4608-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TOWER-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX092022\  
Data File : VX031496.D  
Acq On : 20 Sep 2022 15:23  
Operator : JC/MD  
Sample : N4608-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TOWER-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|