


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092622\
Data File : VX031640.D
Acq On : 26 Sep 2022 09:00
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Title : SW846 8260
Last Update : Tue Sep 27 01:44:18 2022

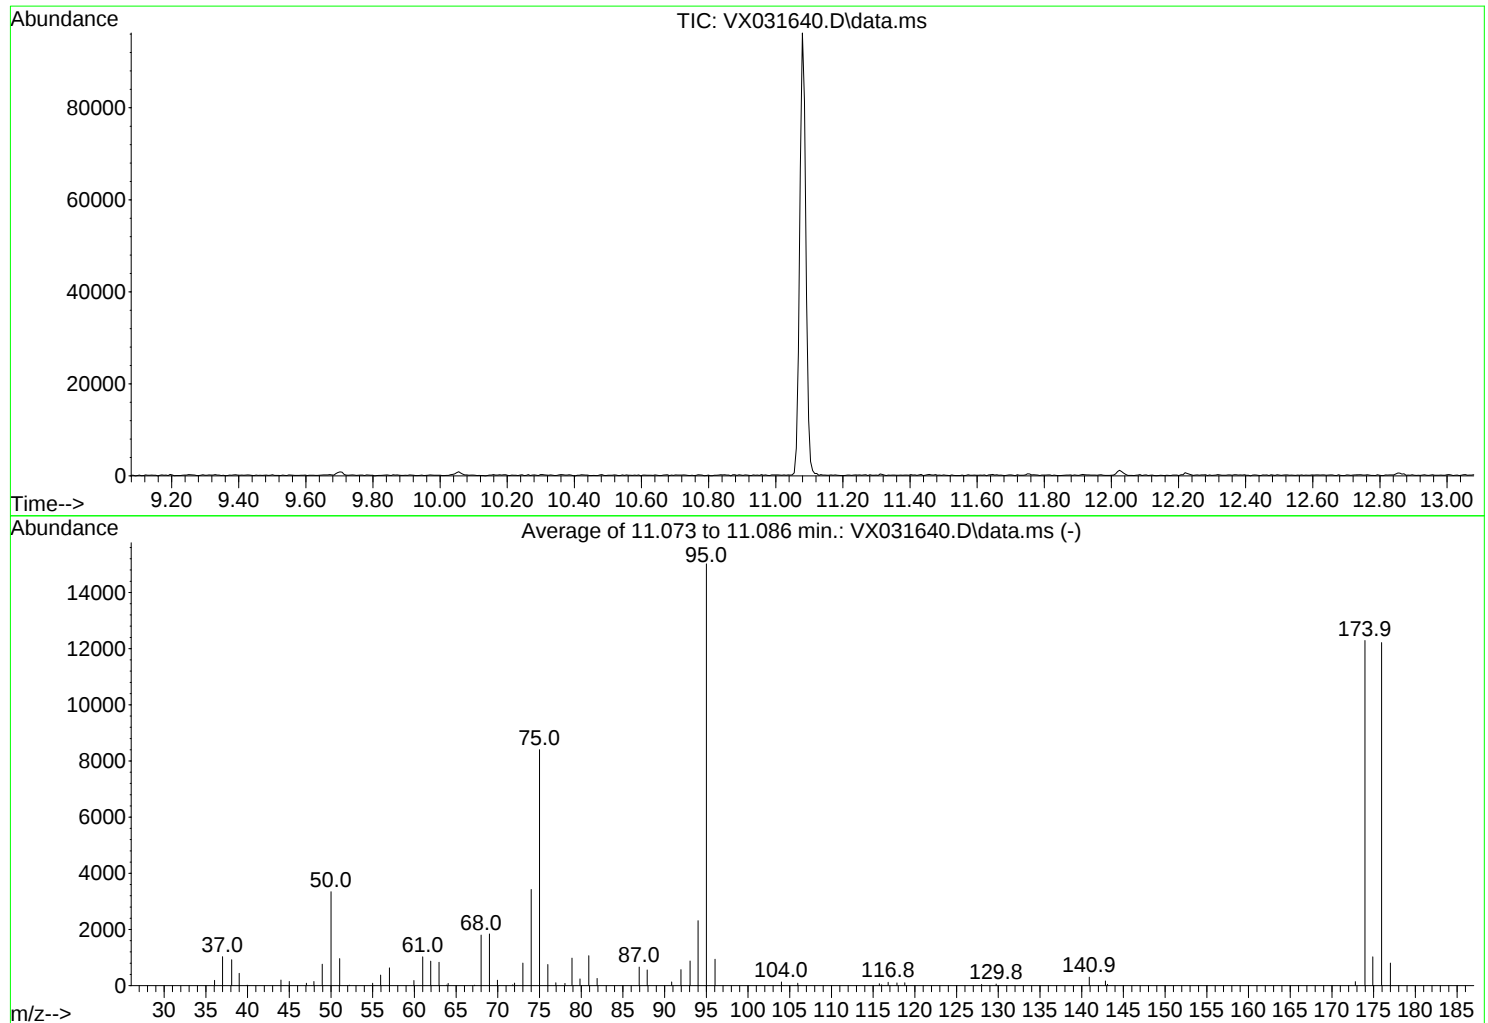

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	3344	PASS
75	95	30	60	56.0	8404	PASS
95	95	100	100	100.0	15020	PASS
96	95	5	9	6.3	941	PASS
173	174	0.00	2	1.1	140	PASS
174	95	50	100	81.8	12289	PASS
175	174	5	9	8.4	1027	PASS
176	174	95	101	99.4	12217	PASS
177	176	5	9	6.6	802	PASS