
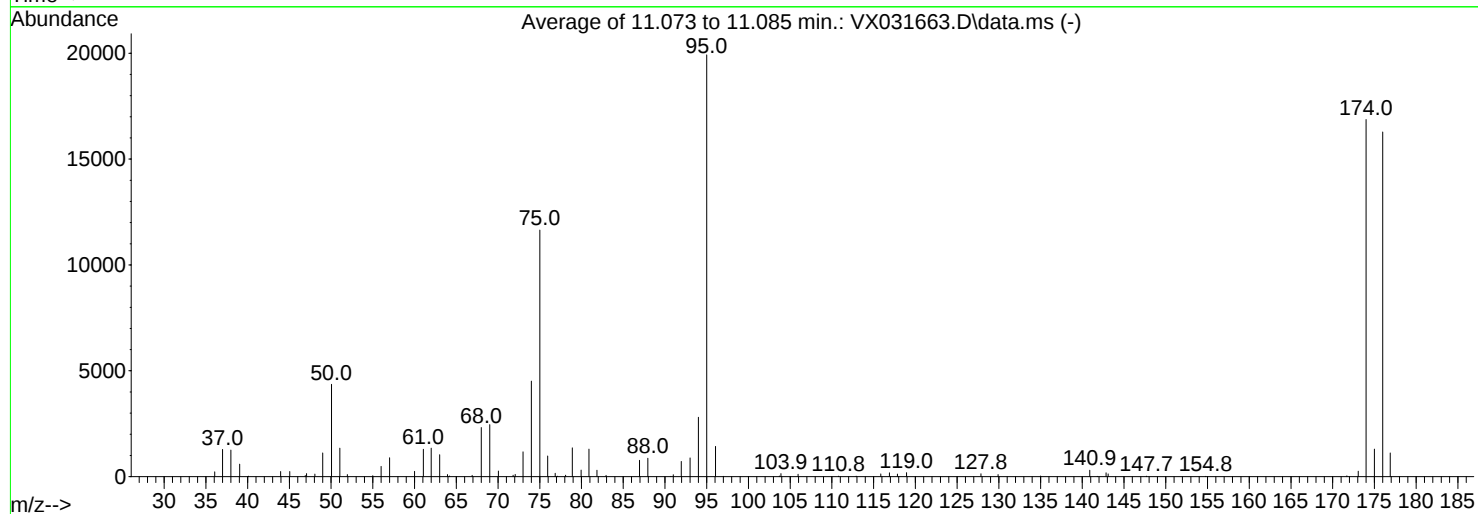


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092622\
Data File : VX031663.D
Acq On : 26 Sep 2022 21:19
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092622W.M
Title : SW846 8260
Last Update : Tue Sep 27 01:44:18 2022

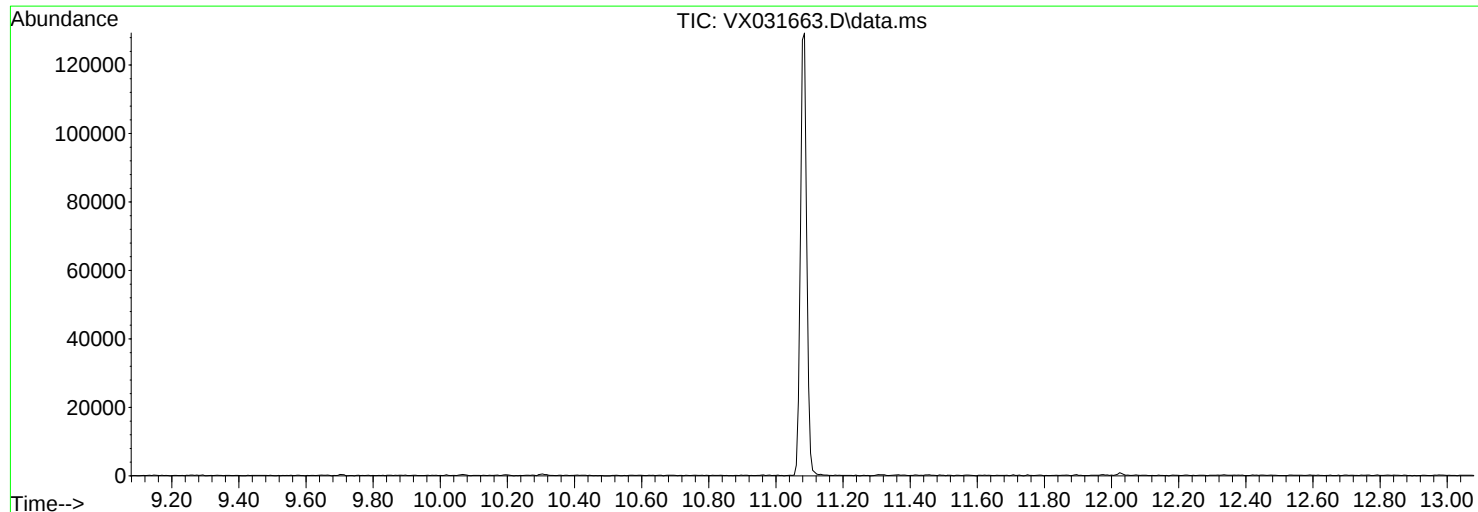

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	4358	PASS
75	95	30	60	58.5	11650	PASS
95	95	100	100	100.0	19925	PASS
96	95	5	9	7.2	1425	PASS
173	174	0.00	2	1.5	255	PASS
174	95	50	100	84.7	16870	PASS
175	174	5	9	7.7	1302	PASS
176	174	95	101	96.5	16282	PASS
177	176	5	9	6.9	1122	PASS