

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100323\
Data File : VX038045.D
Acq On : 03 Oct 2023 18:29
Operator : JC/MD
Sample : VX1003MBL01
Misc : 5.00g/10 mL/100uL/5.0mL/MSVOA_X/MeOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1003MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100323W.M

Title : SW846 8260

Signal : TIC: VX038045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	36	rBV	14460	33629	4.32%	0.805%
2	1.551	70	76	82	rBV2	15774	27403	3.52%	0.656%
3	5.385	694	705	722	rBV	90108	265353	34.11%	6.352%
4	5.550	722	732	749	rVB	140840	393280	50.56%	9.414%
5	5.958	788	799	817	rBV	108896	292026	37.54%	6.990%
6	6.763	921	931	946	rBV	222545	530430	68.19%	12.697%
7	8.647	1234	1240	1250	rBV	485503	777877	100.00%	18.620%
8	10.055	1465	1471	1485	rBV	489372	662165	85.12%	15.850%
9	11.079	1634	1639	1654	rBV	395847	523295	67.27%	12.526%
10	12.024	1788	1794	1804	rBV	511387	672287	86.43%	16.092%




Sum of corrected areas: 4177745

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100323\
Data File : VX038045.D
Acq On : 03 Oct 2023 18:29
Operator : JC/MD
Sample : VX1003MBL01
Misc : 5.00g/10 mL/100uL/5.0mL/MSVOA_X/MeOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1003MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

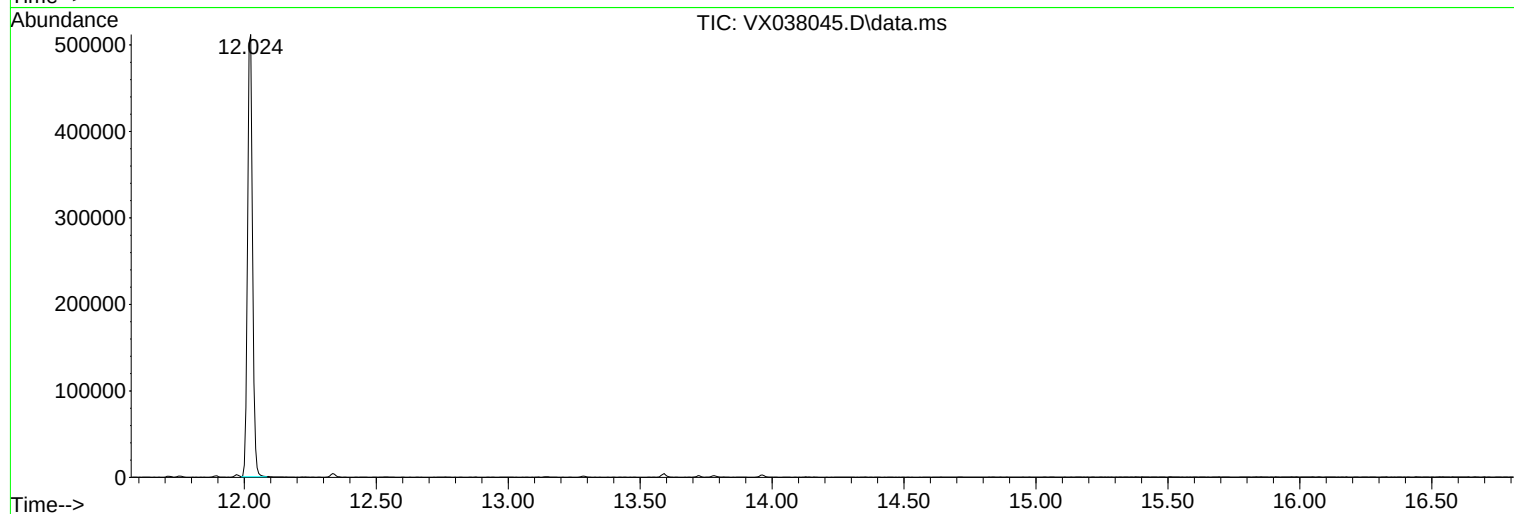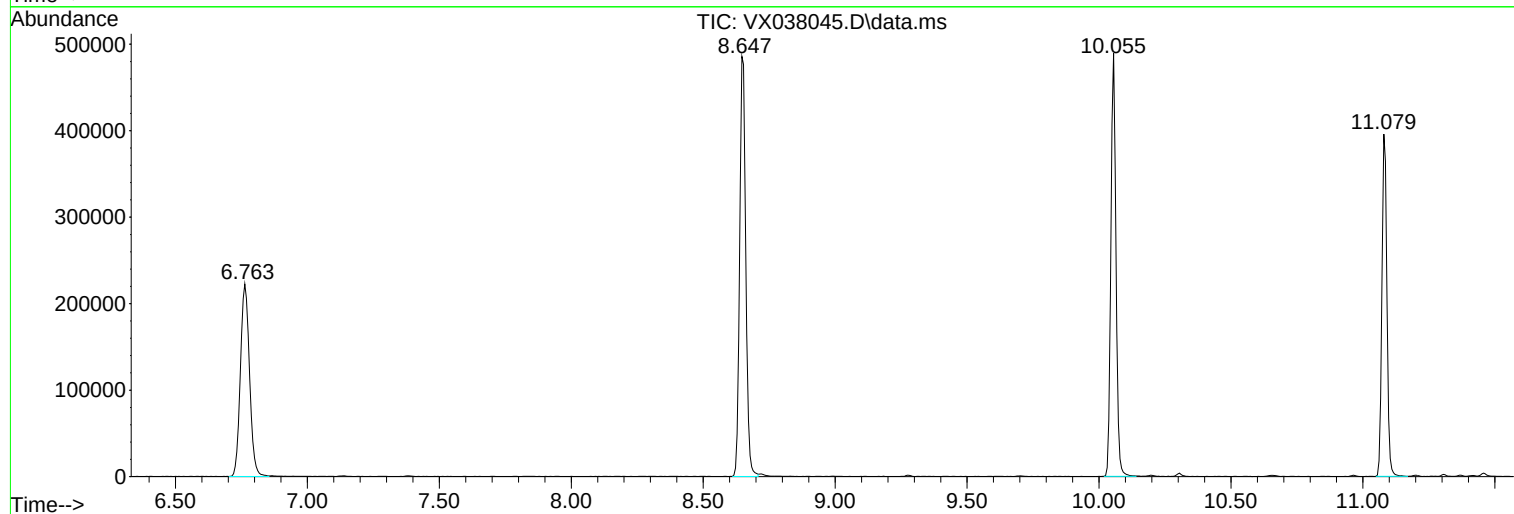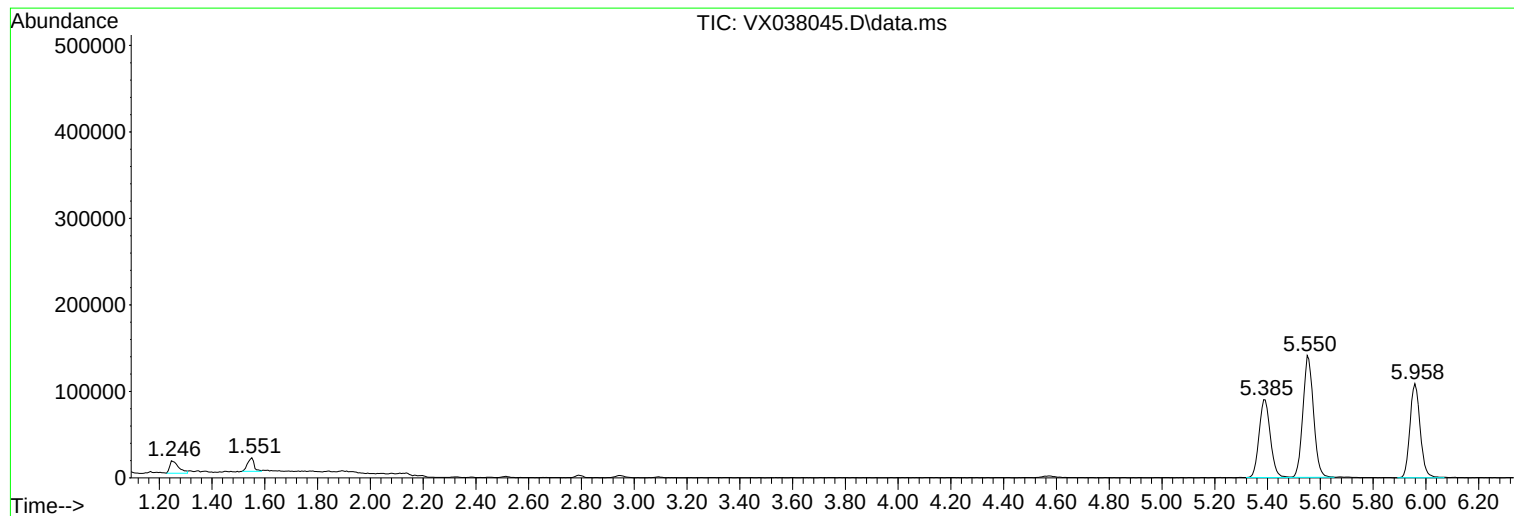

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100323\
Data File : VX038045.D
Acq On : 03 Oct 2023 18:29
Operator : JC/MD
Sample : VX1003MBL01
Misc : 5.00g/10 mL/100uL/5.0mL/MSVOA_X/MeOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1003MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100323\
Data File : VX038045.D
Acq On : 03 Oct 2023 18:29
Operator : JC/MD
Sample : VX1003MBL01
Misc : 5.00g/10 mL/100uL/5.0mL/MSVOA_X/MeOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1003MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------