



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100323\
Data File : VX038030.D
Acq On : 03 Oct 2023 10:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100323W.M
Title : SW846 8260
Last Update : Wed Oct 04 09:08:35 2023

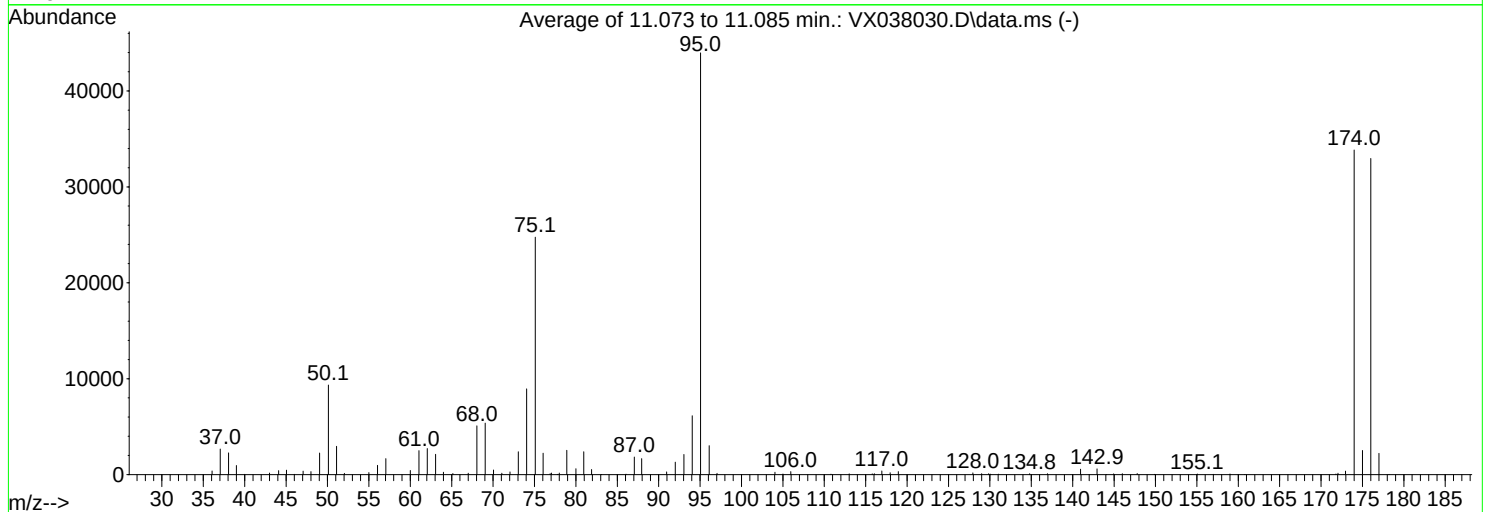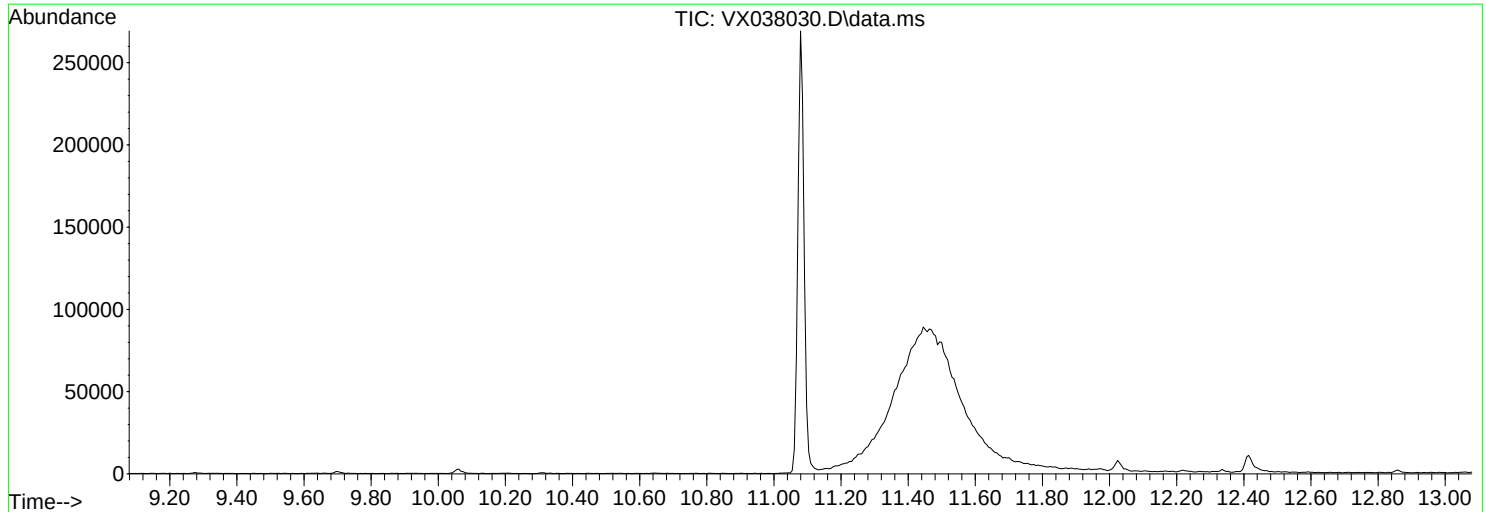

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	9348	PASS
75	95	30	60	56.3	24760	PASS
95	95	100	100	100.0	43973	PASS
96	95	5	9	6.9	3020	PASS
173	174	0.00	2	1.1	368	PASS
174	95	50	100	77.0	33840	PASS
175	174	5	9	7.4	2519	PASS
176	174	95	101	97.4	32968	PASS
177	176	5	9	6.7	2224	PASS