

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101323\
 Data File : VX038287.D
 Acq On : 13 Oct 2023 16:15
 Operator : JC/MD
 Sample : 04884-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 026-OUTFALL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Title : SW846 8260

Signal : TIC: VX038287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.374	206	211	224	rBV	28291	48840	7.25%	1.280%
2	4.562	564	570	583	rBV2	2878	8084	1.20%	0.212%
3	5.385	694	705	721	rBV2	75521	218776	32.49%	5.736%
4	5.550	721	732	755	rVB	114706	330422	49.06%	8.663%
5	5.958	788	799	811	rBV	80613	220749	32.78%	5.787%
6	6.763	921	931	948	rBV	191985	459830	68.28%	12.055%
7	8.580	1223	1229	1234	rBV	4081	6934	1.03%	0.182%
8	8.647	1234	1240	1260	rVV	415494	663337	98.50%	17.390%
9	10.055	1465	1471	1483	rBV	464713	629748	93.51%	16.510%
10	10.372	1516	1523	1534	rVB	6580	8991	1.34%	0.236%
11	10.659	1565	1570	1579	rVB	36335	50317	7.47%	1.319%
12	11.079	1634	1639	1651	rBV	382461	494890	73.48%	12.974%
13	12.024	1788	1794	1804	rBV	520382	673464	100.00%	17.656%




Sum of corrected areas: 3814382

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101323\
Data File : VX038287.D
Acq On : 13 Oct 2023 16:15
Operator : JC/MD
Sample : 04884-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
026-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

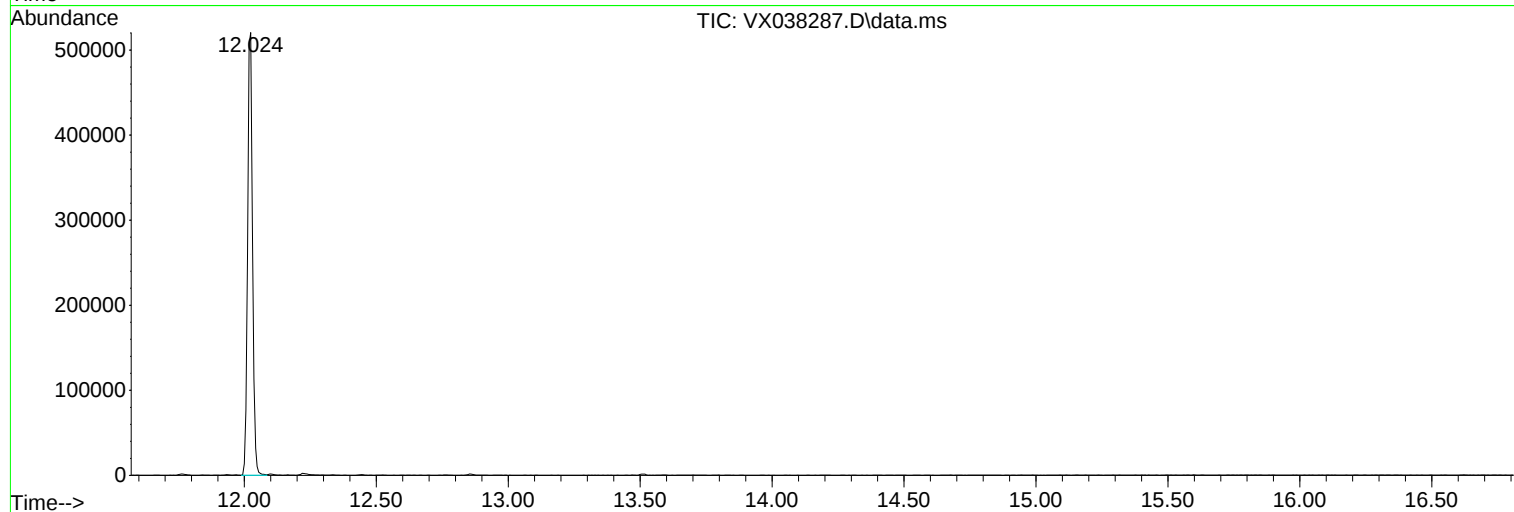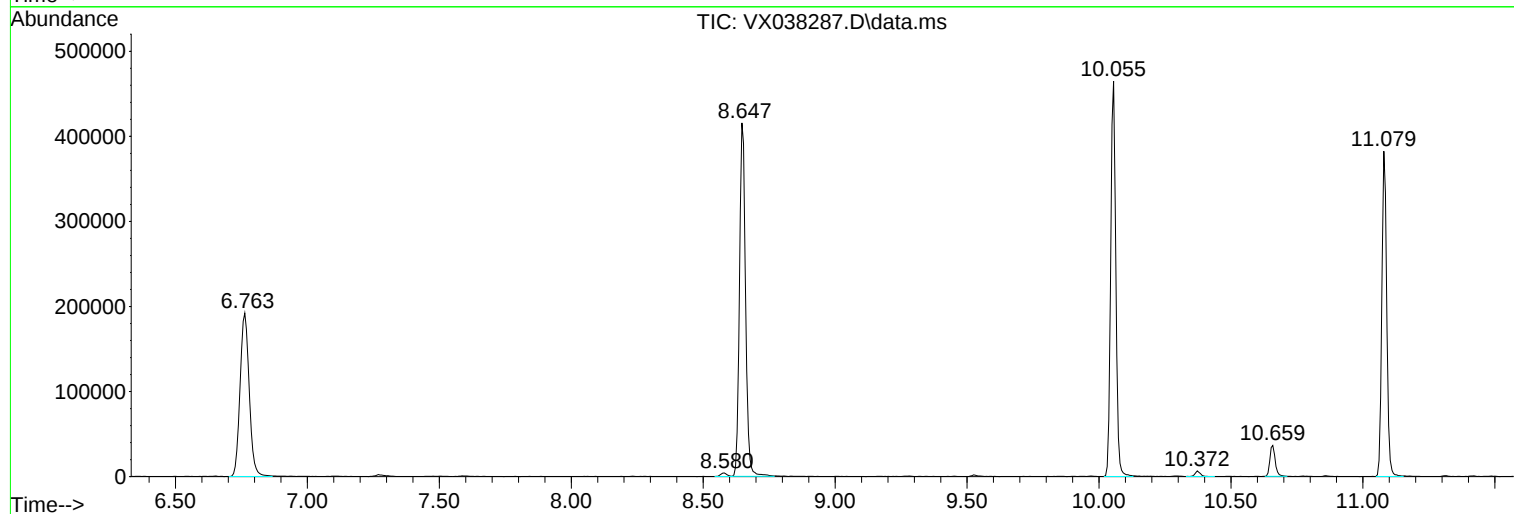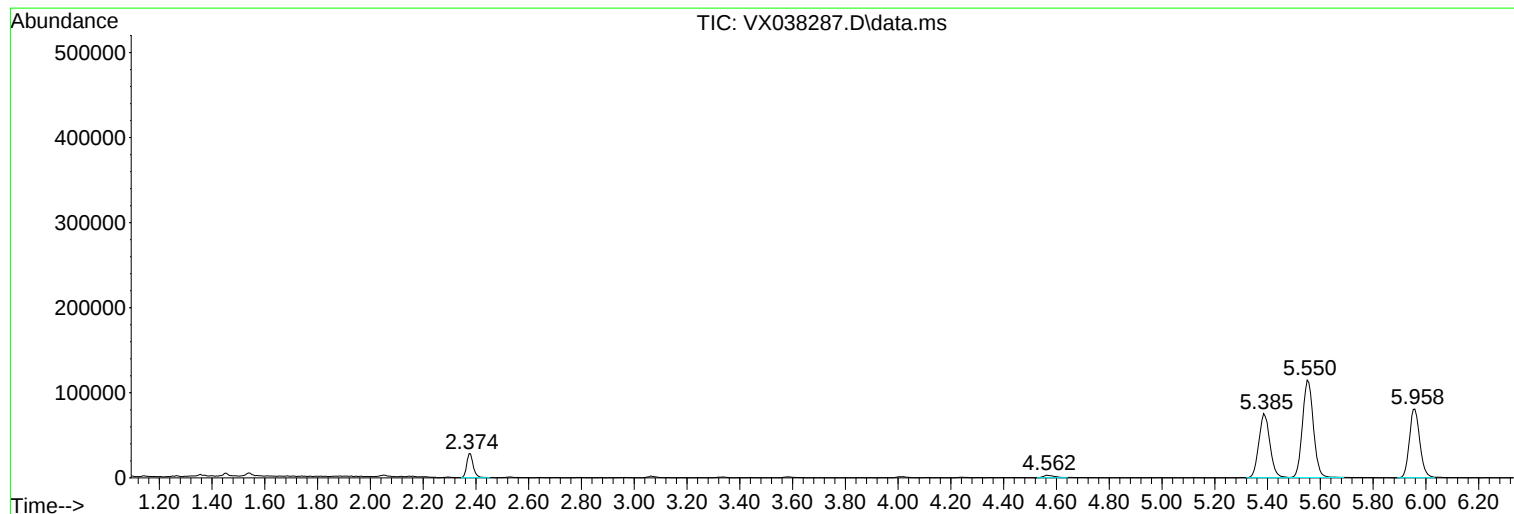

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101323\
Data File : VX038287.D
Acq On : 13 Oct 2023 16:15
Operator : JC/MD
Sample : 04884-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
026-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101323\
Data File : VX038287.D
Acq On : 13 Oct 2023 16:15
Operator : JC/MD
Sample : 04884-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
026-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------