

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101623\
Data File : VX038295.D
Acq On : 16 Oct 2023 11:35
Operator : JC/MD
Sample : VX1016MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1016MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	721	rBV2	99433	289412	32.51%	5.893%
2	5.550	721	732	747	rVV	158424	453978	51.00%	9.244%
3	5.952	787	798	814	rBV	107039	286796	32.22%	5.840%
4	6.757	921	930	947	rBV	254462	621380	69.80%	12.653%
5	8.647	1234	1240	1259	rBV	554863	874109	98.19%	17.799%
6	10.055	1465	1471	1490	rBV	593196	833304	93.61%	16.968%
7	11.079	1634	1639	1650	rBV	513600	661768	74.34%	13.475%
8	12.024	1788	1794	1805	rBV	690208	890227	100.00%	18.127%




Sum of corrected areas: 4910974

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101623\
Data File : VX038295.D
Acq On : 16 Oct 2023 11:35
Operator : JC/MD
Sample : VX1016MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1016MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

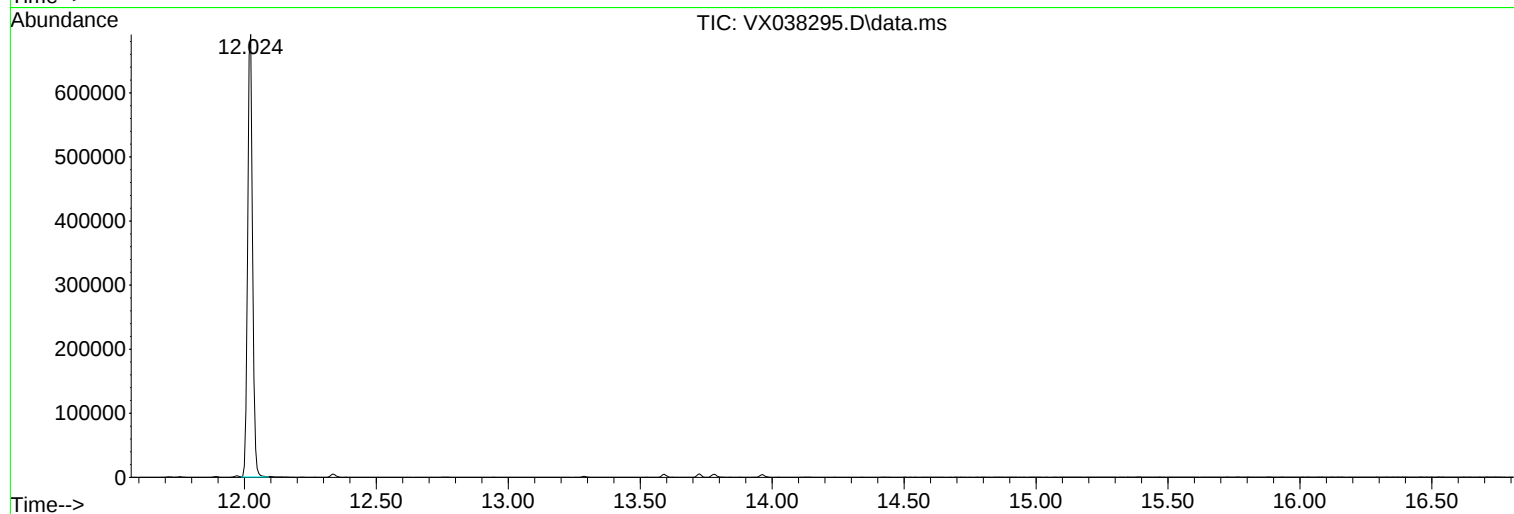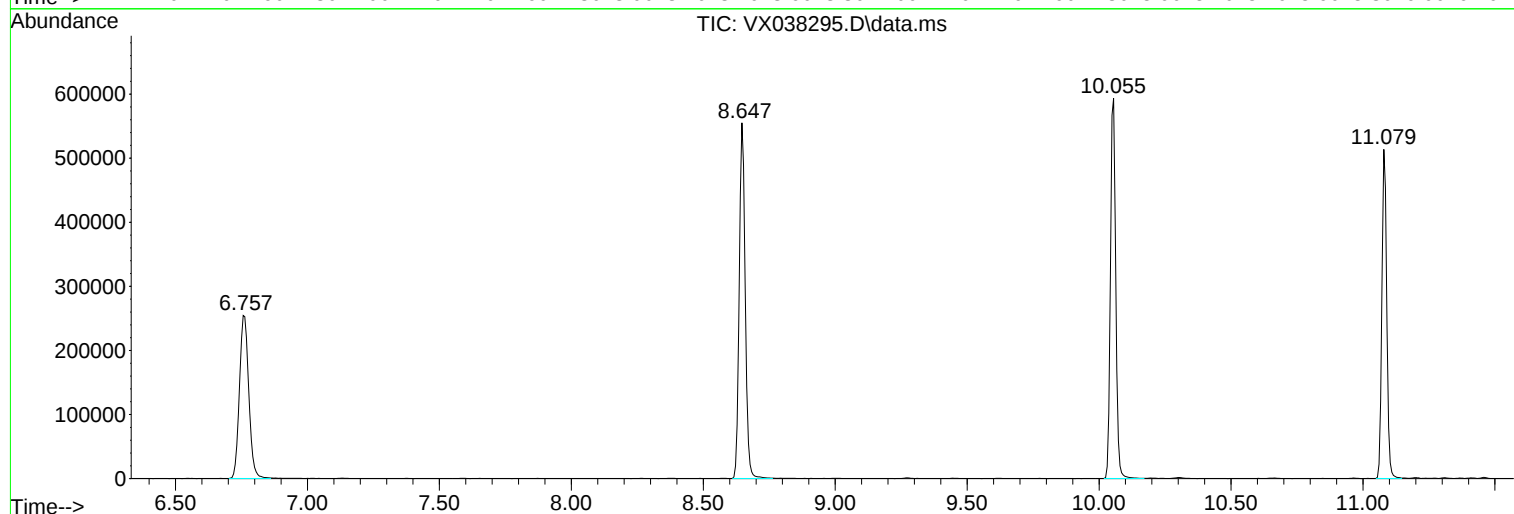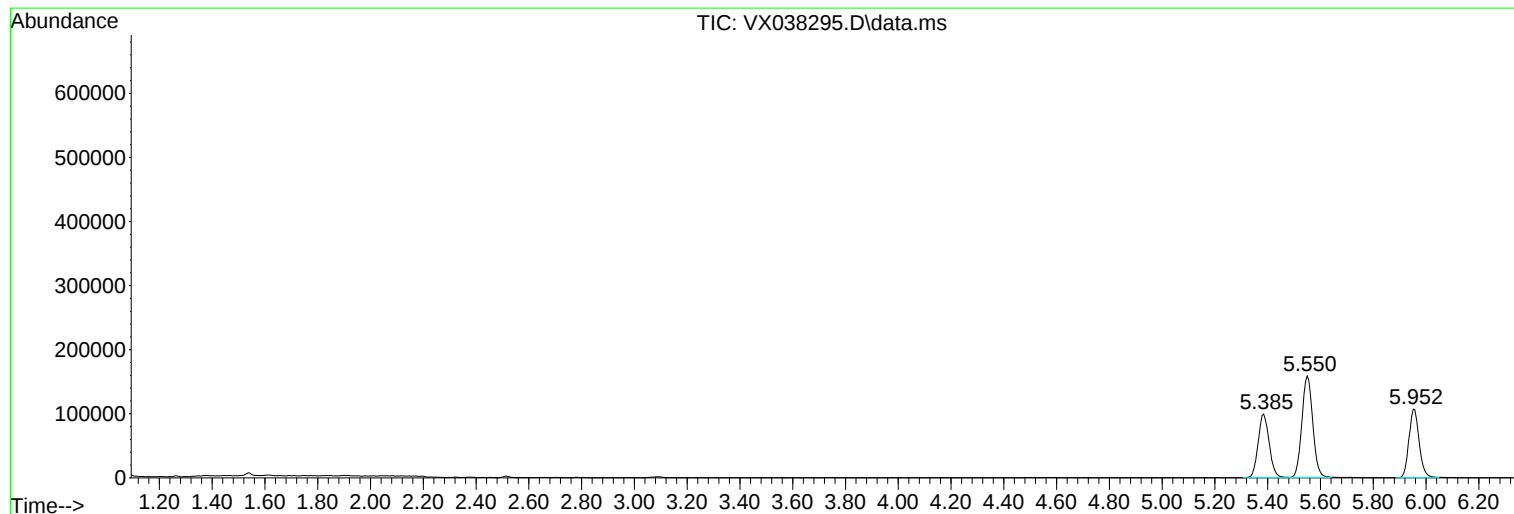

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101623\
Data File : VX038295.D
Acq On : 16 Oct 2023 11:35
Operator : JC/MD
Sample : VX1016MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1016MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101623\
Data File : VX038295.D
Acq On : 16 Oct 2023 11:35
Operator : JC/MD
Sample : VX1016MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1016MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc