

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX101623\  
Data File : VX038314.D  
Acq On : 16 Oct 2023 19:13  
Operator : JC/MD  
Sample : 04899-18  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
DUP-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038314.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.551       | 68            | 76          | 80           | rBV3     | 8315           | 13501         | 1.41%           | 0.256%        |
| 2         | 5.093       | 642           | 657         | 672          | rBV2     | 105180         | 307172        | 32.15%          | 5.833%        |
| 3         | 5.385       | 694           | 705         | 721          | rBV2     | 112637         | 332546        | 34.81%          | 6.315%        |
| 4         | 5.550       | 721           | 732         | 747          | rVV      | 150740         | 430979        | 45.11%          | 8.184%        |
| 5         | 5.952       | 789           | 798         | 814          | rBV2     | 131773         | 344291        | 36.03%          | 6.538%        |
| 6         | 6.763       | 921           | 931         | 948          | rBV      | 245924         | 586639        | 61.40%          | 11.140%       |
| 7         | 8.647       | 1234          | 1240        | 1261         | rBV      | 599776         | 955440        | 100.00%         | 18.143%       |
| 8         | 10.055      | 1465          | 1471        | 1482         | rBV      | 571588         | 769694        | 80.56%          | 14.616%       |
| 9         | 11.079      | 1634          | 1639        | 1653         | rBV      | 541625         | 702133        | 73.49%          | 13.333%       |
| 10        | 12.024      | 1788          | 1794        | 1803         | rBV      | 632328         | 823827        | 86.22%          | 15.644%       |




Sum of corrected areas: 5266222

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX101623\  
Data File : VX038314.D  
Acq On : 16 Oct 2023 19:13  
Operator : JC/MD  
Sample : 04899-18  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
DUP-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

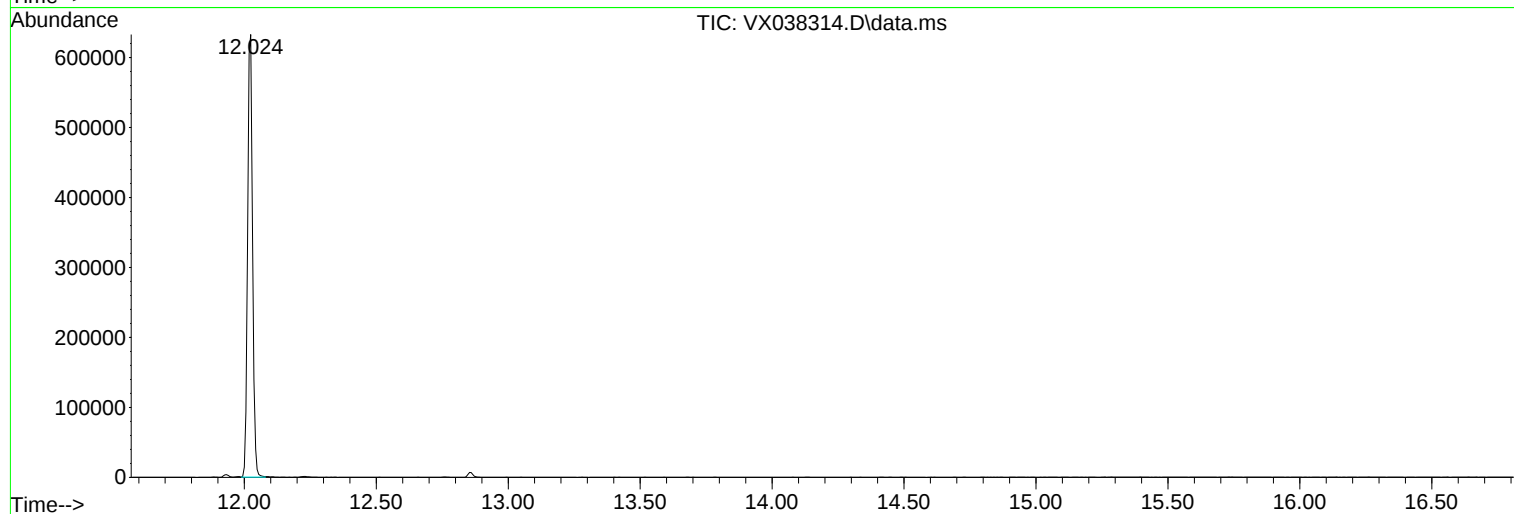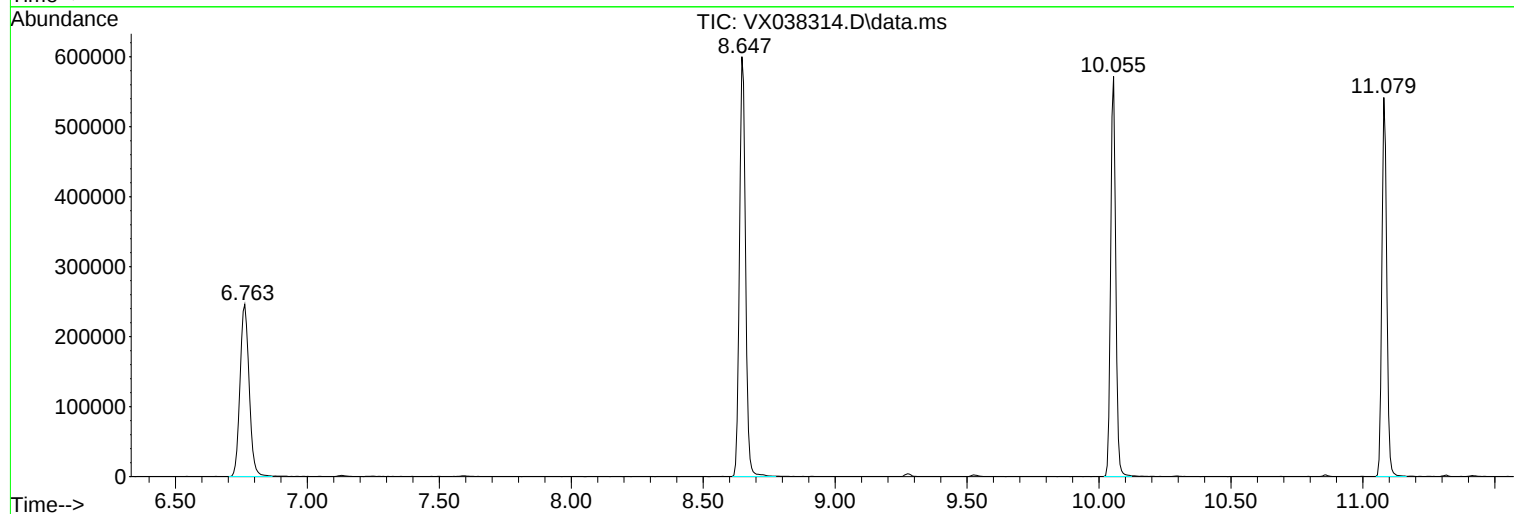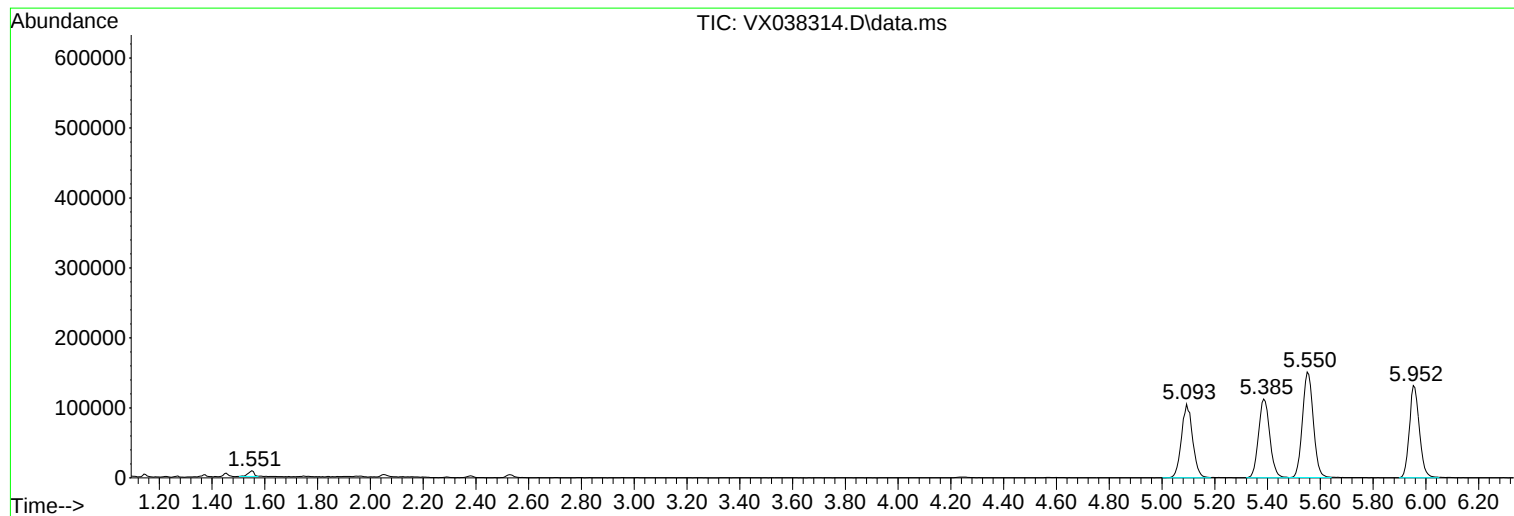

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX101623\  
Data File : VX038314.D  
Acq On : 16 Oct 2023 19:13  
Operator : JC/MD  
Sample : 04899-18  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
DUP-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX101623\  
Data File : VX038314.D  
Acq On : 16 Oct 2023 19:13  
Operator : JC/MD  
Sample : 04899-18  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
DUP-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|