



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101623\
Data File : VX038293.D
Acq On : 16 Oct 2023 08:40
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Title : SW846 8260
Last Update : Thu Oct 05 15:27:13 2023

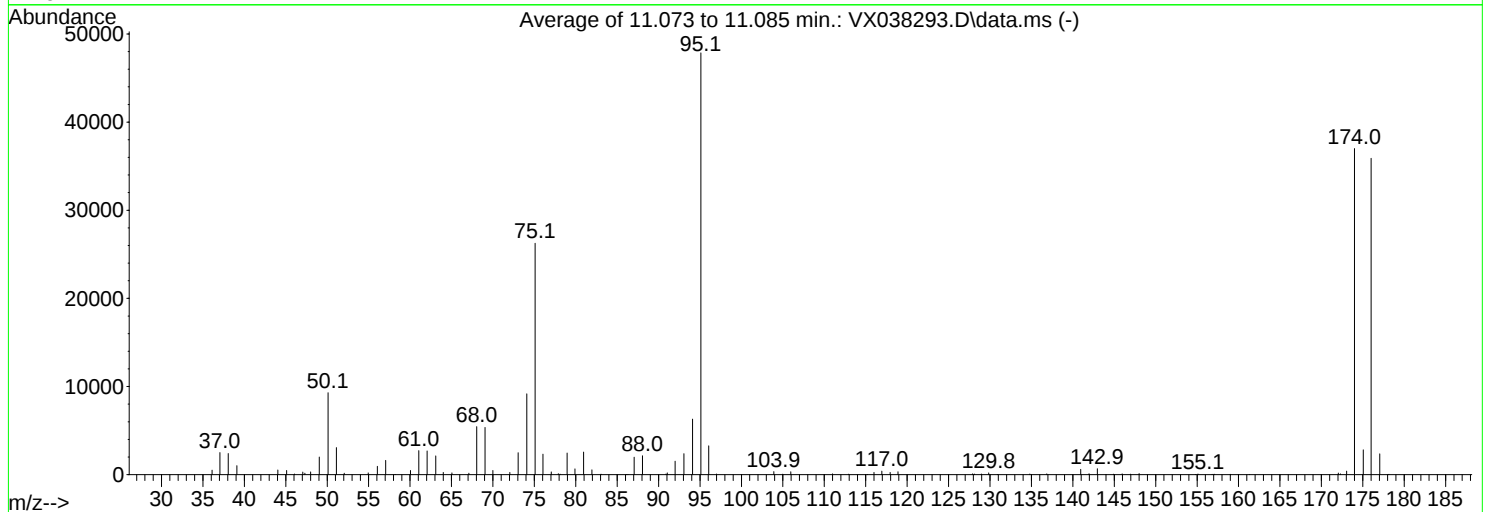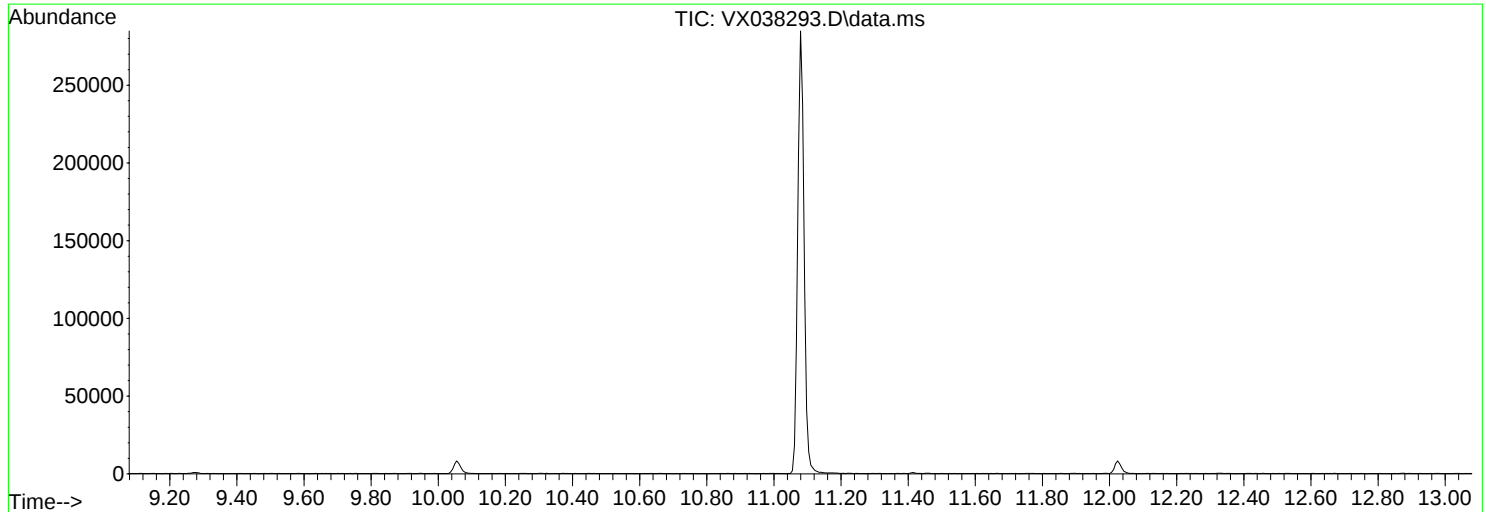

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	9292	PASS
75	95	30	60	54.9	26253	PASS
95	95	100	100	100.0	47859	PASS
96	95	5	9	6.8	3261	PASS
173	174	0.00	2	1.1	407	PASS
174	95	50	100	77.3	37000	PASS
175	174	5	9	7.6	2822	PASS
176	174	95	101	97.0	35896	PASS
177	176	5	9	6.6	2357	PASS