

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102324\
Data File : VX043489.D
Acq On : 23 Oct 2024 15:50
Operator : JC/MD
Sample : VX1023WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1023WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102324W.M

Title : SW846 8260

Signal : TIC: VX043489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	69	78	79	rBV4	6346	11701	2.74%	0.533%
2	1.605	80	85	86	rBV4	4097	6417	1.51%	0.292%
3	1.666	93	95	99	rVB5	8324	13624	3.20%	0.620%
4	2.178	175	179	187	rVB4	2370	6208	1.46%	0.283%
5	2.940	298	304	314	rBV2	4014	8594	2.02%	0.391%
6	5.385	694	705	722	rBV3	45350	141254	33.13%	6.432%
7	5.550	722	732	748	rVB2	81456	234720	55.06%	10.688%
8	5.958	788	799	817	rBV2	52643	142020	33.31%	6.467%
9	6.763	921	931	946	rBV	128740	317630	74.50%	14.463%
10	8.647	1234	1240	1256	rBV	255702	426336	100.00%	19.413%
11	10.055	1465	1471	1484	rBV	246064	351645	82.48%	16.012%
12	11.079	1635	1639	1653	rBV	174119	246288	57.77%	11.215%
13	12.024	1788	1794	1813	rBV	211414	289717	67.96%	13.192%


Sum of corrected areas: 2196154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102324\
Data File : VX043489.D
Acq On : 23 Oct 2024 15:50
Operator : JC/MD
Sample : VX1023WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1023WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102324W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

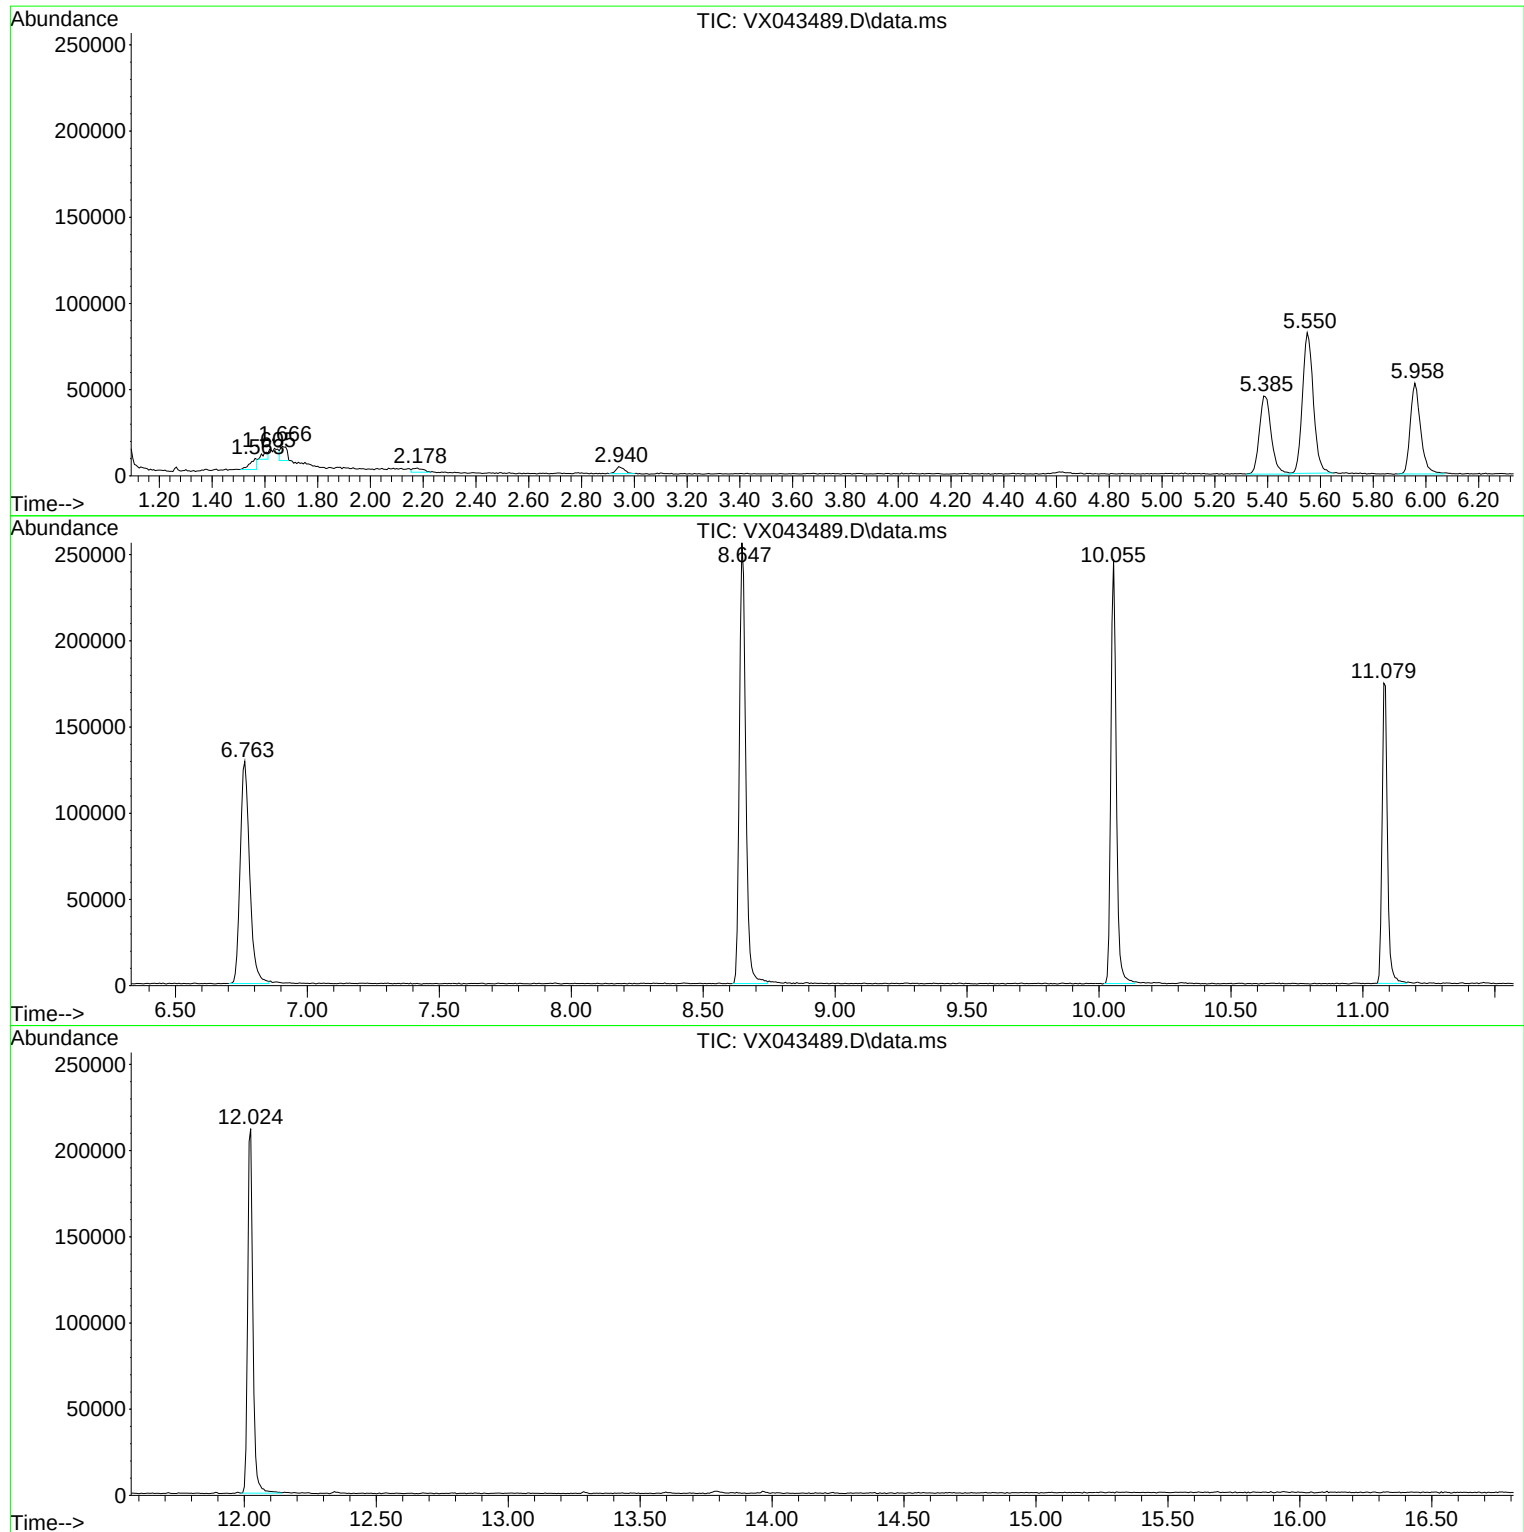

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102324\
Data File : VX043489.D
Acq On : 23 Oct 2024 15:50
Operator : JC/MD
Sample : VX1023WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1023WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102324W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102324\
Data File : VX043489.D
Acq On : 23 Oct 2024 15:50
Operator : JC/MD
Sample : VX1023WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1023WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102324W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
