

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043513.D
 Acq On : 25 Oct 2024 10:57
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 26 00:11:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 26 00:05:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	276017	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	239725	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	109116	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	76753	51.118	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	102.240%
7) Chloroethane-d5	1.666	69	64482	53.625	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.260%
11) 1,1-Dichloroethene-d2	2.306	65	37110	52.338	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	104.680%
21) 2-Butanone-d5	4.458	46	131613	105.230	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.230%
24) Chloroform-d	5.056	84	176188	50.735	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.460%
26) 1,2-Dichloroethane-d4	5.952	65	124101	53.186	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.380%
32) Benzene-d6	5.970	84	333734	54.842	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.680%
36) 1,2-Dichloropropane-d6	7.305	67	107035	56.503	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	113.000%
41) Toluene-d8	8.647	98	299396	53.738	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.480%
43) trans-1,3-Dichloroprop...	8.952	79	51108	51.283	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	102.560%
47) 2-Hexanone-d5	9.384	63	106480	113.334	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	113.330%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	152052	53.918	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	107.840%
66) 1,2-Dichlorobenzene-d4	12.317	152	109347	55.211	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.420%
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.319	96	2954	1.936	ug/L #	1
14) Carbon disulfide	2.508	76	14804	3.945	ug/L	98
15) Methyl Acetate	2.703	43	1906	0.899	ug/L	91
16) Methylene chloride	2.788	84	2614	1.479	ug/L	89
17) trans-1,2-Dichloroethene	3.093	96	4121	2.569	ug/L	98
20) cis-1,2-Dichloroethene	4.483	96	3066	1.602	ug/L	90
31) Carbon tetrachloride	5.672	117	2696	1.062	ug/L	100
35) Methylcyclohexane	7.385	83	3807	1.377	ug/L	97
37) 1,2-Dichloropropane	7.434	63	1838	1.055	ug/L #	86
39) cis-1,3-Dichloropropene	8.372	75	4828	1.676	ug/L	89
42) Toluene	8.720	91	12203	1.763	ug/L	95
44) trans-1,3-Dichloropropene	8.982	75	5754	2.133	ug/L	91
46) Tetrachloroethene	9.275	164	3492	2.712	ug/L	97
48) 2-Hexanone	9.433	43	4263	2.056	ug/L #	95
49) Dibromochloromethane	9.525	129	2190	1.233	ug/L	99
50) 1,2-Dibromoethane	9.610	107	2806	1.464	ug/L	100
51) Chlorobenzene	10.079	112	12019	2.629	ug/L	96
52) Ethylbenzene	10.195	91	17937	2.309	ug/L	99
53) m,p-Xylene	10.305	106	7026	2.419	ug/L	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043513.D
 Acq On : 25 Oct 2024 10:57
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 26 00:11:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 26 00:05:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


54) o-Xylene	10.640	106	6062	2.084	ug/L	99
55) Styrene	10.659	104	12184	2.493	ug/L	91
57) 1,1,2,2-Tetrachloroethane	11.207	83	4615	1.630	ug/L #	81
59) Bromoform	10.799	173	1630	1.385	ug/L #	96
60) Isopropylbenzene	10.963	105	16202	2.161	ug/L	97
61) 1,2,3-Trichloropropane	11.238	75	3131	1.444	ug/L	96
62) 1,3,5-Trimethylbenzene	11.451	105	15570	2.532	ug/L	99
63) 1,2,4-Trimethylbenzene	11.750	105	17474	2.838	ug/L	96
64) 1,3-Dichlorobenzene	11.969	146	14127	4.341	ug/L	94
65) 1,4-Dichlorobenzene	12.042	146	15951	4.814	ug/L	97
67) 1,2-Dichlorobenzene	12.335	146	11421	3.530	ug/L	95
68) 1,2-Dibromo-3-chloropr...	12.945	75	1186	1.929	ug/L #	86
69) 1,3,5-Trichlorobenzene	13.115	180	10599	4.848	ug/L	98
70) 1,2,4-trichlorobenzene	13.585	180	12176	5.946	ug/L	99
71) Naphthalene	13.774	128	32710	4.230	ug/L	99
72) 1,2,3-Trichlorobenzene	13.963	180	11252	5.491	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043513.D
Acq On : 25 Oct 2024 10:57
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Oct 26 00:11:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 26 00:05:57 2024
Response via : Initial Calibration




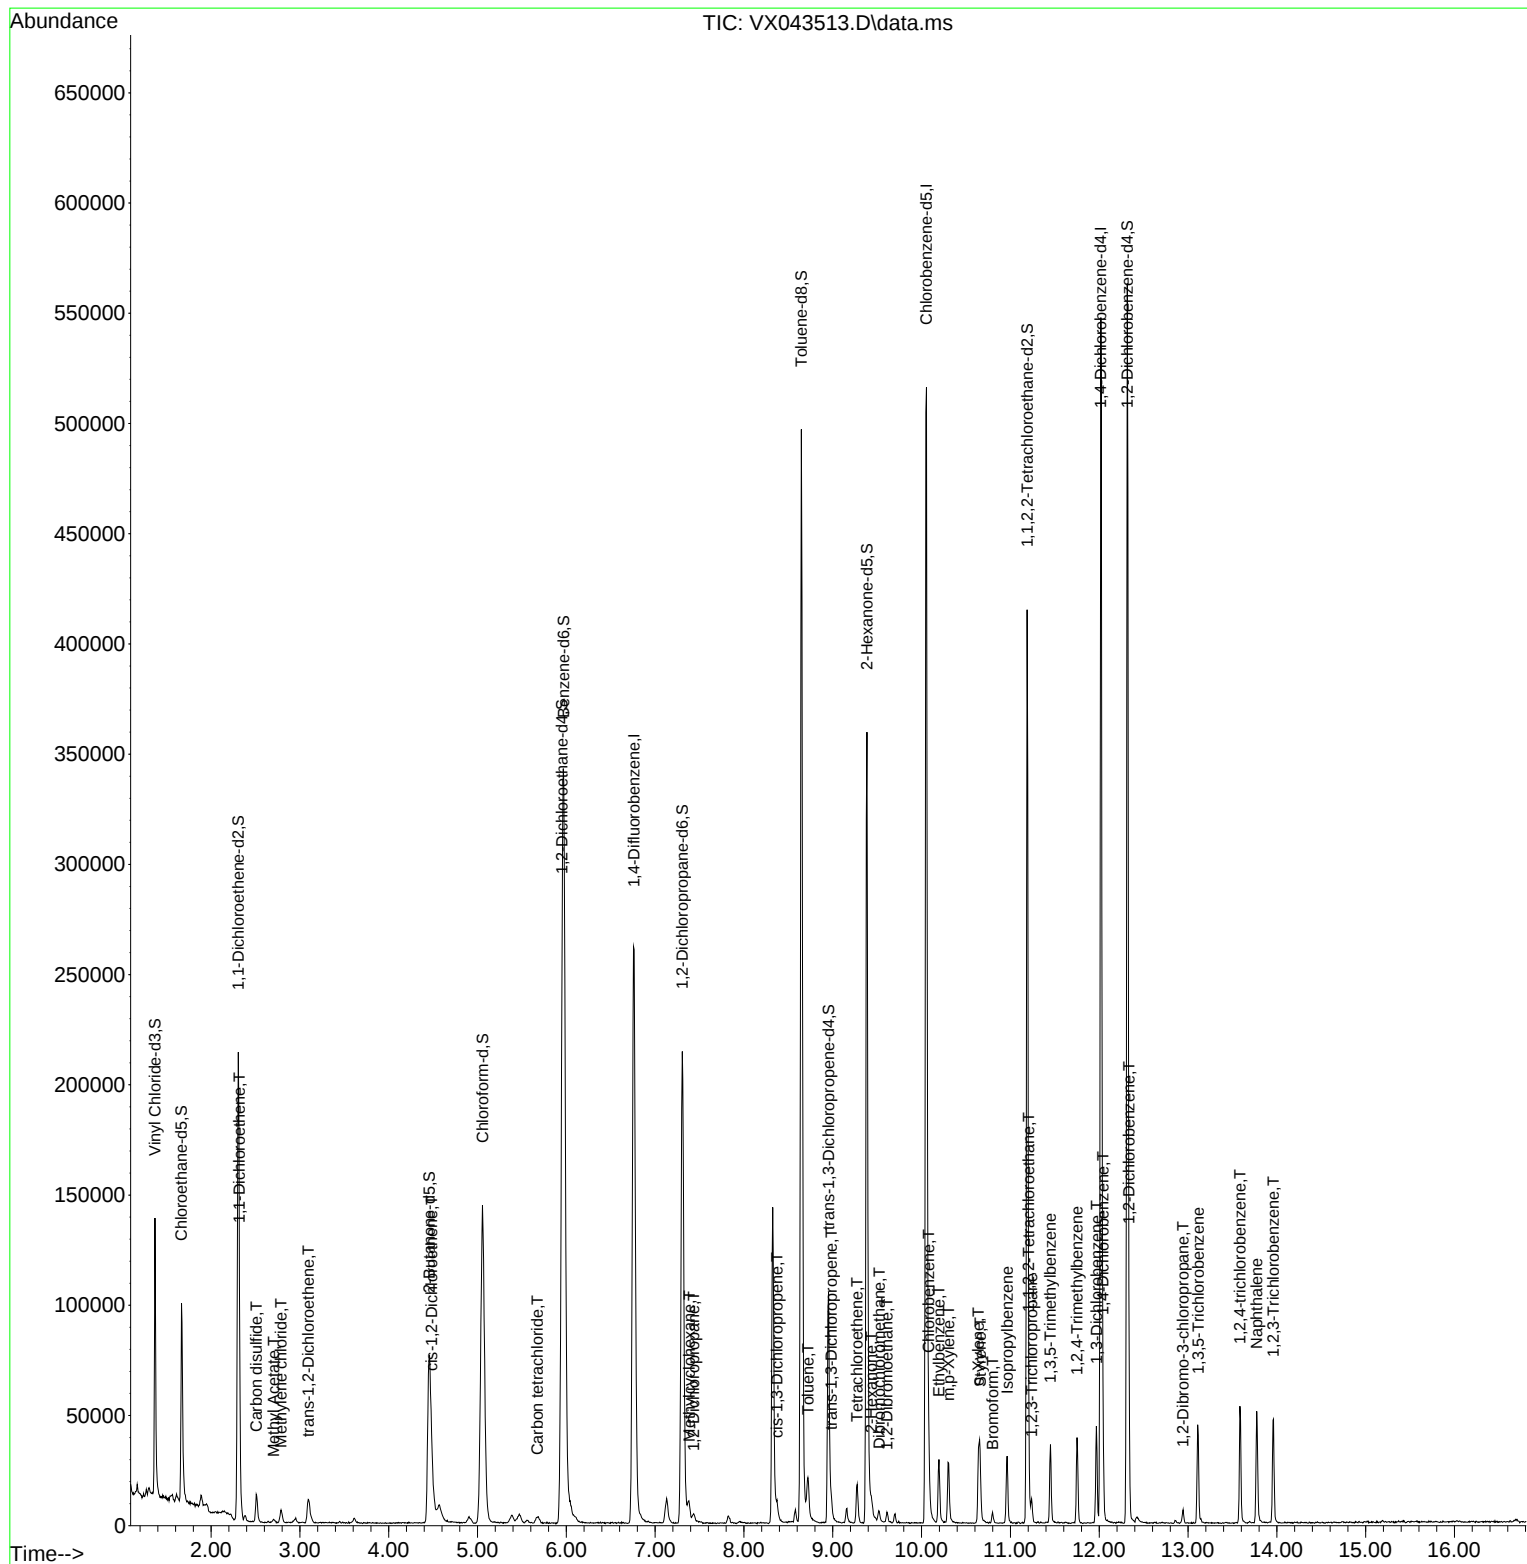




#12
1,1-Dichloroethene
Concen: 1.936 ug/L
RT: 2.319 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 96 Resp: 2954
Ion Ratio Lower Upper
96 100
61 386.8 119.8 222.6#
63 2017.2 85.0 158.0#

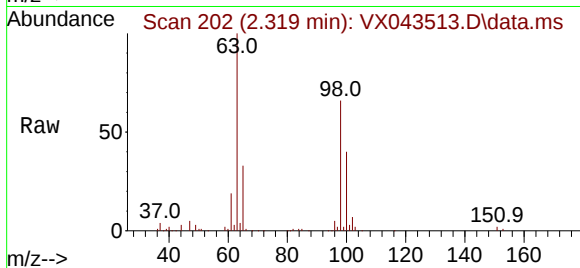

#14
Carbon disulfide
Concen: 3.945 ug/L
RT: 2.508 min Scan# 233
Delta R.T. -0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57

Tgt Ion: 76 Resp: 14804
Ion Ratio Lower Upper
76 100
78 10.0 7.5 11.3

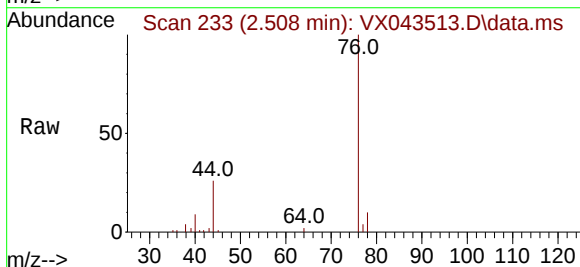



#15

Methyl Acetate

Concen: 0.899 ug/L

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 1906

Ion Ratio Lower Upper

43 100

74 19.0 18.7 28.1

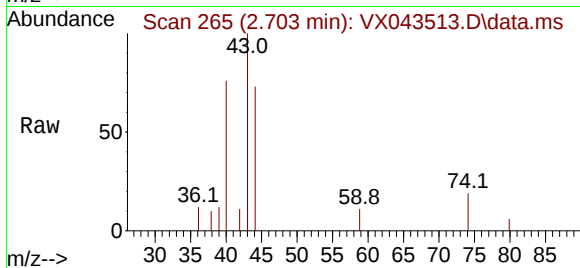

#16

Methylene chloride

Concen: 1.479 ug/L

RT: 2.788 min Scan# 279

Delta R.T. 0.000 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57




Tgt Ion: 84 Resp: 2614


Ion Ratio Lower Upper

84 100

86 48.3 44.7 82.9

49 116.1 86.2 160.2



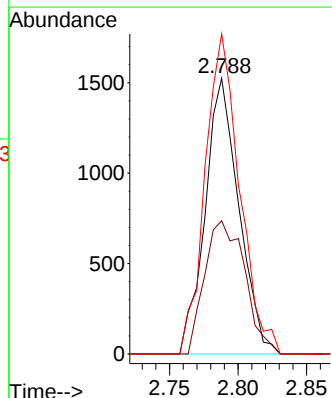
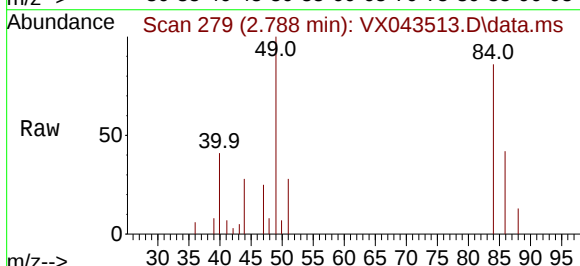




#17
trans-1,2-Dichloroethene
Concen: 2.569 ug/L
RT: 3.093 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 96 Resp: 4121
Ion Ratio Lower Upper
96 100
61 135.9 94.3 175.1
98 66.8 44.3 82.3

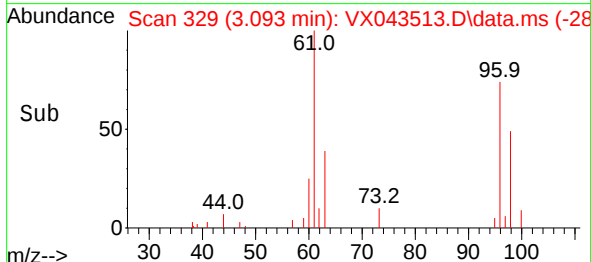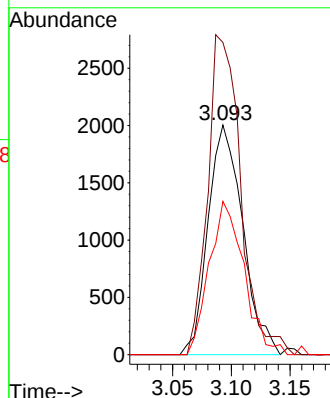

#20
cis-1,2-Dichloroethene
Concen: 1.602 ug/L
RT: 4.483 min Scan# 557
Delta R.T. -0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57


Tgt Ion: 96 Resp: 3066
Ion Ratio Lower Upper
96 100
61 114.6 87.9 163.3
98 53.9 44.0 81.6

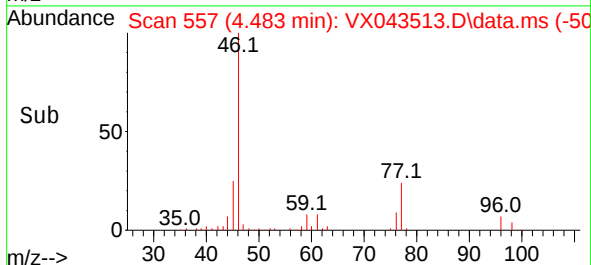






#31
Carbon tetrachloride
Concen: 1.062 ug/L
RT: 5.672 min Scan# 752
Delta R.T. -0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:117 Resp: 2696
Ion Ratio Lower Upper
117 100
119 97.8 78.0 117.0

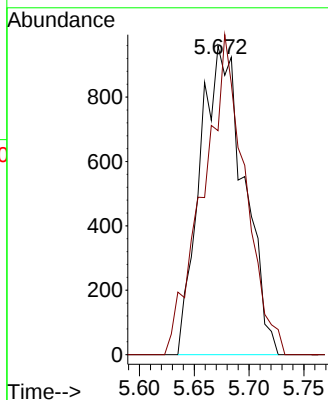


#35
Methylcyclohexane
Concen: 1.377 ug/L
RT: 7.385 min Scan# 1033
Delta R.T. 0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57



Tgt Ion: 83 Resp: 3807
Ion Ratio Lower Upper
83 100
55 79.8 60.6 91.0
98 50.4 41.0 61.6



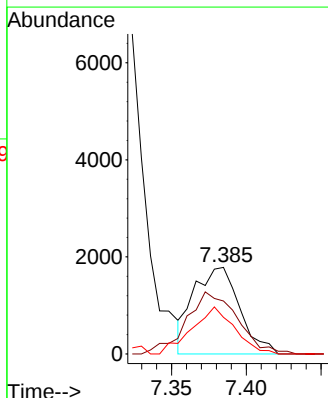
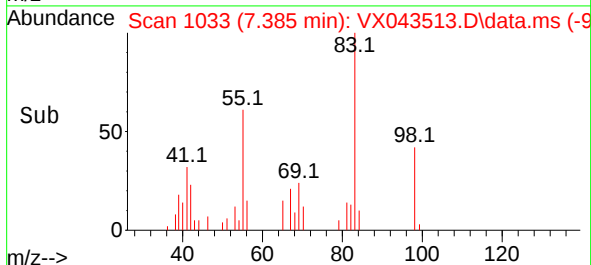




#37
1,2-Dichloropropane
Concen: 1.055 ug/L
RT: 7.434 min Scan# 1195
Delta R.T. 0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 63 Resp: 1838
Ion Ratio Lower Upper
63 100
112 0.0 3.7 5.5#



#39
cis-1,3-Dichloropropene
Concen: 1.676 ug/L
RT: 8.372 min Scan# 1195
Delta R.T. 0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57

Tgt Ion: 75 Resp: 4828
Ion Ratio Lower Upper
75 100
77 25.1 21.6 40.2

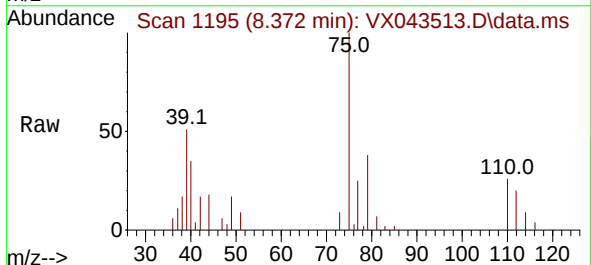

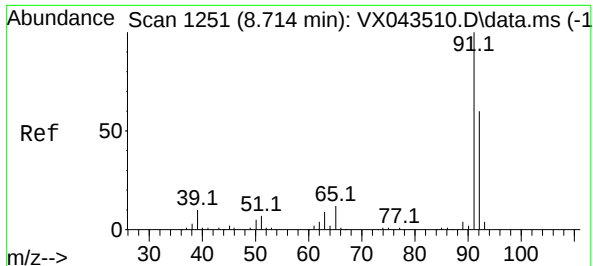

#42

Toluene

Concen: 1.763 ug/L

RT: 8.720 min Scan# 1252

Delta R.T. 0.006 min MSVOA_X

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 12203

Ion Ratio Lower Upper

91 100

92 63.7 42.1 78.1

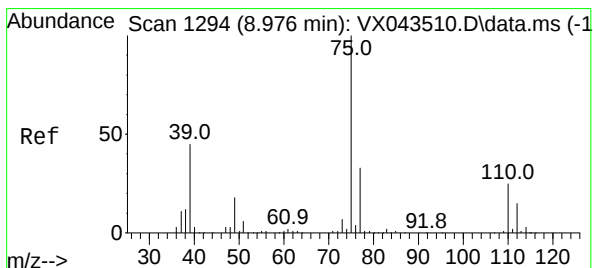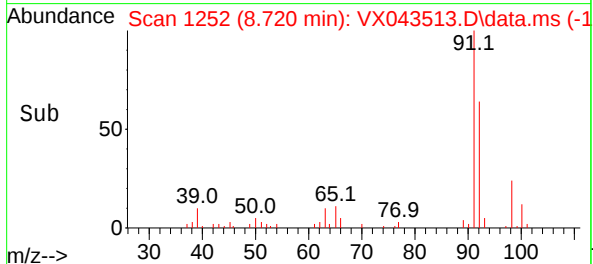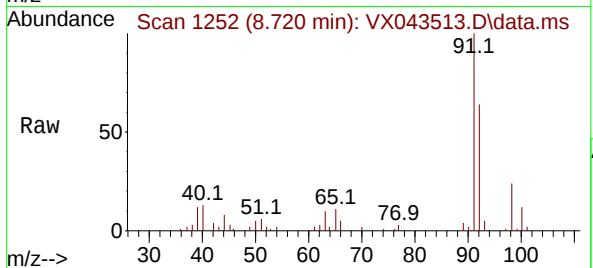

#44

trans-1,3-Dichloropropene

Concen: 2.133 ug/L

RT: 8.982 min Scan# 1295

Delta R.T. 0.006 min

Lab File: VX043513.D




Acq: 25 Oct 2024 10:57


Tgt Ion: 75 Resp: 5754

Ion Ratio Lower Upper

75 100

77 27.9 22.9 42.5

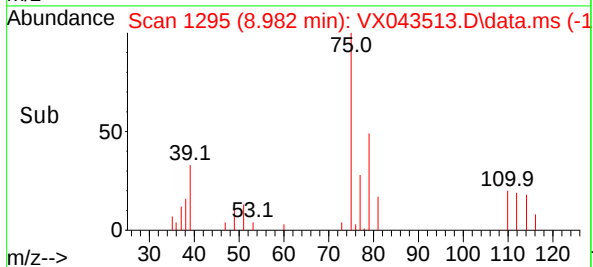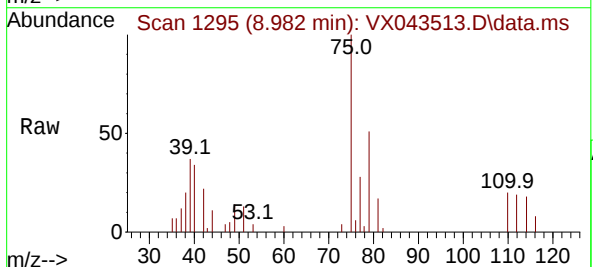



#46

Tetrachloroethene

Concen: 2.712 ug/L

RT: 9.275 min Scan# 1343

Delta R.T. 0.006 min


Lab File: VX043513.D

Acq: 25 Oct 2024 10:57

Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion:164 Resp: 3492




Ion Ratio Lower Upper

164 100

129 92.2 69.9 129.9

131 90.0 64.0 119.0

166 121.8 84.7 157.3



#48

2-Hexanone

Concen: 2.056 ug/L

RT: 9.433 min Scan# 1369

Delta R.T. 0.006 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57

Tgt Ion: 43 Resp: 4263




Ion Ratio Lower Upper


43 100

58 57.6 44.6 67.0

57 26.2 16.2 24.2#

100 14.6 10.7 16.1

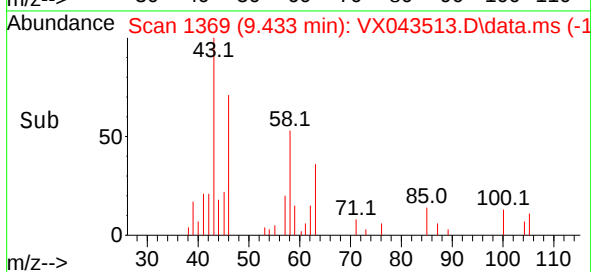



#49

Dibromochloromethane

Concen: 1.233 ug/L

RT: 9.525 min Scan# 1384

Delta R.T. 0.006 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:129 Resp: 2190

Ion Ratio Lower Upper

129 100

127 78.4 54.0 100.4

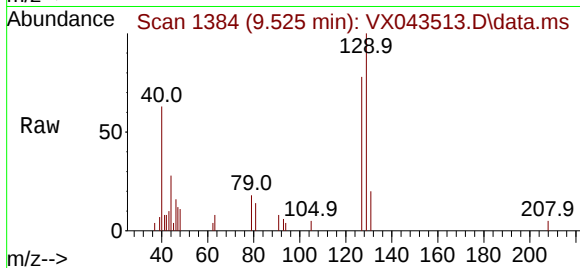

#50

1,2-Dibromoethane

Concen: 1.464 ug/L

RT: 9.610 min Scan# 1398

Delta R.T. 0.000 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57




Tgt Ion:107 Resp: 2806


Ion Ratio Lower Upper

107 100

109 92.9 65.0 120.6

188 2.9 2.8 4.2




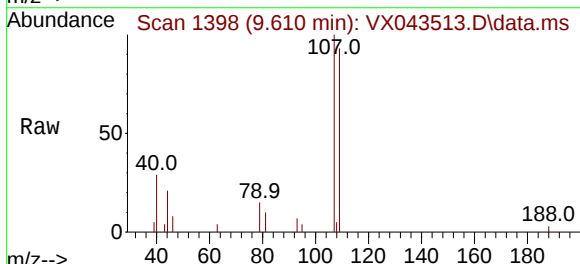




#51
Chlorobenzene
Concen: 2.629 ug/L
RT: 10.079 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:112 Resp: 12019
Ion Ratio Lower Upper
112 100
114 31.7 23.4 43.4
77 60.6 46.1 69.1



#52
Ethylbenzene
Concen: 2.309 ug/L
RT: 10.195 min Scan# 1494
Delta R.T. 0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57

Tgt Ion: 91 Resp: 17937
Ion Ratio Lower Upper
91 100
106 30.6 20.9 38.7



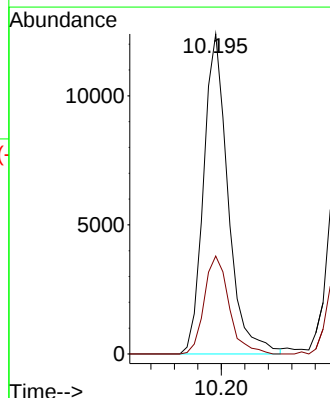





#53
m,p-Xylene
Concen: 2.419 ug/L
RT: 10.305 min Scan# 1511
Delta R.T. 0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 7026
Ion Ratio Lower Upper
106 100
91 218.0 149.0 276.8



#54
o-Xylene
Concen: 2.084 ug/L
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57

Tgt Ion:106 Resp: 6062
Ion Ratio Lower Upper
106 100
91 219.4 152.9 284.1





#55

Styrene

Concen: 2.493 ug/L

RT: 10.659 min Scan# 1569

Delta R.T. 0.006 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:104 Resp: 12184

Ion Ratio Lower Upper

104 100

78 41.1 32.8 61.0



#57

1,1,2,2-Tetrachloroethane

Concen: 1.630 ug/L

RT: 11.207 min Scan# 1660

Delta R.T. 0.000 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57




Tgt Ion: 83 Resp: 4615


Ion Ratio Lower Upper

83 100

85 77.6 44.7 82.9


131 20.0 8.2 12.4#








#59
Bromoform
Concen: 1.385 ug/L
RT: 10.799 min Scan# 1593
Delta R.T. 0.000 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:173 Resp: 1630
Ion Ratio Lower Upper
173 100
175 49.9 38.4 57.6
254 12.4 6.6 9.8#




#60
Isopropylbenzene
Concen: 2.161 ug/L
RT: 10.963 min Scan# 1620
Delta R.T. 0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57



Tgt Ion:105 Resp: 16202
Ion Ratio Lower Upper
105 100
120 25.7 21.0 31.4
77 18.3 12.6 19.0

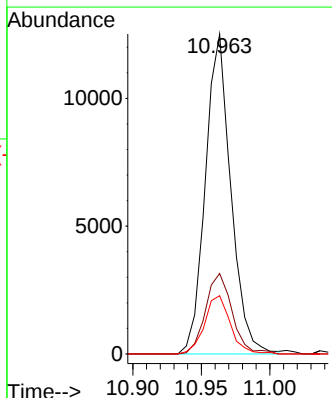



#61

1,2,3-Trichloropropane

Concen: 1.444 ug/L

RT: 11.238 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX043513.D





Acq: 25 Oct 2024 10:57

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 75	Resp:	3131
Ion Ratio	Lower	Upper
75	100	
77	28.3	25.5 38.3
110	42.9	33.3 49.9

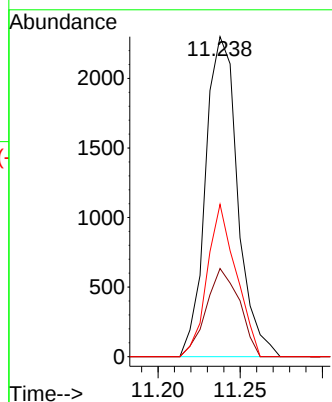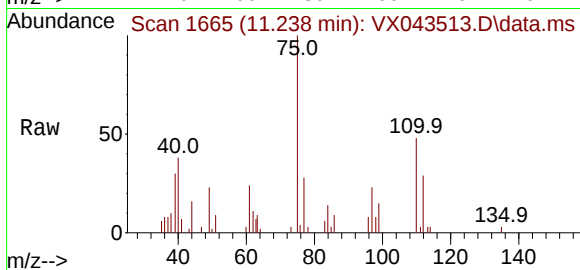

#62

1,3,5-Trimethylbenzene

Concen: 2.532 ug/L




RT: 11.451 min Scan# 1700


Delta R.T. 0.000 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57

Tgt Ion: 105	Resp:	15570
Ion Ratio	Lower	Upper
105	100	
120	48.2	38.3 57.5

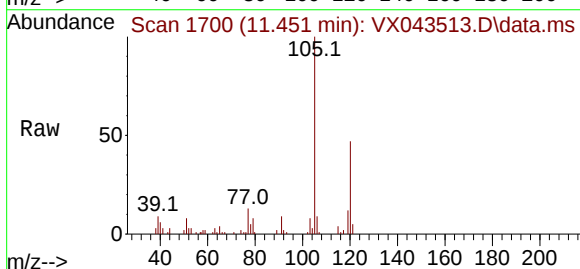



#63

1,2,4-Trimethylbenzene

Concen: 2.838 ug/L

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 17474

Ion Ratio Lower Upper

105 100

120 42.1 35.8 53.8



#64

1,3-Dichlorobenzene

Concen: 4.341 ug/L

RT: 11.969 min Scan# 1785

Delta R.T. 0.000 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57




Tgt Ion:146 Resp: 14127


Ion Ratio Lower Upper

146 100

111 41.8 28.6 53.0

148 58.8 45.8 85.0

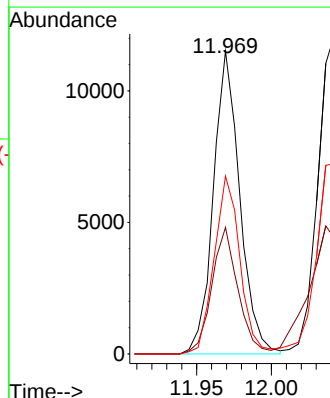



#65

1,4-Dichlorobenzene

Concen: 4.814 ug/L

RT: 12.042 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:146 Resp: 15951

Ion Ratio Lower Upper

146 100

111 36.1 26.8 49.8

148 59.4 43.4 80.6

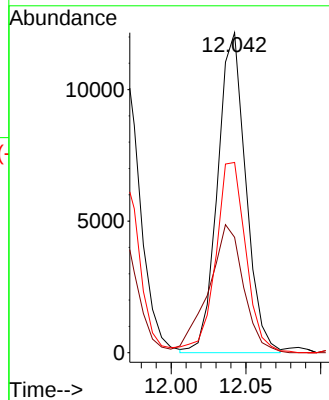

#67

1,2-Dichlorobenzene

Concen: 3.530 ug/L

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX043513.D

Acq: 25 Oct 2024 10:57




Tgt Ion:146 Resp: 11421


Ion Ratio Lower Upper

146 100

111 46.4 34.6 51.8

148 64.4 48.2 72.4



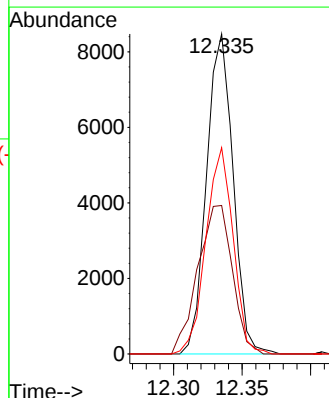



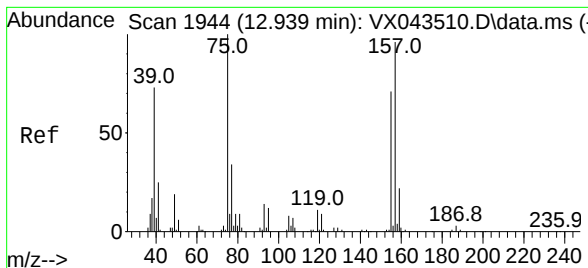

#68
1,2-Dibromo-3-chloropropane
Concen: 1.929 ug/L
RT: 12.945 min Scan# 1945
Delta R.T. 0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 1186
Ion Ratio Lower Upper
75 100
155 85.7 56.9 85.3#
157 107.1 76.8 115.2

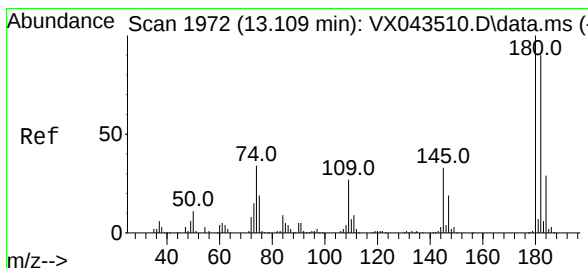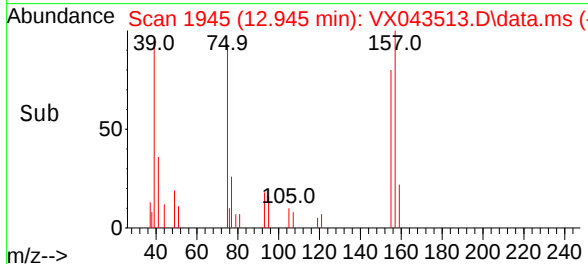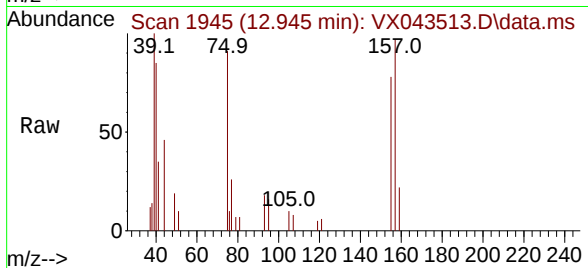

#69
1,3,5-Trichlorobenzene
Concen: 4.848 ug/L
RT: 13.115 min Scan# 1973
Delta R.T. 0.006 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57


Tgt Ion:180 Resp: 10599
Ion Ratio Lower Upper
180 100
182 95.5 74.1 111.1
184 30.1 23.1 34.7
145 32.8 25.9 38.9

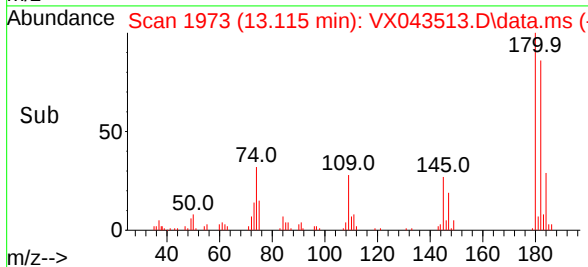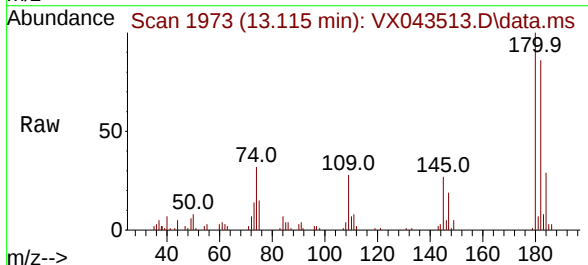






#70
1,2,4-trichlorobenzene
Concen: 5.946 ug/L
RT: 13.585 min Scan# 2050
Delta R.T. 0.000 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:180 Resp: 12176
Ion Ratio Lower Upper
180 100
182 93.0 74.9 112.3
145 32.7 26.6 40.0




#71
Naphthalene
Concen: 4.230 ug/L
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX043513.D
Acq: 25 Oct 2024 10:57




Tgt Ion:128 Resp: 32710
Ion Ratio Lower Upper
128 100
127 12.7 10.1 15.1
129 10.3 8.7 13.1

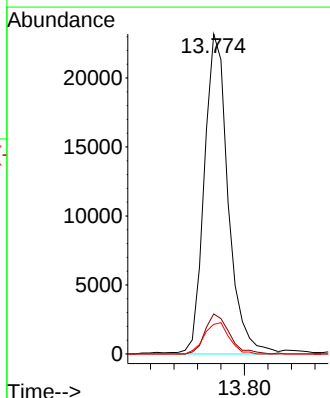



#72
 1,2,3-Trichlorobenzene
 Concen: 5.491 ug/L
 RT: 13.963 min Scan# 2112
 Delta R.T. 0.006 min
 Lab File: VX043513.D
 Acq: 25 Oct 2024 10:57

Instrument :
 MSVOA_X
 ClientSampleId :



Tgt Ion:180 Resp: 11252
 Ion Ratio Lower Upper
 180 100
 182 90.7 77.4 116.0
 145 35.6 28.6 43.0

