

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043521.D
 Acq On : 25 Oct 2024 14:29
 Operator : JC/MD
 Sample : P4436-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FE9

Quant Time: Oct 26 01:36:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 26 01:33:53 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	294694	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	271188	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	122656	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	88352	55.113	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 110.220%	
7) Chloroethane-d5	1.666	69	73779	57.468	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	= 114.940%	
11) 1,1-Dichloroethene-d2	2.306	65	41655	55.024	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 110.040%	
21) 2-Butanone-d5	4.452	46	137666	103.093	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	= 103.090%	
24) Chloroform-d	5.056	84	197277	53.207	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 106.420%	
26) 1,2-Dichloroethane-d4	5.952	65	134361	53.933	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 107.860%	
32) Benzene-d6	5.970	84	383413	55.696	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 111.400%	
36) 1,2-Dichloropropane-d6	7.306	67	117859	54.999	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	= 110.000%	
41) Toluene-d8	8.647	98	344950	54.732	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 109.460%	
43) trans-1,3-Dichloroprop...	8.952	79	53460	47.419	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 94.840%	
47) 2-Hexanone-d5	9.384	63	110661	104.119	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	= 104.120%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	165607	51.911	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	= 103.820%	
66) 1,2-Dichlorobenzene-d4	12.317	152	123652	55.542	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 111.080%	
Target Compounds						
13) Acetone	2.380	43	24500	20.152	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043521.D
Acq On : 25 Oct 2024 14:29
Operator : JC/MD
Sample : P4436-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FE9

Quant Time: Oct 26 01:36:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 26 01:33:53 2024
Response via : Initial Calibration

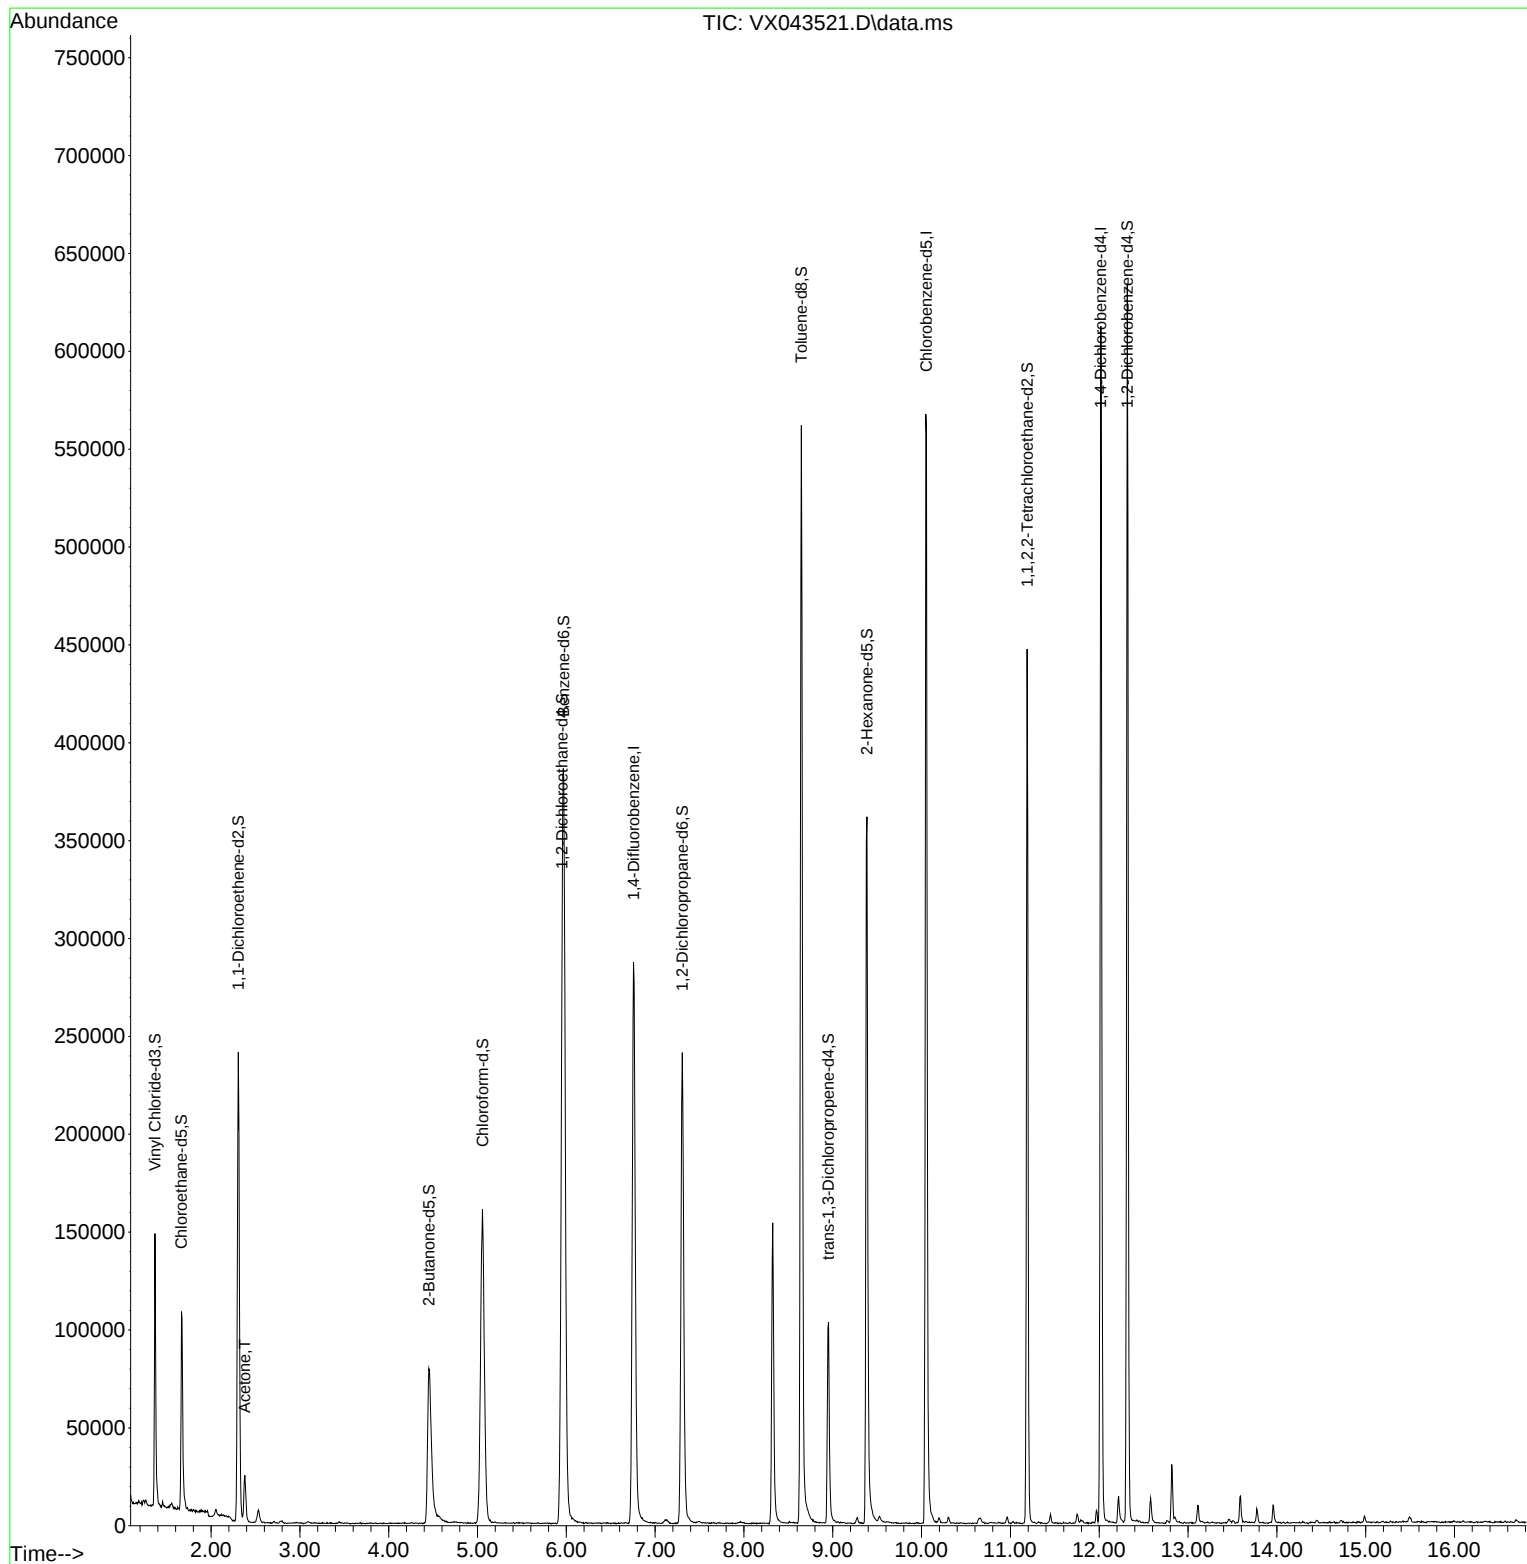

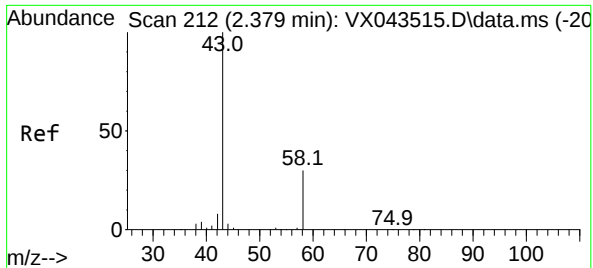

#13
 Acetone
 Concen: 20.152 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX043521.D
 Acq: 25 Oct 2024 14:29

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FE9

Tgt Ion: 43 Resp: 24500
 Ion Ratio Lower Upper
 43 100
 58 30.4 0.0 59.2

