

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043524.D
 Acq On : 25 Oct 2024 15:38
 Operator : JC/MD
 Sample : P4492-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF1

Quant Time: Oct 26 01:36:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 26 01:33:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	262362	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	232371	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	99622	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	82808	58.021	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 116.040%			
7) Chloroethane-d5	1.642	69	38016	33.261	ug/L	-0.02
Spiked Amount 50.000	Range 70 - 130		Recovery = 66.520%#			
11) 1,1-Dichloroethene-d2	2.294	65	36460	54.097	ug/L	-0.01
Spiked Amount 50.000	Range 60 - 125		Recovery = 108.200%			
21) 2-Butanone-d5	4.465	46	121396	102.112	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 102.110%			
24) Chloroform-d	5.050	84	177672	53.825	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 107.660%			
26) 1,2-Dichloroethane-d4	5.952	65	124246	56.019	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 112.040%			
32) Benzene-d6	5.964	84	354136	60.036	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 120.080%			
36) 1,2-Dichloropropane-d6	7.306	67	110554	60.208	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 120.420%#			
41) Toluene-d8	8.647	98	315740	58.466	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 116.940%			
43) trans-1,3-Dichloroprop...	8.952	79	44435	45.998	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 92.000%			
47) 2-Hexanone-d5	9.385	63	101348	111.285	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 111.290%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	158243	57.889	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 115.780%			
66) 1,2-Dichlorobenzene-d4	12.317	152	112690	62.322	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 124.640%#			
Target Compounds					Qvalue	
13) Acetone	2.392	43	17087	15.786	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043524.D
Acq On : 25 Oct 2024 15:38
Operator : JC/MD
Sample : P4492-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF1

Quant Time: Oct 26 01:36:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 26 01:33:53 2024
Response via : Initial Calibration

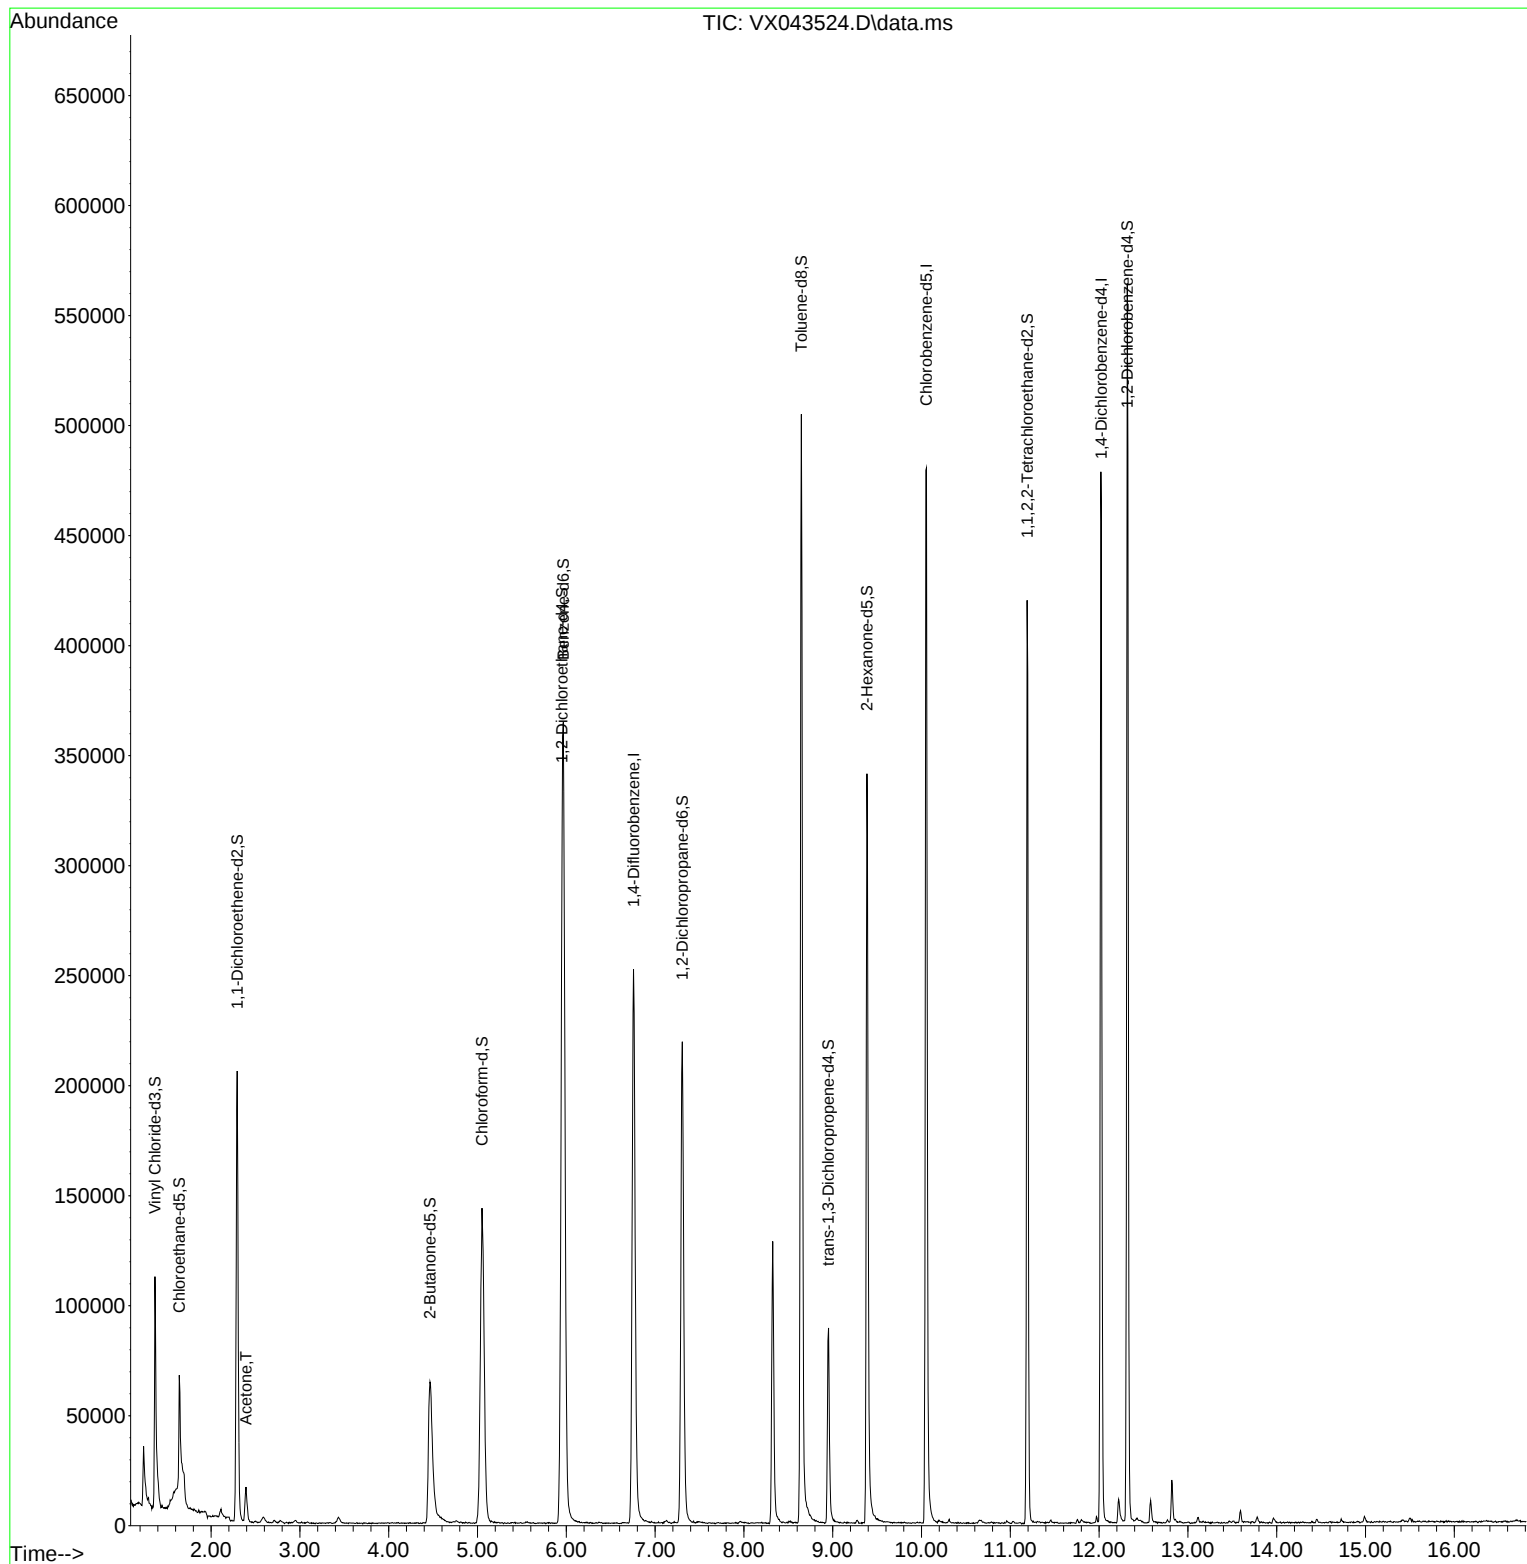

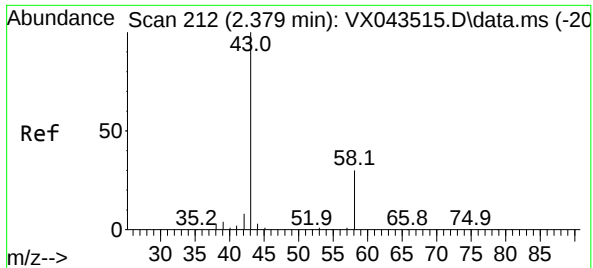

#13
 Acetone
 Concen: 15.786 ug/L
 RT: 2.392 min Scan# 21
 Delta R.T. 0.013 min
 Lab File: VX043524.D
 Acq: 25 Oct 2024 15:38

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF1

Tgt Ion: 43 Resp: 17087
 Ion Ratio Lower Upper
 43 100
 58 30.7 0.0 59.2

