

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043516.D
 Acq On : 25 Oct 2024 12:09
 Operator : JC/MD
 Sample : VX1025MBL01
 Misc : 5.00g/5mL/100ul/5mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK713

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	112622	113991	12.22%	1.425%
2	1.666	92	95	103	rVB	80797	106476	11.41%	1.331%
3	2.306	193	200	209	rBV	188324	299462	32.10%	3.744%
4	2.514	229	234	242	rVB	5186	9267	0.99%	0.116%
5	2.690	261	263	264	rBV	608	370	0.04%	0.005%
6	2.788	275	279	284	rBV3	2405	4242	0.45%	0.053%
7	3.093	324	329	337	rBV6	3635	8144	0.87%	0.102%
8	3.349	369	371	373	rVB2	471	402	0.04%	0.005%
9	3.446	382	387	392	rVB5	866	1769	0.19%	0.022%
10	3.928	463	466	467	rVV	571	466	0.05%	0.006%
11	4.074	486	490	493	rVB3	460	563	0.06%	0.007%
12	4.221	511	514	515	rBV2	401	395	0.04%	0.005%
13	4.330	530	532	535	rVB	648	513	0.05%	0.006%
14	4.355	535	536	539	rBV	801	640	0.07%	0.008%
15	4.385	539	541	542	rBV	389	401	0.04%	0.005%
16	4.458	544	553	567	rBV	74468	238176	25.53%	2.978%
17	4.824	611	613	614	rBV2	477	398	0.04%	0.005%
18	5.050	639	650	668	rVV2	125061	385447	41.32%	4.820%
19	5.294	689	690	692	rBV	572	325	0.03%	0.004%
20	5.342	694	698	700	rBV3	508	525	0.06%	0.007%
21	5.385	700	705	711	rBV4	1567	3209	0.34%	0.040%
22	5.531	726	729	730	rBV2	569	518	0.06%	0.006%
23	5.550	730	732	741	rVB4	1359	3057	0.33%	0.038%
24	5.617	741	743	745	rBV2	469	455	0.05%	0.006%
25	5.964	788	800	821	rBV2	309393	932913	100.00%	11.665%
26	6.208	839	840	842	rBV	411	397	0.04%	0.005%
27	6.348	861	863	865	rVB2	406	397	0.04%	0.005%
28	6.391	868	870	872	rVB2	457	416	0.04%	0.005%
29	6.415	872	874	875	rBV	408	325	0.03%	0.004%
30	6.507	887	889	893	rBV2	477	802	0.09%	0.010%
31	6.604	903	905	909	rVB2	600	611	0.07%	0.008%
32	6.757	921	930	945	rBV	280758	680989	73.00%	8.515%
33	7.129	985	991	1002	rVB6	4970	12116	1.30%	0.151%
34	7.251	1009	1011	1012	rBV	634	487	0.05%	0.006%
35	7.305	1012	1020	1039	rVV	189043	430476	46.14%	5.383%
36	7.744	1090	1092	1094	rVB2	584	447	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043516.D
 Acq On : 25 Oct 2024 12:09
 Operator : JC/MD
 Sample : VX1025MBL01
 Misc : 5.00g/5mL/100ul/5mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK713

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
 Title : VOC Analysis

37	7.824	1101	1105	1109	rBV5	809	1415	0.15%	0.018%
38	8.043	1140	1141	1144	rVB	498	325	0.03%	0.004%
39	8.068	1144	1145	1149	rBV2	433	494	0.05%	0.006%
40	8.165	1158	1161	1162	rVB	649	541	0.06%	0.007%
41	8.183	1162	1164	1166	rBV3	283	331	0.04%	0.004%
42	8.208	1166	1168	1172	rVV3	395	516	0.06%	0.006%
43	8.324	1181	1187	1206	rVV	135524	230042	24.66%	2.876%
44	8.574	1226	1228	1233	rVB4	1068	1152	0.12%	0.014%
45	8.647	1234	1240	1249	rBV	460971	727818	78.02%	9.100%
46	8.952	1285	1290	1305	rVB	92909	153755	16.48%	1.923%
47	9.153	1321	1323	1330	rVB3	1688	2354	0.25%	0.029%
48	9.275	1339	1343	1349	rVV2	7236	10685	1.15%	0.134%
49	9.384	1356	1361	1378	rBV	351189	524194	56.19%	6.554%
50	9.695	1408	1412	1418	rBV4	1640	2431	0.26%	0.030%
51	9.762	1421	1423	1424	rBV	471	402	0.04%	0.005%
52	9.823	1431	1433	1435	rBV	486	468	0.05%	0.006%
53	9.951	1451	1454	1457	rBV2	364	554	0.06%	0.007%
54	10.055	1465	1471	1488	rBV	554669	830928	89.07%	10.390%
55	10.195	1490	1494	1499	rVB	9998	13754	1.47%	0.172%
56	10.299	1507	1511	1516	rBV	9783	13953	1.50%	0.174%
57	10.396	1525	1527	1528	rVB2	659	388	0.04%	0.005%
58	10.427	1530	1532	1535	rVB2	465	437	0.05%	0.005%
59	10.451	1535	1536	1539	rBV2	281	321	0.03%	0.004%
60	10.604	1559	1561	1562	rBV	754	590	0.06%	0.007%
61	10.659	1563	1570	1579	rVB2	13026	28337	3.04%	0.354%
62	10.799	1590	1593	1597	rVB4	1639	2041	0.22%	0.026%
63	10.884	1605	1607	1609	rBV	564	581	0.06%	0.007%
64	10.963	1615	1620	1627	rBV	11967	16108	1.73%	0.201%
65	11.018	1627	1629	1631	rBV2	312	351	0.04%	0.004%
66	11.079	1636	1639	1640	rBV3	577	474	0.05%	0.006%
67	11.189	1652	1657	1664	rBV	378305	491334	52.67%	6.144%
68	11.354	1682	1684	1685	rBV	585	373	0.04%	0.005%
69	11.451	1696	1700	1706	rVV	14582	18739	2.01%	0.234%
70	11.536	1710	1714	1716	rBV2	321	501	0.05%	0.006%
71	11.683	1736	1738	1740	rVB2	460	358	0.04%	0.004%
72	11.707	1740	1742	1744	rVB	394	341	0.04%	0.004%
73	11.750	1745	1749	1756	rVB	16163	20560	2.20%	0.257%
74	11.860	1764	1767	1770	rBV3	477	740	0.08%	0.009%
75	11.933	1777	1779	1781	rBV2	368	373	0.04%	0.005%
76	11.969	1781	1785	1788	rBV	19980	25221	2.70%	0.315%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043516.D
 Acq On : 25 Oct 2024 12:09
 Operator : JC/MD
 Sample : VX1025MBL01
 Misc : 5.00g/5mL/100ul/5ml/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK713

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1806	rVB	626270	795343	85.25%	9.945%
78	12.219	1824	1826	1827	rBV2	520	447	0.05%	0.006%
79	12.317	1837	1842	1854	rBV	540214	696539	74.66%	8.709%
80	12.762	1910	1915	1920	rVB4	970	1694	0.18%	0.021%
81	12.872	1928	1933	1936	rVV3	759	1240	0.13%	0.016%
82	12.945	1940	1945	1949	rVV3	1901	2790	0.30%	0.035%
83	13.006	1953	1955	1958	rBV2	513	556	0.06%	0.007%
84	13.115	1967	1973	1980	rBV	21835	30387	3.26%	0.380%
85	13.219	1989	1990	1992	rVB	562	354	0.04%	0.004%
86	13.250	1992	1995	1996	rBV2	362	397	0.04%	0.005%
87	13.341	2009	2010	2014	rBV4	509	487	0.05%	0.006%
88	13.585	2046	2050	2057	rBV	27296	34508	3.70%	0.431%
89	13.634	2057	2058	2060	rVB2	745	322	0.03%	0.004%
90	13.695	2065	2068	2069	rBV2	894	780	0.08%	0.010%
91	13.737	2072	2075	2077	rBV2	332	373	0.04%	0.005%
92	13.774	2077	2081	2089	rBV	22960	31217	3.35%	0.390%
93	13.963	2107	2112	2120	rVB	22372	30600	3.28%	0.383%
94	14.127	2135	2139	2143	rVB4	1671	2470	0.26%	0.031%
95	14.176	2145	2147	2148	rVV	530	402	0.04%	0.005%
96	14.341	2172	2174	2178	rVB3	807	707	0.08%	0.009%
97	14.396	2182	2183	2187	rBV2	553	662	0.07%	0.008%
98	14.444	2187	2191	2192	rBV	349	424	0.05%	0.005%
99	15.011	2282	2284	2286	rVB2	831	643	0.07%	0.008%
100	15.188	2311	2313	2314	rBV2	596	408	0.04%	0.005%




Sum of corrected areas: 7997617

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043516.D
Acq On : 25 Oct 2024 12:09
Operator : JC/MD
Sample : VX1025MBL01
Misc : 5.00g/5mL/100ul/5mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK713

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

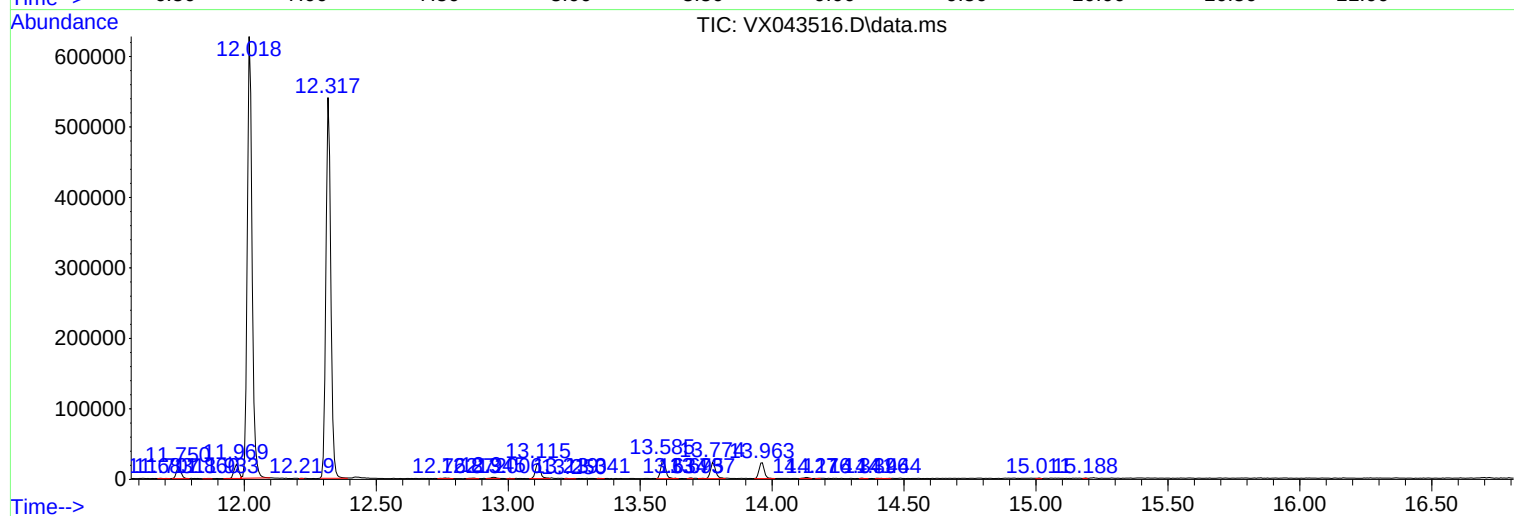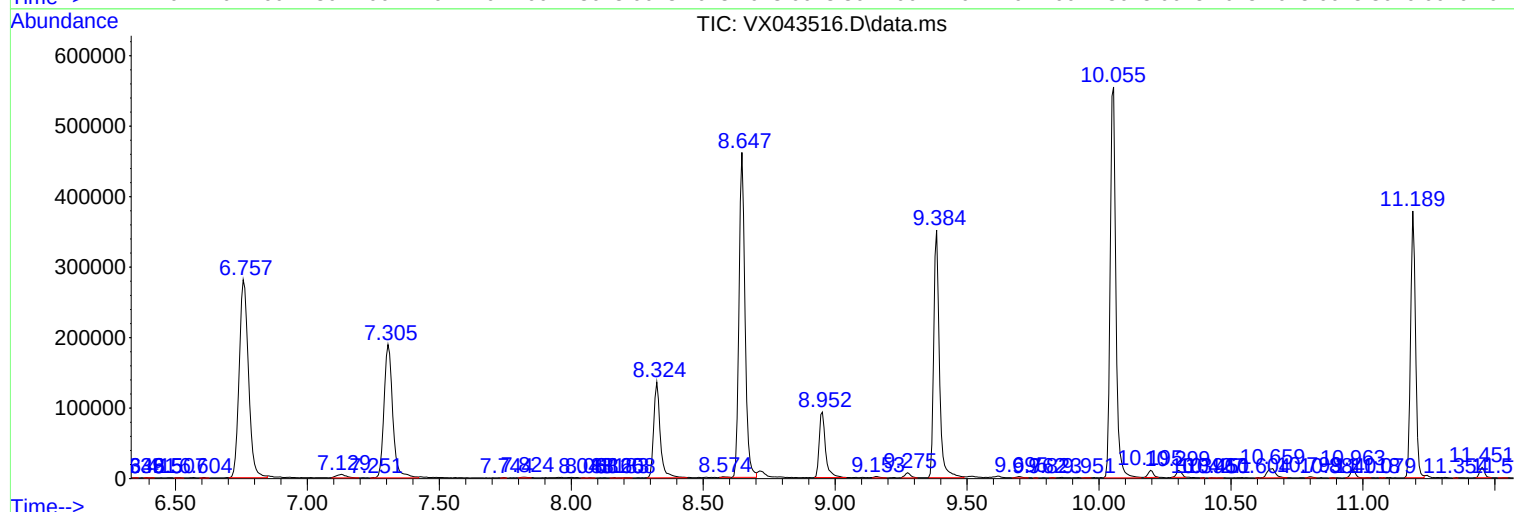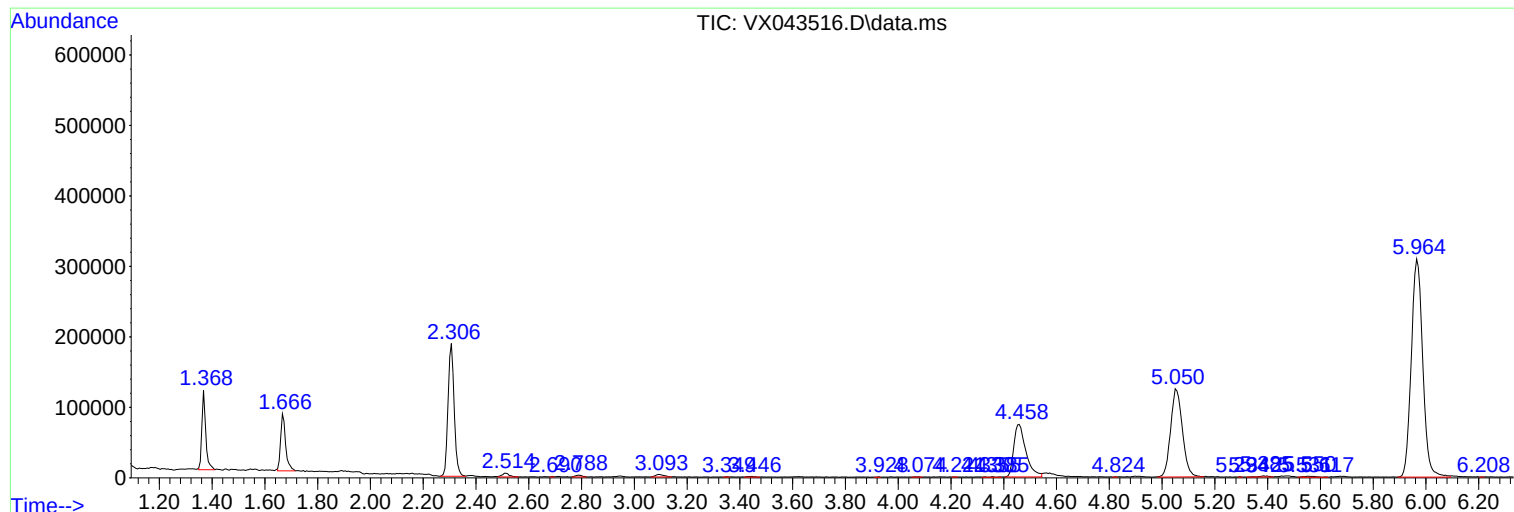

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043516.D
Acq On : 25 Oct 2024 12:09
Operator : JC/MD
Sample : VX1025MBL01
Misc : 5.00g/5mL/100ul/5ml/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK713

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043516.D
Acq On : 25 Oct 2024 12:09
Operator : JC/MD
Sample : VX1025MBL01
Misc : 5.00g/5mL/100ul/5ml/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK713

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc