

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043520.D
 Acq On : 25 Oct 2024 14:06
 Operator : JC/MD
 Sample : P4415-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	29	rBV	11202	16273	1.74%	0.217%
2	1.368	43	46	56	rVB	108715	112699	12.08%	1.506%
3	1.666	91	95	107	rVB	80473	107144	11.49%	1.432%
4	2.306	194	200	209	rBV	177743	277888	29.79%	3.714%
5	2.465	224	226	228	rVB2	535	352	0.04%	0.005%
6	2.514	228	234	240	rVB3	2027	3671	0.39%	0.049%
7	2.703	261	265	267	rBV4	603	654	0.07%	0.009%
8	2.788	275	279	284	rVV3	1428	2648	0.28%	0.035%
9	2.831	284	286	288	rVV2	485	398	0.04%	0.005%
10	2.873	290	293	294	rBV2	704	519	0.06%	0.007%
11	2.941	297	304	313	rVV	11068	27177	2.91%	0.363%
12	3.026	316	318	320	rVV2	394	429	0.05%	0.006%
13	3.056	322	323	324	rBV	634	350	0.04%	0.005%
14	3.093	325	329	335	rVB4	1288	2470	0.26%	0.033%
15	3.361	369	373	377	rBV2	369	741	0.08%	0.010%
16	3.434	383	385	386	rBV2	663	395	0.04%	0.005%
17	3.477	390	392	395	rVB2	421	369	0.04%	0.005%
18	3.587	406	410	411	rBV3	369	449	0.05%	0.006%
19	3.636	416	418	419	rVB2	714	397	0.04%	0.005%
20	3.660	419	422	425	rBV3	511	676	0.07%	0.009%
21	3.696	425	428	430	rVB2	431	357	0.04%	0.005%
22	3.916	462	464	465	rVB2	545	350	0.04%	0.005%
23	4.227	512	515	517	rBV2	361	345	0.04%	0.005%
24	4.452	544	552	564	rBV	72912	227443	24.38%	3.040%
25	4.751	600	601	603	rBV	491	530	0.06%	0.007%
26	4.904	624	626	630	rBV3	603	808	0.09%	0.011%
27	5.050	638	650	666	rBV	123641	383792	41.15%	5.129%
28	5.446	713	715	716	rBV	555	484	0.05%	0.006%
29	5.544	727	731	734	rBV4	607	1114	0.12%	0.015%
30	5.653	746	749	752	rBV2	349	488	0.05%	0.007%
31	5.714	758	759	763	rBV2	388	483	0.05%	0.006%
32	5.842	778	780	783	rBV2	361	503	0.05%	0.007%
33	5.964	788	800	820	rBV2	306091	932727	100.00%	12.465%
34	6.202	836	839	841	rBV4	524	659	0.07%	0.009%
35	6.251	845	847	849	rBV3	383	429	0.05%	0.006%
36	6.294	852	854	858	rVB3	424	513	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043520.D
 Acq On : 25 Oct 2024 14:06
 Operator : JC/MD
 Sample : P4415-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

37	6.452	877	880	881	rBV2	337	368	0.04%	0.005%
38	6.568	896	899	900	rBV3	503	505	0.05%	0.007%
39	6.757	919	930	952	rBV	251971	621820	66.67%	8.310%
40	7.050	976	978	981	rVB2	437	394	0.04%	0.005%
41	7.117	982	989	990	rBV4	1701	3195	0.34%	0.043%
42	7.299	1011	1019	1037	rVV	186215	428088	45.90%	5.721%
43	7.476	1046	1048	1049	rBV2	600	517	0.06%	0.007%
44	7.531	1054	1057	1058	rBV2	449	327	0.04%	0.004%
45	7.671	1077	1080	1081	rVV2	472	476	0.05%	0.006%
46	7.708	1084	1086	1087	rBV	520	394	0.04%	0.005%
47	7.787	1097	1099	1100	rBV2	409	368	0.04%	0.005%
48	7.830	1103	1106	1108	rBV2	532	797	0.09%	0.011%
49	7.927	1119	1122	1123	rBV	369	382	0.04%	0.005%
50	7.958	1125	1127	1132	rVV2	728	1135	0.12%	0.015%
51	8.080	1146	1147	1151	rVB3	558	488	0.05%	0.007%
52	8.116	1151	1153	1155	rBV2	377	435	0.05%	0.006%
53	8.324	1179	1187	1197	rBV	110610	195927	21.01%	2.618%
54	8.482	1212	1213	1218	rBV3	512	904	0.10%	0.012%
55	8.647	1233	1240	1249	rBV	434006	717849	76.96%	9.594%
56	8.946	1284	1289	1299	rVV	82500	129180	13.85%	1.726%
57	9.220	1332	1334	1338	rBV2	406	519	0.06%	0.007%
58	9.269	1338	1342	1348	rVV5	2758	4737	0.51%	0.063%
59	9.384	1355	1361	1375	rBV	325791	512779	54.98%	6.853%
60	9.689	1407	1411	1416	rBV5	2713	4329	0.46%	0.058%
61	9.762	1422	1423	1427	rVB3	529	560	0.06%	0.007%
62	10.012	1462	1464	1465	rBV	525	348	0.04%	0.005%
63	10.049	1465	1470	1487	rVV	501839	740435	79.38%	9.896%
64	10.195	1490	1494	1499	rVB3	2410	3805	0.41%	0.051%
65	10.305	1507	1512	1519	rBV3	3012	4905	0.53%	0.066%
66	10.354	1519	1520	1523	rBV2	512	392	0.04%	0.005%
67	10.433	1531	1533	1535	rBV2	305	319	0.03%	0.004%
68	10.457	1535	1537	1540	rBV3	395	512	0.05%	0.007%
69	10.500	1542	1544	1546	rVB3	447	389	0.04%	0.005%
70	10.518	1546	1547	1550	rBV2	543	505	0.05%	0.007%
71	10.543	1550	1551	1552	rBV	658	326	0.03%	0.004%
72	10.659	1564	1570	1576	rVV5	3868	8190	0.88%	0.109%
73	10.915	1608	1612	1614	rVB2	610	705	0.08%	0.009%
74	10.963	1615	1620	1624	rBV2	3914	5291	0.57%	0.071%
75	11.006	1626	1627	1630	rBV2	508	341	0.04%	0.005%
76	11.134	1646	1648	1651	rBV3	374	429	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043520.D
 Acq On : 25 Oct 2024 14:06
 Operator : JC/MD
 Sample : P4415-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	11.189	1652	1657	1670	rVV	383657	492031	52.75%	6.576%
78	11.451	1696	1700	1709	rBV2	4707	6713	0.72%	0.090%
79	11.677	1735	1737	1739	rVB3	628	447	0.05%	0.006%
80	11.713	1739	1743	1744	rBV2	676	644	0.07%	0.009%
81	11.750	1746	1749	1754	rVB2	6140	7365	0.79%	0.098%
82	11.817	1758	1760	1763	rBV2	485	472	0.05%	0.006%
83	11.847	1763	1765	1767	rBV2	373	404	0.04%	0.005%
84	11.969	1782	1785	1788	rBV2	6302	6998	0.75%	0.094%
85	12.018	1788	1793	1809	rVB	564464	718389	77.02%	9.601%
86	12.213	1819	1825	1827	rBV6	937	2070	0.22%	0.028%
87	12.317	1837	1842	1856	rBV	544092	689822	73.96%	9.219%
88	12.542	1878	1879	1882	rBV2	702	641	0.07%	0.009%
89	12.591	1886	1887	1888	rVV	835	385	0.04%	0.005%
90	12.634	1892	1894	1896	rVB	1191	850	0.09%	0.011%
91	12.677	1899	1901	1905	rBV3	639	1103	0.12%	0.015%
92	12.792	1919	1920	1925	rBV6	676	886	0.09%	0.012%
93	13.018	1955	1957	1958	rVB2	715	320	0.03%	0.004%
94	13.109	1968	1972	1980	rBV2	9481	15206	1.63%	0.203%
95	13.591	2047	2051	2056	rBV	10477	14103	1.51%	0.188%
96	13.780	2077	2082	2085	rBV	7012	10459	1.12%	0.140%
97	13.963	2108	2112	2115	rBV2	8899	10827	1.16%	0.145%
98	14.731	2236	2238	2239	rBV2	1152	637	0.07%	0.009%
99	15.713	2398	2399	2402	rBV3	936	698	0.07%	0.009%
100	16.688	2557	2559	2561	rBV	999	938	0.10%	0.013%




Sum of corrected areas: 7482497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043520.D
Acq On : 25 Oct 2024 14:06
Operator : JC/MD
Sample : P4415-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

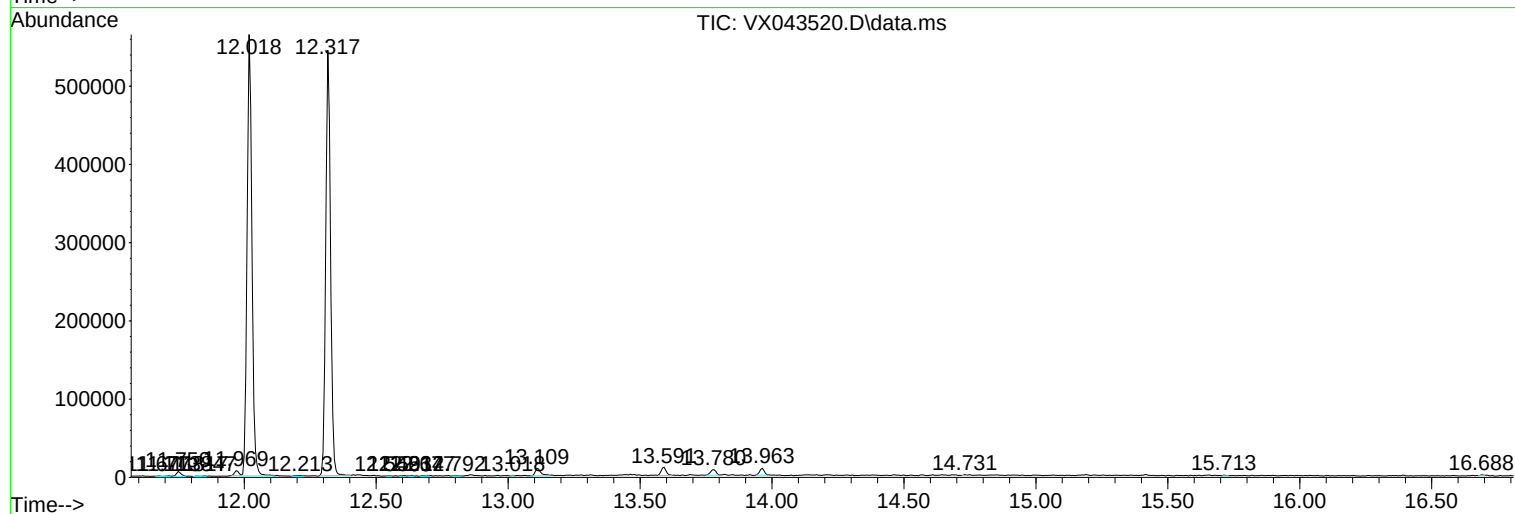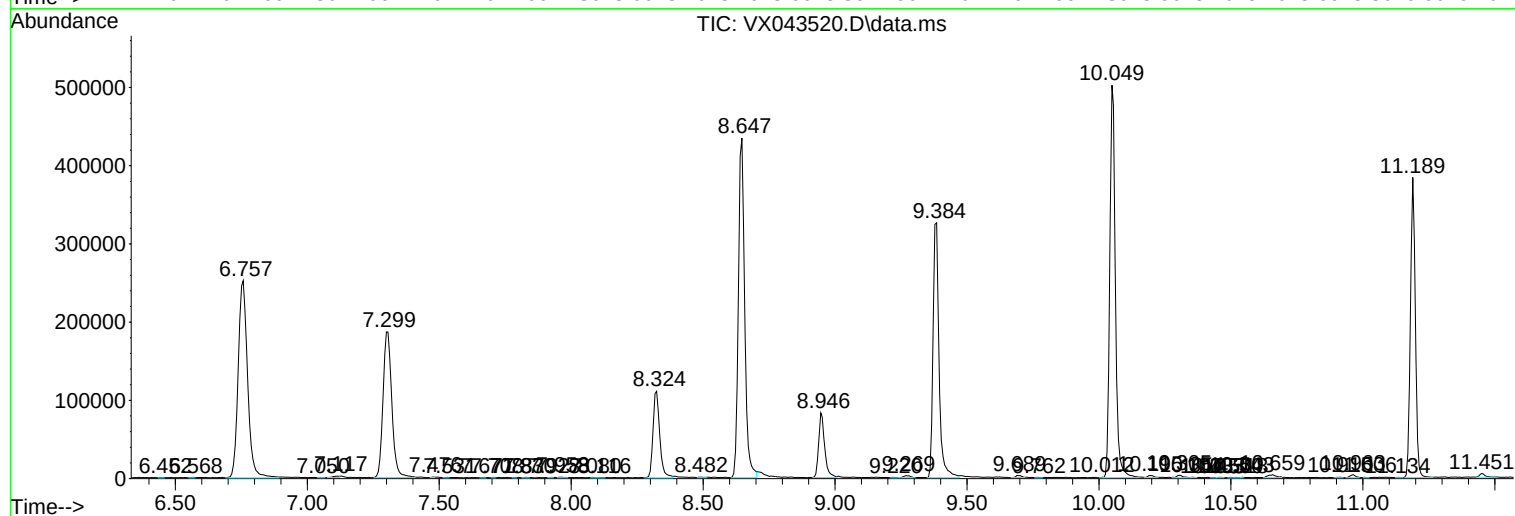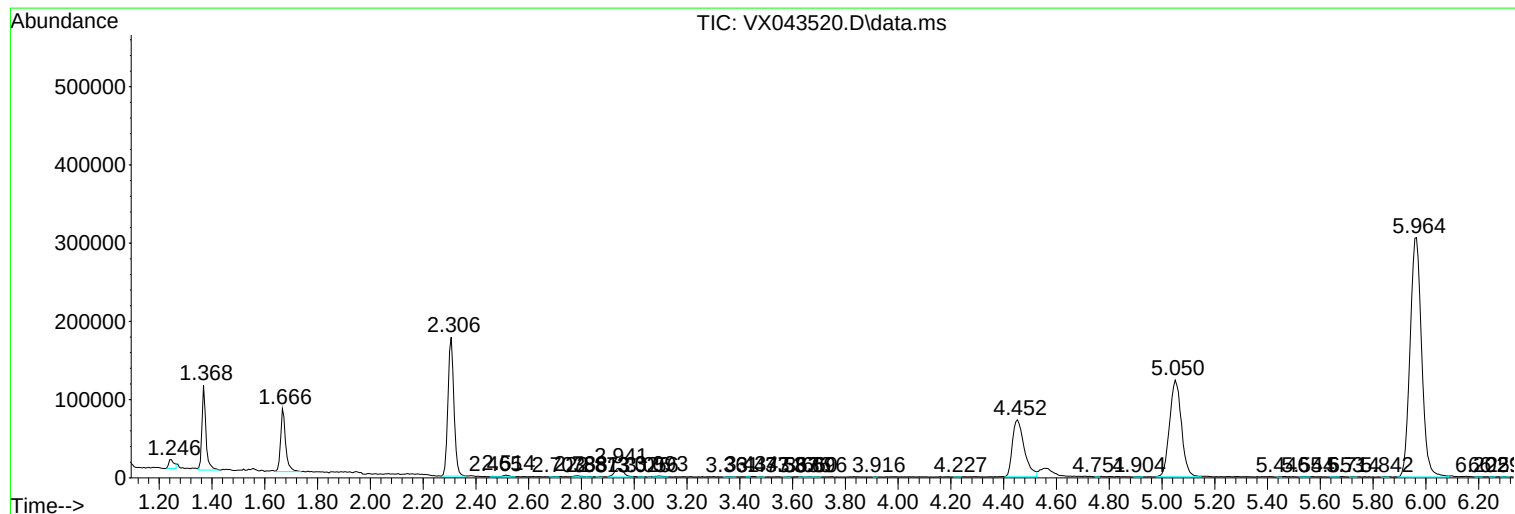

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043520.D
Acq On : 25 Oct 2024 14:06
Operator : JC/MD
Sample : P4415-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043520.D
Acq On : 25 Oct 2024 14:06
Operator : JC/MD
Sample : P4415-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc