

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043521.D
 Acq On : 25 Oct 2024 14:29
 Operator : JC/MD
 Sample : P4436-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rVB	139537	144763	12.42%	1.612%
2	1.666	92	95	104	rVB	100611	135667	11.64%	1.511%
3	2.306	194	200	207	rBV	239737	372027	31.93%	4.143%
4	2.380	208	212	224	rVB	24061	39436	3.38%	0.439%
5	2.532	231	237	245	rVB2	6477	12597	1.08%	0.140%
6	2.709	262	266	269	rBV3	1070	1683	0.14%	0.019%
7	2.782	274	278	279	rBV3	970	1282	0.11%	0.014%
8	2.934	300	303	305	rBV3	351	377	0.03%	0.004%
9	2.959	305	307	308	rBV2	509	363	0.03%	0.004%
10	3.093	325	329	334	rVB7	818	1560	0.13%	0.017%
11	3.166	339	341	343	rVV2	409	362	0.03%	0.004%
12	3.440	382	386	391	rVV3	899	1335	0.11%	0.015%
13	3.532	400	401	406	rVB2	594	739	0.06%	0.008%
14	3.678	424	425	427	rVB	810	434	0.04%	0.005%
15	3.709	427	430	432	rBV2	472	714	0.06%	0.008%
16	3.751	435	437	439	rBV2	371	391	0.03%	0.004%
17	3.800	443	445	448	rVB3	493	427	0.04%	0.005%
18	3.940	466	468	472	rBV3	478	567	0.05%	0.006%
19	4.257	518	520	524	rVB3	479	601	0.05%	0.007%
20	4.300	524	527	528	rBV2	393	403	0.03%	0.004%
21	4.349	533	535	538	rBV2	429	534	0.05%	0.006%
22	4.452	543	552	567	rBV2	79159	248014	21.29%	2.762%
23	5.056	638	651	668	rBV	160461	481003	41.28%	5.357%
24	5.403	706	708	710	rVB2	667	583	0.05%	0.006%
25	5.440	710	714	715	rBV	611	554	0.05%	0.006%
26	5.623	741	744	746	rBV2	401	550	0.05%	0.006%
27	5.678	751	753	757	rVB2	465	453	0.04%	0.005%
28	5.806	773	774	778	rVB2	431	474	0.04%	0.005%
29	5.964	788	800	816	rBV3	385915	1165109	100.00%	12.976%
30	6.190	835	837	838	rVB2	685	424	0.04%	0.005%
31	6.220	838	842	844	rBV3	719	888	0.08%	0.010%
32	6.318	855	858	859	rBV3	346	375	0.03%	0.004%
33	6.403	870	872	873	rBV	419	364	0.03%	0.004%
34	6.513	888	890	893	rBV3	485	618	0.05%	0.007%
35	6.665	913	915	918	rBV3	517	522	0.04%	0.006%
36	6.757	921	930	945	rBV	286802	697039	59.83%	7.763%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043521.D
 Acq On : 25 Oct 2024 14:29
 Operator : JC/MD
 Sample : P4436-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
 Title : VOC Analysis

37	7.117	984	989	990	rBV5	1777	2611	0.22%	0.029%
38	7.306	1012	1020	1042	rVB	240385	528337	45.35%	5.884%
39	7.659	1076	1078	1083	rVB2	727	761	0.07%	0.008%
40	7.702	1083	1085	1087	rBV2	401	493	0.04%	0.005%
41	7.873	1112	1113	1118	rVB	507	451	0.04%	0.005%
42	8.147	1157	1158	1160	rBV2	517	387	0.03%	0.004%
43	8.324	1181	1187	1203	rBV	153714	259387	22.26%	2.889%
44	8.513	1215	1218	1220	rBV2	894	812	0.07%	0.009%
45	8.647	1233	1240	1261	rBV	560990	930683	79.88%	10.366%
46	8.952	1284	1290	1300	rBV	102535	166014	14.25%	1.849%
47	9.086	1311	1312	1314	rBV2	573	410	0.04%	0.005%
48	9.275	1337	1343	1347	rBV5	3091	4749	0.41%	0.053%
49	9.384	1355	1361	1381	rBV	360982	572736	49.16%	6.379%
50	10.049	1465	1470	1487	rBV	566604	843746	72.42%	9.397%
51	10.195	1491	1494	1497	rVB4	2248	2757	0.24%	0.031%
52	10.299	1508	1511	1516	rVB2	3076	4288	0.37%	0.048%
53	10.433	1532	1533	1536	rBV2	437	436	0.04%	0.005%
54	10.659	1564	1570	1576	rBV5	2843	7374	0.63%	0.082%
55	10.726	1579	1581	1584	rBV2	468	511	0.04%	0.006%
56	10.781	1584	1590	1594	rBV3	713	1580	0.14%	0.018%
57	10.872	1602	1605	1610	rVB3	664	875	0.08%	0.010%
58	10.963	1616	1620	1625	rVB	3139	4050	0.35%	0.045%
59	11.030	1627	1631	1634	rBV4	1201	1559	0.13%	0.017%
60	11.189	1652	1657	1668	rVV	446243	566173	48.59%	6.306%
61	11.317	1676	1678	1682	rVB3	886	1000	0.09%	0.011%
62	11.451	1697	1700	1707	rVB2	4598	5388	0.46%	0.060%
63	11.543	1714	1715	1717	rBV	407	396	0.03%	0.004%
64	11.597	1720	1724	1725	rBV2	771	663	0.06%	0.007%
65	11.665	1733	1735	1739	rVB3	701	753	0.06%	0.008%
66	11.707	1740	1742	1745	rBV3	467	452	0.04%	0.005%
67	11.750	1745	1749	1754	rBV	4581	6594	0.57%	0.073%
68	11.793	1754	1756	1757	rBV	1345	939	0.08%	0.010%
69	11.884	1770	1771	1774	rBV2	556	524	0.04%	0.006%
70	11.927	1776	1778	1779	rBV2	593	511	0.04%	0.006%
71	11.969	1782	1785	1788	rBV2	6509	7930	0.68%	0.088%
72	12.018	1788	1793	1802	rVV	610825	778334	66.80%	8.669%
73	12.219	1821	1826	1835	rBV	13746	21783	1.87%	0.243%
74	12.317	1837	1842	1855	rVB	632393	801624	68.80%	8.928%
75	12.579	1881	1885	1893	rVB2	12603	17477	1.50%	0.195%
76	12.762	1913	1915	1920	rBV4	1418	2305	0.20%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043521.D
 Acq On : 25 Oct 2024 14:29
 Operator : JC/MD
 Sample : P4436-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	12.817	1920	1924	1928	rBV	29738	37238	3.20%	0.415%
78	12.957	1945	1947	1950	rBV3	721	671	0.06%	0.007%
79	13.018	1955	1957	1960	rBV4	361	413	0.04%	0.005%
80	13.109	1968	1972	1977	rBV	8705	11852	1.02%	0.132%
81	13.378	2015	2016	2019	rBV2	394	475	0.04%	0.005%
82	13.457	2025	2029	2035	rBV4	1879	3673	0.32%	0.041%
83	13.500	2035	2036	2041	rVB5	1252	1916	0.16%	0.021%
84	13.554	2042	2045	2046	rBV3	495	439	0.04%	0.005%
85	13.591	2046	2051	2055	rBV2	13707	19510	1.67%	0.217%
86	13.774	2077	2081	2086	rVB	7184	9356	0.80%	0.104%
87	13.914	2102	2104	2105	rBV	517	458	0.04%	0.005%
88	13.957	2108	2111	2120	rVB	9114	12999	1.12%	0.145%
89	14.079	2126	2131	2134	rBV3	779	1087	0.09%	0.012%
90	14.121	2134	2138	2141	rVV	668	699	0.06%	0.008%
91	14.371	2176	2179	2180	rBV2	670	714	0.06%	0.008%
92	14.451	2188	2192	2197	rVB8	1359	2237	0.19%	0.025%
93	14.731	2233	2238	2240	rVV6	1185	1921	0.16%	0.021%
94	14.810	2249	2251	2254	rBV4	479	628	0.05%	0.007%
95	14.914	2266	2268	2270	rBV2	763	707	0.06%	0.008%
96	14.987	2277	2280	2285	rVB4	3141	3754	0.32%	0.042%
97	15.341	2336	2338	2340	rBV2	675	530	0.05%	0.006%
98	15.493	2359	2363	2371	rVB6	2786	5255	0.45%	0.059%
99	15.859	2421	2423	2426	rBV3	543	474	0.04%	0.005%
100	16.456	2519	2521	2523	rBV	733	532	0.05%	0.006%

Sum of corrected areas: 8978623




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043521.D
Acq On : 25 Oct 2024 14:29
Operator : JC/MD
Sample : P4436-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

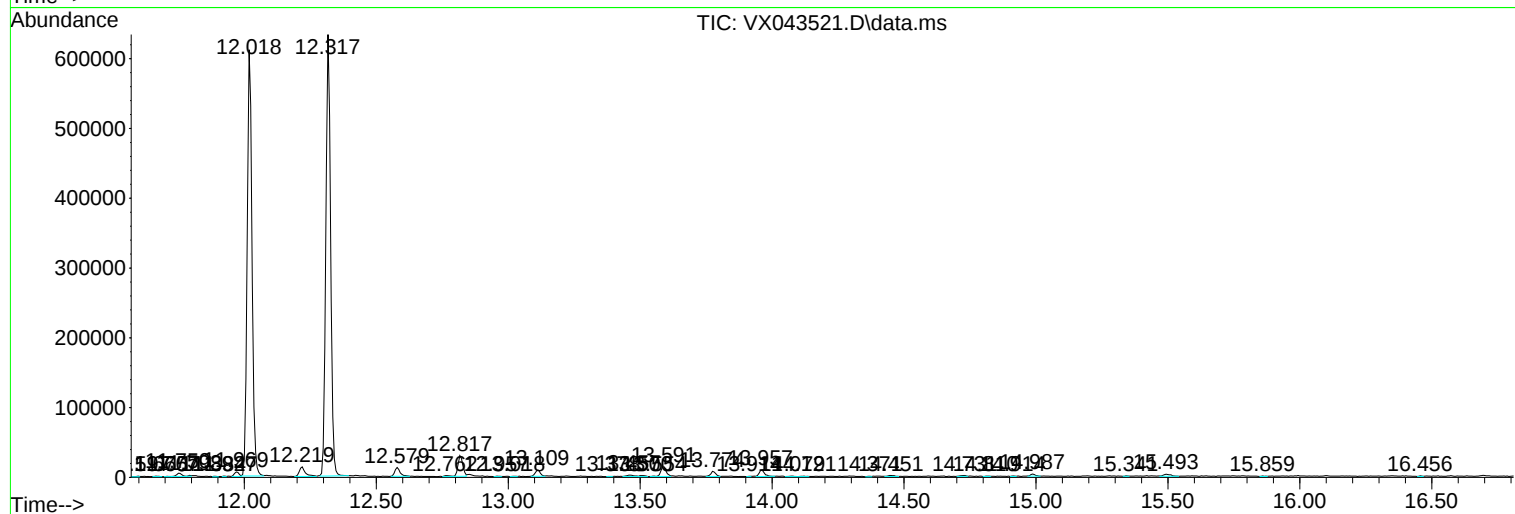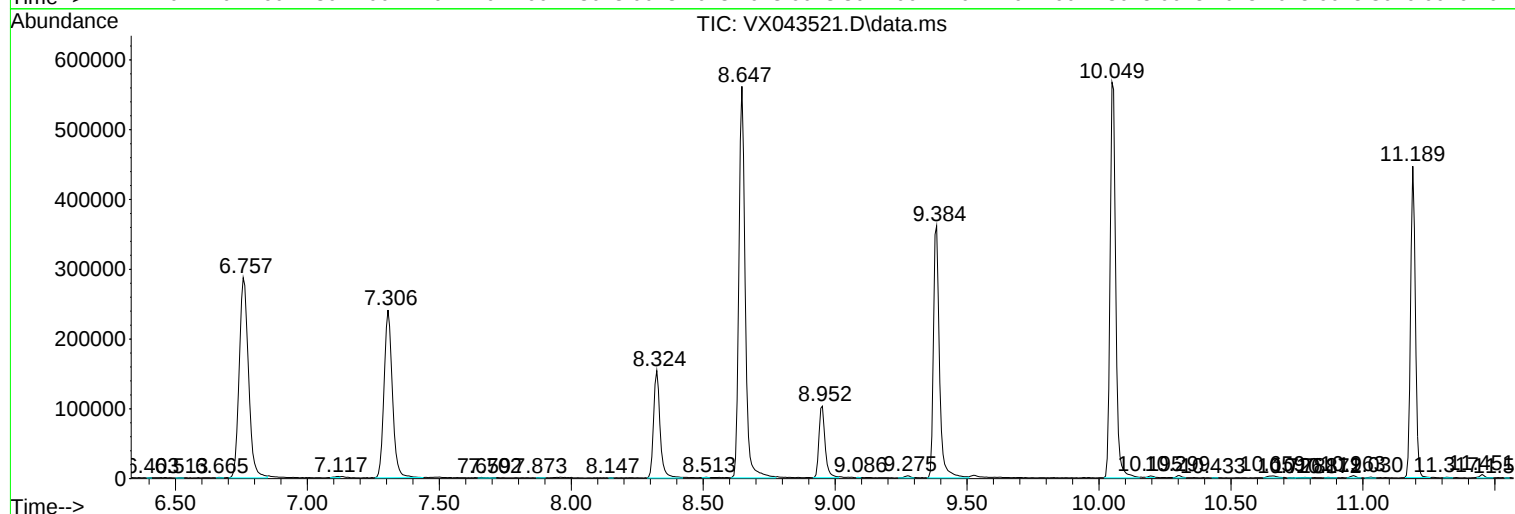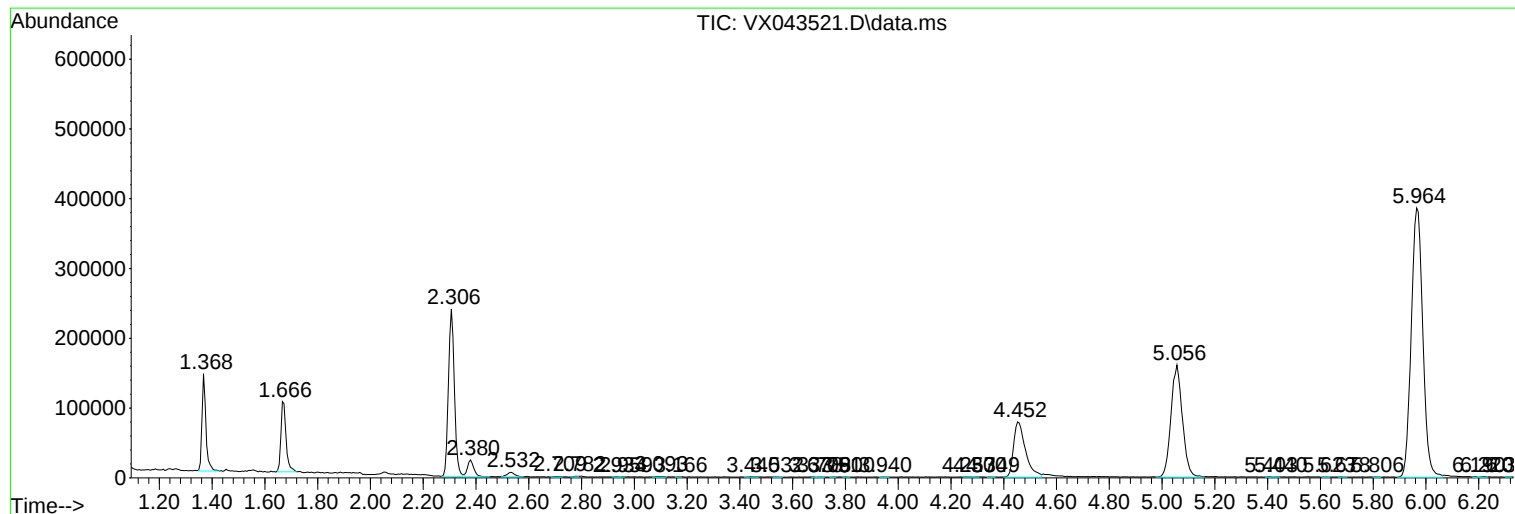

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043521.D
Acq On : 25 Oct 2024 14:29
Operator : JC/MD
Sample : P4436-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043521.D
Acq On : 25 Oct 2024 14:29
Operator : JC/MD
Sample : P4436-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc