

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043522.D
 Acq On : 25 Oct 2024 14:52
 Operator : JC/MD
 Sample : P4436-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M

Title : VOC Analysis

Signal : TIC: VX043522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.227	183	187	193	rBV	51156	79031	9.23%	1.477%
2	3.343	367	370	378	rVB4	4127	8467	0.99%	0.158%
3	3.568	405	407	410	rBV2	392	356	0.04%	0.007%
4	3.599	410	412	414	rVV2	304	265	0.03%	0.005%
5	3.855	452	454	457	rVB2	451	430	0.05%	0.008%
6	3.879	457	458	460	rBV2	389	328	0.04%	0.006%
7	3.910	461	463	464	rVV	454	337	0.04%	0.006%
8	3.952	468	470	471	rBV	404	280	0.03%	0.005%
9	4.105	494	495	497	rVB2	445	282	0.03%	0.005%
10	4.129	497	499	502	rBV2	317	306	0.04%	0.006%
11	4.251	518	519	521	rVB	474	346	0.04%	0.006%
12	4.276	521	523	524	rBV2	362	265	0.03%	0.005%
13	4.355	535	536	539	rVB3	581	463	0.05%	0.009%
14	4.385	539	541	544	rBV2	557	722	0.08%	0.013%
15	4.599	565	576	578	rBV2	9415	30429	3.55%	0.569%
16	5.452	715	716	719	rBV2	626	406	0.05%	0.008%
17	5.525	723	728	729	rBV4	817	1087	0.13%	0.020%
18	5.946	785	797	839	rBV2	205764	856510	100.00%	16.003%
19	6.336	859	861	864	rBV2	292	278	0.03%	0.005%
20	6.397	869	871	872	rBV	274	250	0.03%	0.005%
21	6.422	872	875	878	rBV4	451	630	0.07%	0.012%
22	6.452	878	880	882	rBV3	373	329	0.04%	0.006%
23	6.470	882	883	887	rVB3	784	557	0.07%	0.010%
24	6.507	887	889	891	rBV2	403	538	0.06%	0.010%
25	6.550	894	896	902	rVB4	391	726	0.08%	0.014%
26	6.604	904	905	907	rBV	453	464	0.05%	0.009%
27	6.751	918	929	955	rBV	158594	529093	61.77%	9.885%
28	7.110	982	988	995	rVB8	1712	4725	0.55%	0.088%
29	7.305	1011	1020	1041	rBV2	122244	379762	44.34%	7.095%
30	7.537	1056	1058	1063	rVB3	423	470	0.05%	0.009%
31	7.647	1074	1076	1078	rBV	270	302	0.04%	0.006%
32	7.690	1081	1083	1085	rBV	406	423	0.05%	0.008%
33	7.799	1099	1101	1103	rBV3	590	565	0.07%	0.011%
34	7.824	1103	1105	1107	rVV2	291	293	0.03%	0.005%
35	7.872	1112	1113	1115	rVV2	386	257	0.03%	0.005%
36	8.159	1159	1160	1162	rBV2	718	604	0.07%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043522.D
 Acq On : 25 Oct 2024 14:52
 Operator : JC/MD
 Sample : P4436-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

37	8.214	1168	1169	1172	rVB3	450	331	0.04%	0.006%
38	8.238	1172	1173	1175	rVB2	430	242	0.03%	0.005%
39	8.330	1181	1188	1203	rBV	64732	160705	18.76%	3.003%
40	8.500	1214	1216	1219	rBV3	389	426	0.05%	0.008%
41	8.543	1219	1223	1224	rVB	672	709	0.08%	0.013%
42	8.641	1233	1239	1259	rBV	351008	715644	83.55%	13.371%
43	8.958	1286	1291	1307	rVB2	45452	106824	12.47%	1.996%
44	9.269	1338	1342	1347	rBV5	2282	3716	0.43%	0.069%
45	9.323	1350	1351	1354	rBV2	358	408	0.05%	0.008%
46	9.409	1359	1365	1371	rBV2	59077	169702	19.81%	3.171%
47	9.921	1447	1449	1452	rVB2	486	410	0.05%	0.008%
48	9.951	1452	1454	1456	rBV2	371	282	0.03%	0.005%
49	9.988	1456	1460	1461	rVV	386	430	0.05%	0.008%
50	10.055	1465	1471	1490	rVV	365803	645286	75.34%	12.056%
51	10.195	1492	1494	1499	rVV4	2316	3087	0.36%	0.058%
52	10.244	1500	1502	1508	rVB4	1285	1766	0.21%	0.033%
53	10.305	1508	1512	1516	rBV3	2199	3403	0.40%	0.064%
54	10.396	1524	1527	1529	rBV3	515	707	0.08%	0.013%
55	10.451	1533	1536	1537	rBV2	350	405	0.05%	0.008%
56	10.549	1548	1552	1555	rBV3	422	639	0.07%	0.012%
57	10.579	1555	1557	1559	rBV2	514	446	0.05%	0.008%
58	10.665	1565	1571	1578	rBV6	2601	6812	0.80%	0.127%
59	10.780	1589	1590	1593	rBV2	364	386	0.05%	0.007%
60	10.957	1615	1619	1627	rVB5	2090	3801	0.44%	0.071%
61	11.061	1635	1636	1639	rVB	425	317	0.04%	0.006%
62	11.110	1639	1644	1648	rBV3	1142	1829	0.21%	0.034%
63	11.201	1653	1659	1669	rBV	168388	328994	38.41%	6.147%
64	11.305	1674	1676	1681	rVB3	876	1138	0.13%	0.021%
65	11.378	1686	1688	1689	rBV2	454	393	0.05%	0.007%
66	11.415	1692	1694	1697	rVB2	552	542	0.06%	0.010%
67	11.451	1697	1700	1711	rBV4	3228	5558	0.65%	0.104%
68	11.689	1736	1739	1743	rVB5	767	833	0.10%	0.016%
69	11.750	1743	1749	1755	rBV3	6886	11972	1.40%	0.224%
70	11.890	1770	1772	1773	rBV2	354	240	0.03%	0.004%
71	11.933	1773	1779	1782	rBV5	3820	5489	0.64%	0.103%
72	11.975	1782	1786	1789	rBV	4576	5986	0.70%	0.112%
73	12.024	1789	1794	1803	rVV	426600	609525	71.16%	11.388%
74	12.323	1837	1843	1854	rBV	421203	601078	70.18%	11.230%
75	12.524	1874	1876	1879	rBV2	418	348	0.04%	0.007%
76	12.646	1895	1896	1899	rBV	518	561	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043522.D
 Acq On : 25 Oct 2024 14:52
 Operator : JC/MD
 Sample : P4436-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	12.762	1910	1915	1918	rBV3	1207	2108	0.25%	0.039%
78	12.835	1922	1927	1928	rBV2	815	1075	0.13%	0.020%
79	12.859	1930	1931	1937	rVV5	783	1066	0.12%	0.020%
80	13.115	1968	1973	1982	rBV3	7828	11558	1.35%	0.216%
81	13.335	2007	2009	2012	rBV2	273	283	0.03%	0.005%
82	13.378	2012	2016	2017	rBV3	285	327	0.04%	0.006%
83	13.445	2025	2027	2029	rBV2	246	256	0.03%	0.005%
84	13.475	2031	2032	2035	rBV2	460	452	0.05%	0.008%
85	13.512	2035	2038	2039	rBV2	320	262	0.03%	0.005%
86	13.591	2047	2051	2056	rVB2	8382	9954	1.16%	0.186%
87	13.688	2065	2067	2071	rBV3	686	1012	0.12%	0.019%
88	13.780	2076	2082	2087	rBV5	3191	5262	0.61%	0.098%
89	13.963	2108	2112	2118	rBV4	4846	7217	0.84%	0.135%
90	14.066	2128	2129	2132	rBV2	334	399	0.05%	0.007%
91	14.127	2137	2139	2143	rVB4	520	684	0.08%	0.013%
92	14.237	2155	2157	2158	rBV	456	444	0.05%	0.008%
93	14.457	2190	2193	2196	rVB3	729	939	0.11%	0.018%
94	14.487	2196	2198	2200	rBV2	564	590	0.07%	0.011%
95	14.512	2200	2202	2207	rVB2	566	669	0.08%	0.012%
96	14.627	2218	2221	2222	rBV3	433	454	0.05%	0.008%
97	14.670	2226	2228	2230	rVV3	545	489	0.06%	0.009%
98	15.200	2313	2315	2317	rVB2	630	348	0.04%	0.007%
99	15.420	2344	2351	2356	rBV6	1807	4057	0.47%	0.076%
100	15.895	2428	2429	2431	rVB	930	438	0.05%	0.008%

Sum of corrected areas: 5352289




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043522.D
Acq On : 25 Oct 2024 14:52
Operator : JC/MD
Sample : P4436-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

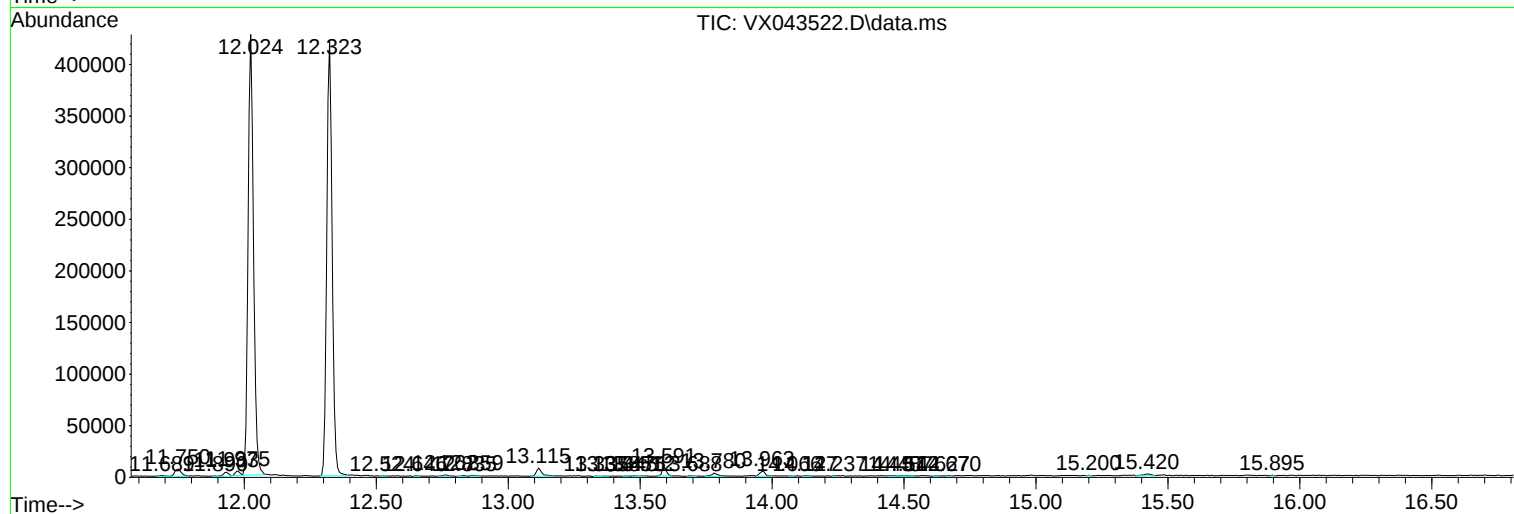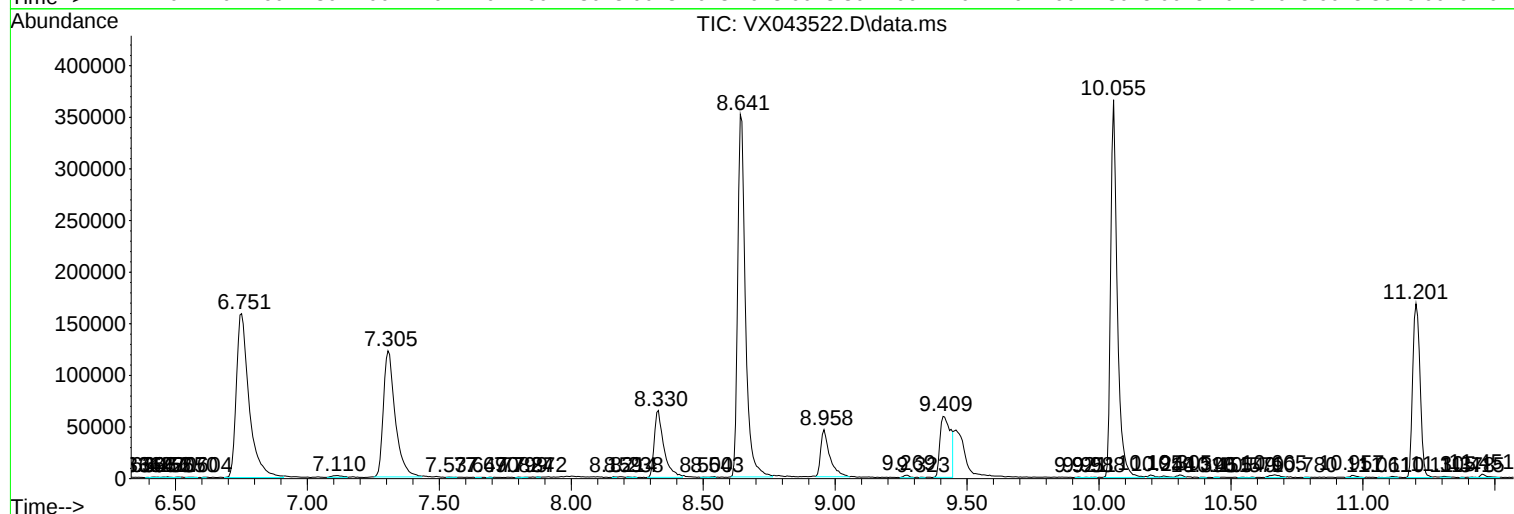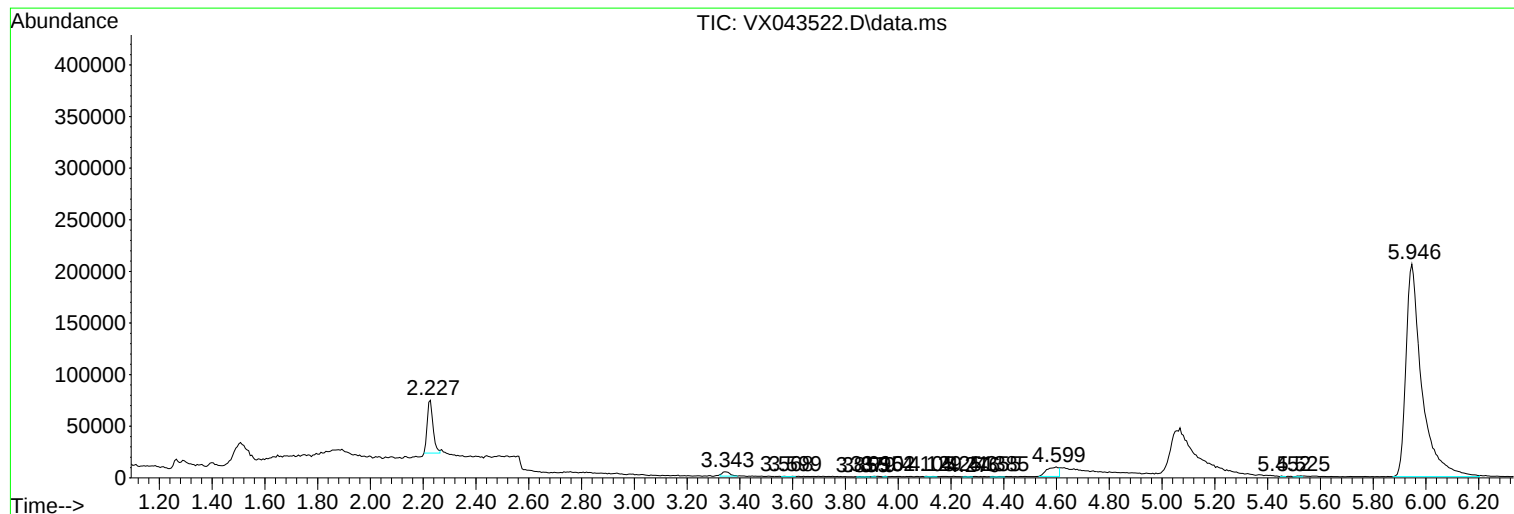

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043522.D
Acq On : 25 Oct 2024 14:52
Operator : JC/MD
Sample : P4436-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043522.D
Acq On : 25 Oct 2024 14:52
Operator : JC/MD
Sample : P4436-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc