

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043523.D
 Acq On : 25 Oct 2024 15:15
 Operator : JC/MD
 Sample : P4493-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4EC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M

Title : VOC Analysis

Signal : TIC: VX043523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	33	rBV	21555	36600	3.80%	0.502%
2	1.367	43	46	57	rVB	92069	123399	12.80%	1.693%
3	1.642	89	91	110	rVB	53172	130439	13.53%	1.790%
4	2.288	192	197	207	rVB	180668	289001	29.97%	3.965%
5	2.398	210	215	227	rVB	19325	35043	3.63%	0.481%
6	2.666	258	259	262	rVB2	625	398	0.04%	0.005%
7	2.709	262	266	272	rVV5	661	1465	0.15%	0.020%
8	2.776	274	277	283	rVB4	1099	2344	0.24%	0.032%
9	2.885	292	295	298	rBV2	617	867	0.09%	0.012%
10	2.940	298	304	314	rBV2	5688	13903	1.44%	0.191%
11	3.081	325	327	333	rVB5	749	1262	0.13%	0.017%
12	3.233	350	352	355	rVB2	377	400	0.04%	0.005%
13	3.434	375	385	392	rBV4	3890	9747	1.01%	0.134%
14	3.580	408	409	412	rVB	471	425	0.04%	0.006%
15	3.751	434	437	442	rVB3	306	493	0.05%	0.007%
16	4.245	514	518	521	rBV3	373	677	0.07%	0.009%
17	4.330	529	532	533	rBV2	380	404	0.04%	0.006%
18	4.404	541	544	547	rBV	475	743	0.08%	0.010%
19	4.471	547	555	571	rBV	58204	201691	20.92%	2.767%
20	4.842	612	616	617	rVB2	450	397	0.04%	0.005%
21	4.903	623	626	628	rBV3	334	465	0.05%	0.006%
22	5.050	638	650	672	rBV	125440	383550	39.78%	5.263%
23	5.379	701	704	705	rBV	409	462	0.05%	0.006%
24	5.525	724	728	730	rBV3	501	810	0.08%	0.011%
25	5.550	730	732	735	rVB	573	589	0.06%	0.008%
26	5.781	769	770	775	rVV3	403	431	0.04%	0.006%
27	5.964	788	800	827	rBV2	326242	964236	100.00%	13.230%
28	6.159	830	832	834	rVB2	760	587	0.06%	0.008%
29	6.275	848	851	852	rBV3	368	424	0.04%	0.006%
30	6.354	861	864	865	rVV2	625	578	0.06%	0.008%
31	6.367	865	866	870	rVV3	1062	1006	0.10%	0.014%
32	6.403	870	872	874	rVB2	533	450	0.05%	0.006%
33	6.452	877	880	881	rBV2	396	451	0.05%	0.006%
34	6.543	893	895	897	rBV2	383	460	0.05%	0.006%
35	6.757	921	930	952	rBV	234003	575868	59.72%	7.902%
36	7.135	984	992	993	rBV5	1863	3461	0.36%	0.047%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043523.D
 Acq On : 25 Oct 2024 15:15
 Operator : JC/MD
 Sample : P4493-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4EC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
 Title : VOC Analysis

37	7.305	1010	1020	1038	rBV	193717	432975	44.90%	5.941%
38	7.470	1045	1047	1052	rBV4	568	936	0.10%	0.013%
39	7.555	1059	1061	1064	rBV3	423	482	0.05%	0.007%
40	7.787	1095	1099	1101	rVB2	449	612	0.06%	0.008%
41	7.958	1124	1127	1128	rBV2	434	467	0.05%	0.006%
42	8.135	1154	1156	1159	rBV2	581	669	0.07%	0.009%
43	8.171	1159	1162	1166	rVB3	431	588	0.06%	0.008%
44	8.324	1181	1187	1203	rBV	110814	191724	19.88%	2.631%
45	8.647	1233	1240	1258	rBV	464615	757184	78.53%	10.389%
46	8.951	1284	1290	1299	rBV	77038	122986	12.75%	1.688%
47	9.116	1315	1317	1322	rVB4	864	913	0.09%	0.013%
48	9.275	1336	1343	1349	rBV3	4500	8138	0.84%	0.112%
49	9.390	1356	1362	1377	rBV	305265	485544	50.36%	6.662%
50	9.732	1416	1418	1421	rVB2	668	498	0.05%	0.007%
51	9.799	1426	1429	1431	rBV3	588	556	0.06%	0.008%
52	9.909	1443	1447	1450	rVB2	424	613	0.06%	0.008%
53	10.055	1465	1471	1492	rVV	454039	671436	69.63%	9.213%
54	10.189	1492	1493	1494	rBV	798	490	0.05%	0.007%
55	10.305	1509	1512	1517	rVV4	1419	2458	0.25%	0.034%
56	10.348	1517	1519	1521	rVB2	581	539	0.06%	0.007%
57	10.585	1556	1558	1561	rVB3	453	413	0.04%	0.006%
58	10.646	1565	1568	1569	rBV2	1022	1122	0.12%	0.015%
59	10.860	1601	1603	1604	rBV2	661	641	0.07%	0.009%
60	10.963	1615	1620	1625	rBV4	1286	2564	0.27%	0.035%
61	11.030	1625	1631	1635	rVV5	1377	2267	0.24%	0.031%
62	11.152	1648	1651	1652	rBV	474	397	0.04%	0.005%
63	11.189	1652	1657	1668	rVV	359014	488135	50.62%	6.698%
64	11.317	1674	1678	1681	rVB4	3232	4479	0.46%	0.061%
65	11.384	1687	1689	1690	rBV	575	486	0.05%	0.007%
66	11.402	1690	1692	1695	rVV2	818	783	0.08%	0.011%
67	11.451	1698	1700	1705	rVV4	1578	2145	0.22%	0.029%
68	11.561	1715	1718	1720	rBV2	479	486	0.05%	0.007%
69	11.689	1737	1739	1741	rBV2	583	467	0.05%	0.006%
70	11.756	1746	1750	1754	rBV3	1614	2592	0.27%	0.036%
71	11.792	1754	1756	1762	rBV4	1361	2158	0.22%	0.030%
72	11.896	1769	1773	1774	rBV4	534	505	0.05%	0.007%
73	11.933	1775	1779	1783	rVV4	1319	2281	0.24%	0.031%
74	11.969	1783	1785	1788	rVV2	2615	3075	0.32%	0.042%
75	12.024	1788	1794	1804	rVV	447995	582842	60.45%	7.997%
76	12.164	1816	1817	1822	rBV4	717	791	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043523.D
 Acq On : 25 Oct 2024 15:15
 Operator : JC/MD
 Sample : P4493-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4EC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	12.219	1822	1826	1835	rBV2	10843	18134	1.88%	0.249%
78	12.317	1837	1842	1855	rVV	514545	640696	66.45%	8.791%
79	12.579	1881	1885	1892	rBV2	9102	12490	1.30%	0.171%
80	12.640	1892	1895	1898	rVB3	1006	1244	0.13%	0.017%
81	12.768	1911	1916	1920	rBV4	1994	3071	0.32%	0.042%
82	12.817	1922	1924	1928	rVV3	4560	6349	0.66%	0.087%
83	12.853	1928	1930	1936	rVB3	2896	4204	0.44%	0.058%
84	12.902	1936	1938	1942	rBV4	698	1038	0.11%	0.014%
85	13.115	1969	1973	1976	rBV3	3129	3847	0.40%	0.053%
86	13.158	1978	1980	1986	rVB5	1055	1748	0.18%	0.024%
87	13.225	1989	1991	1995	rVB3	547	452	0.05%	0.006%
88	13.445	2025	2027	2028	rBV	705	562	0.06%	0.008%
89	13.475	2028	2032	2033	rBV2	730	899	0.09%	0.012%
90	13.591	2047	2051	2058	rVV4	5940	9056	0.94%	0.124%
91	13.780	2079	2082	2086	rVB	4109	4576	0.47%	0.063%
92	13.963	2108	2112	2118	rVB5	3320	5014	0.52%	0.069%
93	14.146	2136	2142	2146	rBV5	1161	1811	0.19%	0.025%
94	14.292	2163	2166	2170	rBV5	736	1168	0.12%	0.016%
95	14.450	2189	2192	2198	rVB3	1789	2568	0.27%	0.035%
96	14.725	2235	2237	2242	rVB3	1228	1280	0.13%	0.018%
97	14.987	2275	2280	2287	rBV7	1620	3568	0.37%	0.049%
98	15.414	2348	2350	2352	rBV2	1060	1250	0.13%	0.017%
99	15.731	2401	2402	2404	rBV	700	636	0.07%	0.009%
100	15.883	2425	2427	2428	rBV2	720	404	0.04%	0.006%




Sum of corrected areas: 7288028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043523.D
Acq On : 25 Oct 2024 15:15
Operator : JC/MD
Sample : P4493-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4EC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

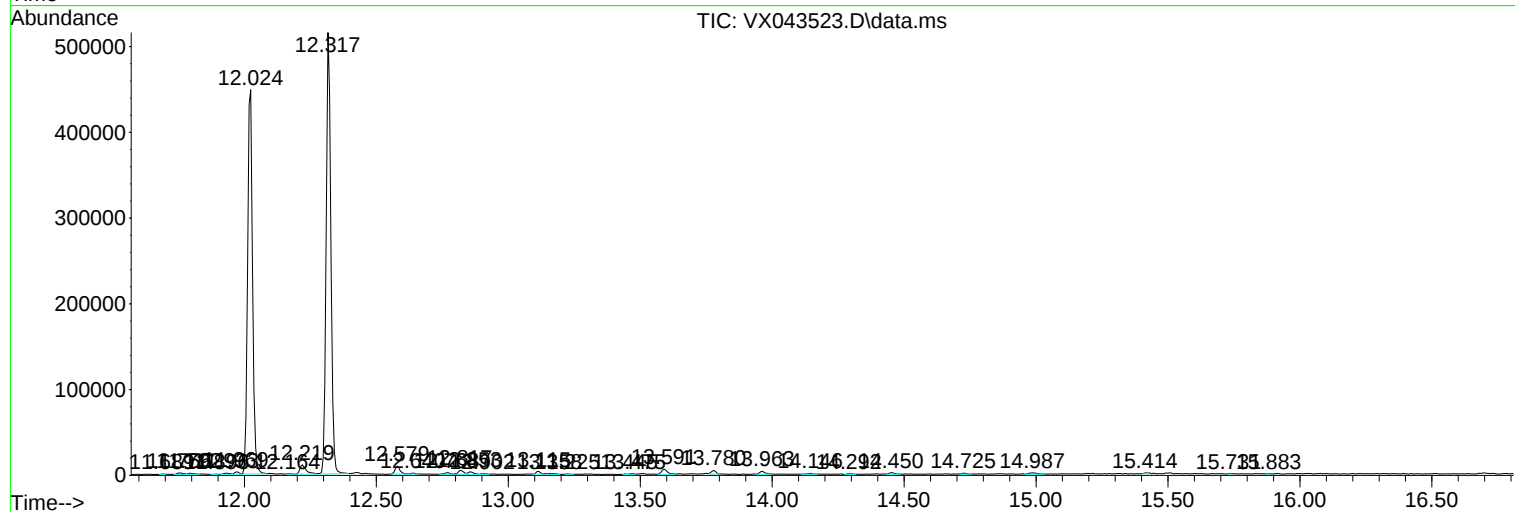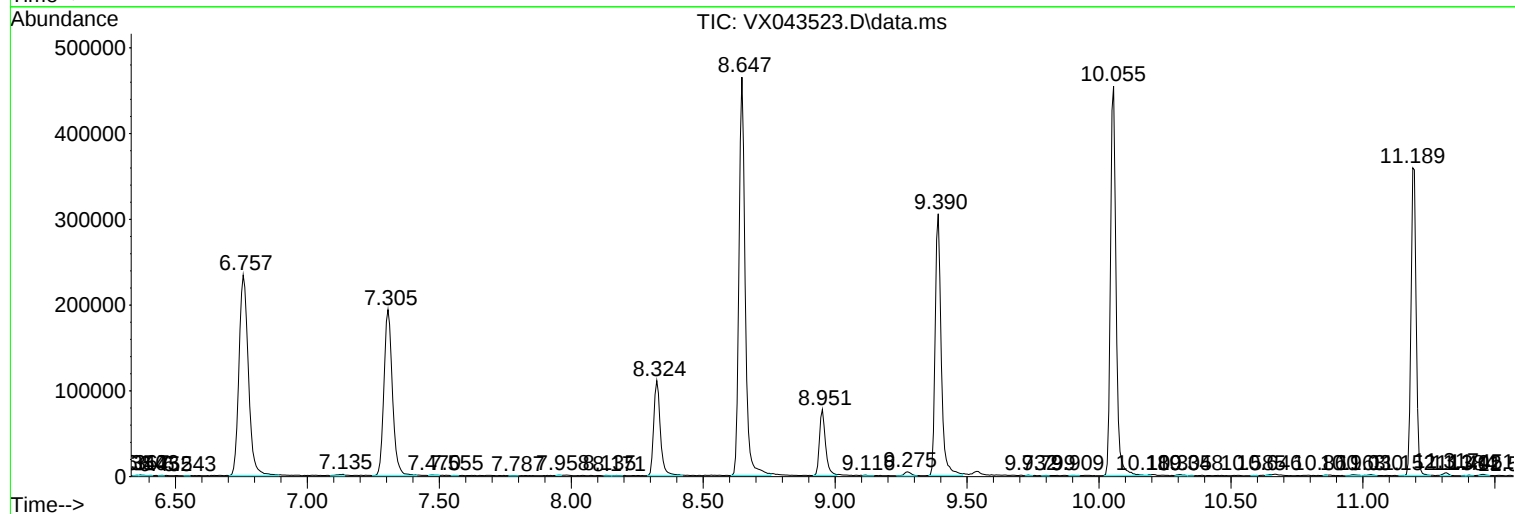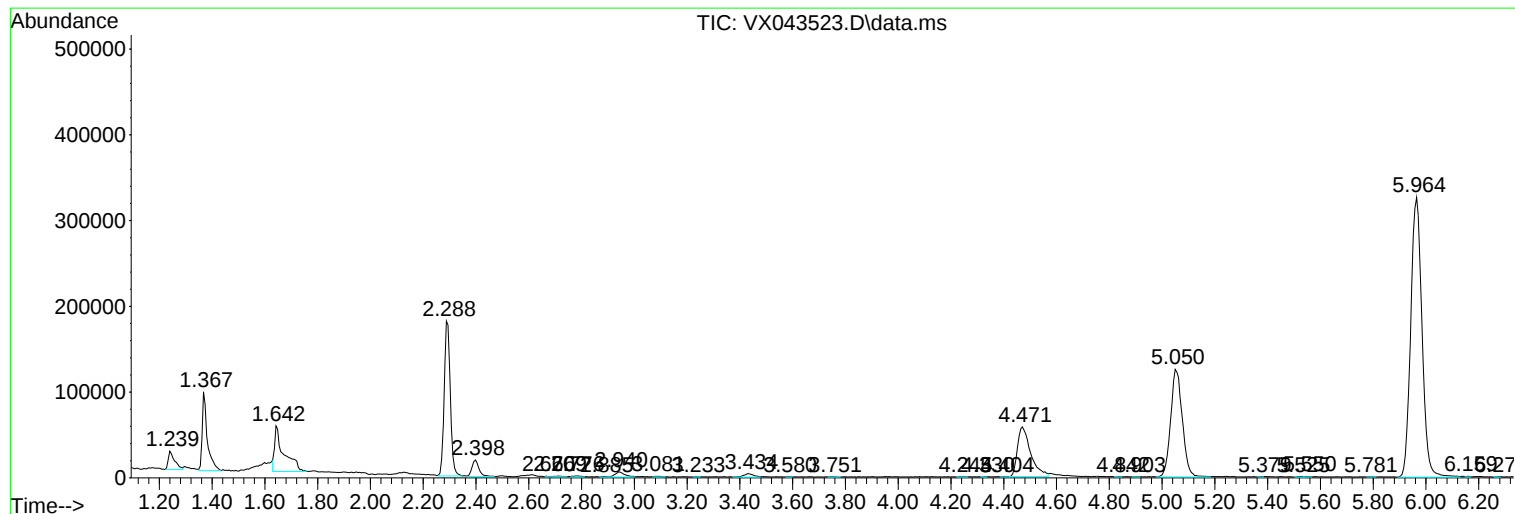

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043523.D
Acq On : 25 Oct 2024 15:15
Operator : JC/MD
Sample : P4493-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4EC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043523.D
Acq On : 25 Oct 2024 15:15
Operator : JC/MD
Sample : P4493-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4EC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc