

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043524.D
 Acq On : 25 Oct 2024 15:38
 Operator : JC/MD
 Sample : P4492-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV	26943	41231	3.85%	0.517%
2	1.368	43	46	57	rVB	105132	139184	13.00%	1.746%
3	1.642	88	91	109	rVB	60738	128201	11.97%	1.609%
4	2.294	192	198	210	rBV	204552	316541	29.56%	3.972%
5	2.392	210	214	223	rVB	15950	26544	2.48%	0.333%
6	2.502	228	232	236	rBV3	792	1274	0.12%	0.016%
7	2.709	263	266	272	rVB4	1220	2123	0.20%	0.027%
8	2.880	293	294	296	rBV	566	352	0.03%	0.004%
9	3.087	324	328	332	rVB4	614	851	0.08%	0.011%
10	3.154	338	339	342	rVB2	426	260	0.02%	0.003%
11	3.178	342	343	348	rBV2	366	546	0.05%	0.007%
12	3.221	348	350	353	rBV2	301	348	0.03%	0.004%
13	3.252	353	355	356	rBV	344	260	0.02%	0.003%
14	3.434	374	385	392	rBV5	2843	7297	0.68%	0.092%
15	3.556	403	405	406	rBV2	414	386	0.04%	0.005%
16	3.642	416	419	420	rVB2	362	285	0.03%	0.004%
17	3.715	430	431	433	rBV	430	399	0.04%	0.005%
18	3.812	446	447	449	rBV	500	365	0.03%	0.005%
19	4.203	510	511	514	rBV2	257	288	0.03%	0.004%
20	4.385	539	541	544	rBV2	544	635	0.06%	0.008%
21	4.465	546	554	573	rBV2	64174	218719	20.42%	2.744%
22	4.867	619	620	624	rVB2	567	444	0.04%	0.006%
23	4.904	624	626	629	rVB2	404	421	0.04%	0.005%
24	5.050	639	650	666	rVV	143173	431774	40.32%	5.418%
25	5.306	690	692	694	rBV3	504	549	0.05%	0.007%
26	5.337	696	697	700	rBV2	354	365	0.03%	0.005%
27	5.440	712	714	716	rBV2	319	325	0.03%	0.004%
28	5.794	768	772	773	rBV2	532	645	0.06%	0.008%
29	5.964	789	800	822	rVV2	363838	1070910	100.00%	13.437%
30	6.233	843	844	846	rVB	566	274	0.03%	0.003%
31	6.275	849	851	853	rVB3	499	429	0.04%	0.005%
32	6.367	864	866	869	rBV2	522	591	0.06%	0.007%
33	6.629	907	909	912	rBV2	519	690	0.06%	0.009%
34	6.757	921	930	951	rBV	251642	612469	57.19%	7.685%
35	6.958	961	963	968	rVB	789	952	0.09%	0.012%
36	7.037	974	976	979	rVB2	520	340	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043524.D
 Acq On : 25 Oct 2024 15:38
 Operator : JC/MD
 Sample : P4492-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

37	7.190	1000	1001	1003	rBV2	387	356	0.03%	0.004%
38	7.214	1003	1005	1006	rVV	637	376	0.04%	0.005%
39	7.306	1011	1020	1039	rVV	218725	487482	45.52%	6.117%
40	7.434	1039	1041	1042	rVB2	787	445	0.04%	0.006%
41	7.470	1045	1047	1048	rBV2	651	501	0.05%	0.006%
42	7.708	1081	1086	1090	rBV2	530	1161	0.11%	0.015%
43	7.964	1123	1128	1129	rBV3	1001	1659	0.15%	0.021%
44	8.080	1143	1147	1148	rBV2	380	476	0.04%	0.006%
45	8.324	1181	1187	1204	rBV	128325	220695	20.61%	2.769%
46	8.507	1215	1217	1219	rBV2	890	917	0.09%	0.012%
47	8.647	1233	1240	1262	rBV	503883	846307	79.03%	10.619%
48	8.952	1285	1290	1304	rBV	88426	139958	13.07%	1.756%
49	9.129	1317	1319	1323	rVB3	571	641	0.06%	0.008%
50	9.275	1338	1343	1346	rBV4	1379	2013	0.19%	0.025%
51	9.324	1349	1351	1352	rVB	528	302	0.03%	0.004%
52	9.342	1352	1354	1356	rBV	518	643	0.06%	0.008%
53	9.385	1356	1361	1380	rBV	340568	527081	49.22%	6.613%
54	9.897	1443	1445	1448	rBV	389	604	0.06%	0.008%
55	9.952	1450	1454	1456	rBV4	576	649	0.06%	0.008%
56	10.055	1465	1471	1486	rBV	479578	721036	67.33%	9.047%
57	10.195	1491	1494	1498	rBV4	1271	1964	0.18%	0.025%
58	10.311	1510	1513	1518	rVB3	1622	1783	0.17%	0.022%
59	10.409	1527	1529	1531	rBV2	534	413	0.04%	0.005%
60	10.531	1548	1549	1551	rBV	480	288	0.03%	0.004%
61	10.616	1560	1563	1565	rBV2	323	368	0.03%	0.005%
62	10.653	1565	1569	1570	rBV	1378	1775	0.17%	0.022%
63	10.823	1595	1597	1598	rBV	469	313	0.03%	0.004%
64	10.903	1608	1610	1613	rBV2	391	460	0.04%	0.006%
65	10.933	1613	1615	1616	rBV	510	281	0.03%	0.004%
66	10.957	1617	1619	1622	rBV3	1012	1013	0.09%	0.013%
67	11.031	1628	1631	1636	rBV2	958	1494	0.14%	0.019%
68	11.140	1647	1649	1650	rBV	414	361	0.03%	0.005%
69	11.189	1652	1657	1667	rVV	419612	548999	51.26%	6.889%
70	11.396	1690	1691	1692	rBV	674	320	0.03%	0.004%
71	11.457	1698	1701	1705	rVB3	1241	1393	0.13%	0.017%
72	11.683	1737	1738	1740	rBV2	534	387	0.04%	0.005%
73	11.756	1746	1750	1754	rBV4	1762	2297	0.21%	0.029%
74	11.799	1754	1757	1762	rVV5	1434	2295	0.21%	0.029%
75	11.969	1782	1785	1788	rBV2	2618	2427	0.23%	0.030%
76	12.018	1788	1793	1805	rVV	477328	624270	58.29%	7.833%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043524.D
 Acq On : 25 Oct 2024 15:38
 Operator : JC/MD
 Sample : P4492-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	12.219	1822	1826	1834	rBV2	10741	19264	1.80%	0.242%
78	12.317	1837	1842	1854	rVB	562691	724827	67.68%	9.095%
79	12.579	1881	1885	1891	rBV2	9994	13885	1.30%	0.174%
80	12.768	1914	1916	1920	rBV3	1112	883	0.08%	0.011%
81	12.817	1920	1924	1929	rBV2	19199	24666	2.30%	0.309%
82	13.049	1958	1962	1963	rBV2	399	439	0.04%	0.006%
83	13.116	1969	1973	1976	rVB5	2277	3080	0.29%	0.039%
84	13.274	1997	1999	2001	rBV3	620	501	0.05%	0.006%
85	13.463	2027	2030	2034	rBV5	935	1269	0.12%	0.016%
86	13.591	2047	2051	2054	rBV4	5437	7041	0.66%	0.088%
87	13.713	2070	2071	2072	rBV	732	481	0.04%	0.006%
88	13.780	2078	2082	2087	rVB2	2801	4286	0.40%	0.054%
89	13.963	2108	2112	2117	rBV4	2374	4044	0.38%	0.051%
90	14.146	2140	2142	2144	rVB2	577	435	0.04%	0.005%
91	14.170	2144	2146	2148	rBV2	497	501	0.05%	0.006%
92	14.213	2151	2153	2154	rVV	530	376	0.04%	0.005%
93	14.243	2156	2158	2160	rVB2	526	389	0.04%	0.005%
94	14.396	2181	2183	2187	rBV3	755	708	0.07%	0.009%
95	14.451	2189	2192	2196	rBV3	1583	2154	0.20%	0.027%
96	14.628	2219	2221	2224	rBV2	496	557	0.05%	0.007%
97	14.725	2234	2237	2241	rBV3	1609	1640	0.15%	0.021%
98	14.987	2277	2280	2285	rVB5	2633	3740	0.35%	0.047%
99	15.847	2420	2421	2422	rBV	642	336	0.03%	0.004%
100	16.286	2489	2493	2495	rBV3	629	808	0.08%	0.010%




Sum of corrected areas: 7969780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043524.D
Acq On : 25 Oct 2024 15:38
Operator : JC/MD
Sample : P4492-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

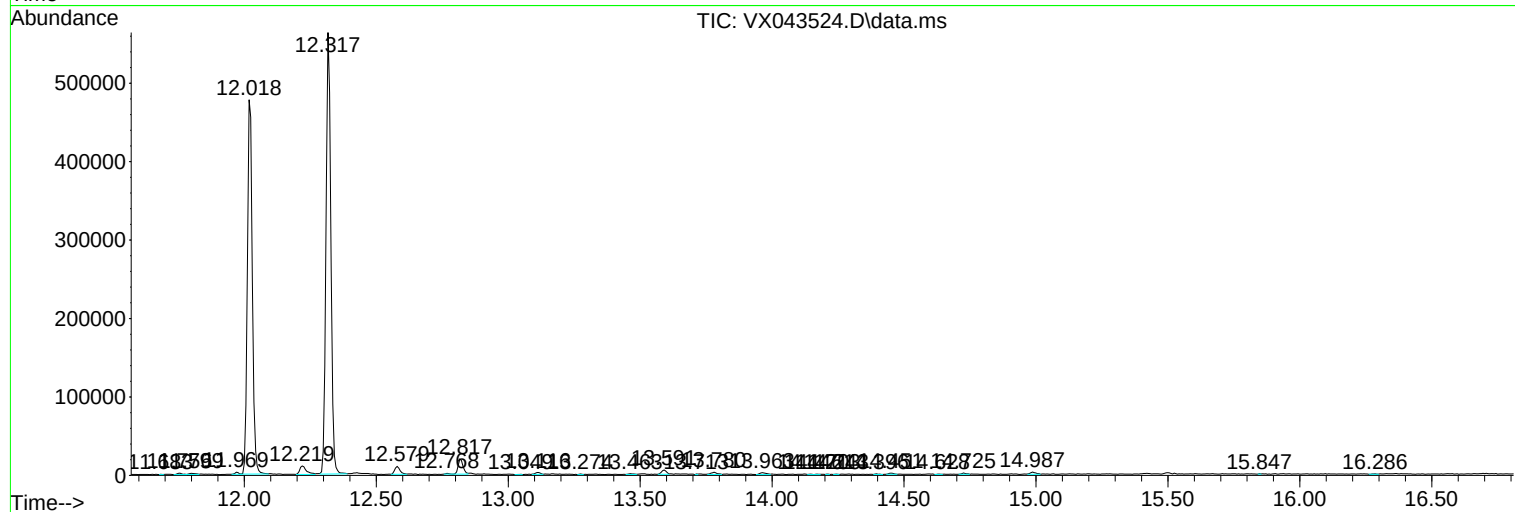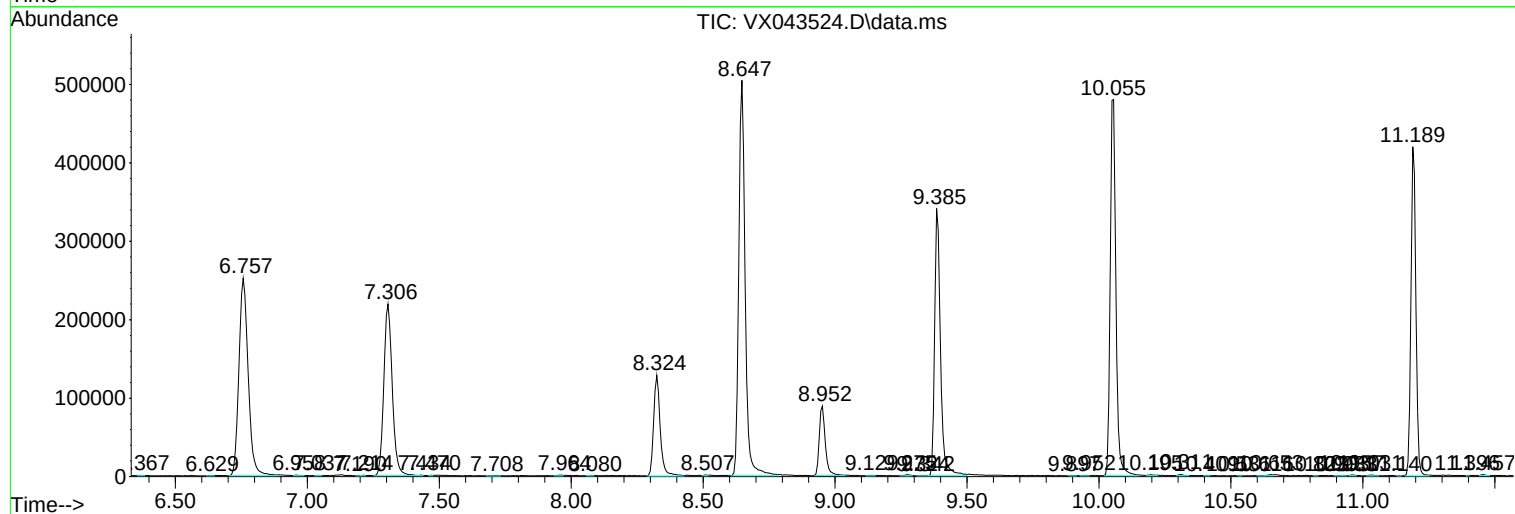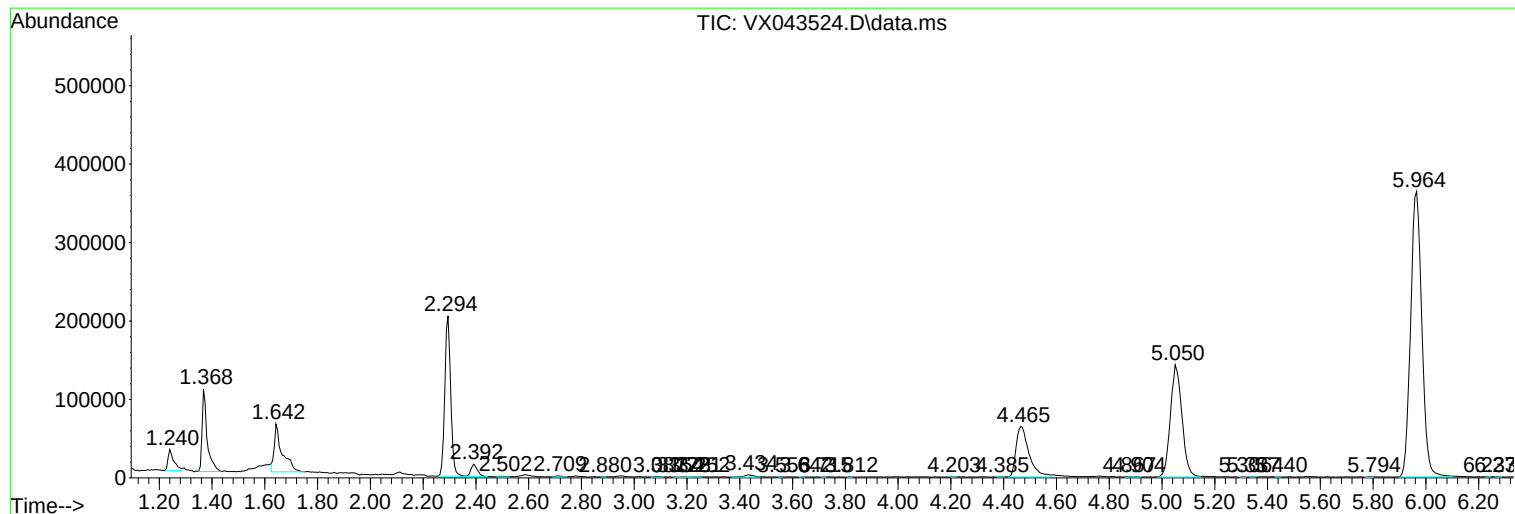

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043524.D
Acq On : 25 Oct 2024 15:38
Operator : JC/MD
Sample : P4492-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043524.D
Acq On : 25 Oct 2024 15:38
Operator : JC/MD
Sample : P4492-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc