

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043525.D
 Acq On : 25 Oct 2024 16:01
 Operator : JC/MD
 Sample : P4429-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV	28029	39908	4.04%	0.556%
2	1.368	43	46	59	rVB	89254	127842	12.94%	1.782%
3	1.642	89	91	97	rBV	38268	48342	4.89%	0.674%
4	2.294	192	198	210	rVB	187290	300586	30.43%	4.190%
5	2.398	210	215	222	rVB3	2300	4567	0.46%	0.064%
6	2.489	228	230	232	rBV3	917	830	0.08%	0.012%
7	2.581	241	245	246	rBV2	817	1083	0.11%	0.015%
8	2.782	273	278	281	rBV4	1706	2668	0.27%	0.037%
9	2.910	297	299	300	rVV2	549	340	0.03%	0.005%
10	2.941	300	304	311	rVV2	1841	3507	0.36%	0.049%
11	3.014	315	316	318	rBV	442	343	0.03%	0.005%
12	3.276	357	359	361	rVB2	530	403	0.04%	0.006%
13	3.434	377	385	392	rBV3	5272	11522	1.17%	0.161%
14	3.520	398	399	403	rBV2	570	576	0.06%	0.008%
15	3.556	403	405	408	rVV2	447	408	0.04%	0.006%
16	3.593	409	411	412	rVV	550	331	0.03%	0.005%
17	3.946	465	469	471	rBV3	425	591	0.06%	0.008%
18	3.965	471	472	474	rVV	400	374	0.04%	0.005%
19	4.087	490	492	494	rVB2	618	395	0.04%	0.006%
20	4.196	508	510	512	rBV2	588	350	0.04%	0.005%
21	4.471	547	555	576	rVV	62319	208001	21.06%	2.900%
22	4.635	581	582	584	rVB2	797	500	0.05%	0.007%
23	5.050	639	650	667	rVV	127904	391159	39.60%	5.453%
24	5.343	695	698	699	rBV2	406	343	0.03%	0.005%
25	5.532	727	729	731	rBV2	331	371	0.04%	0.005%
26	5.818	774	776	778	rVB2	338	326	0.03%	0.005%
27	5.964	788	800	818	rBV2	340003	987841	100.00%	13.771%
28	6.184	834	836	837	rBV2	423	331	0.03%	0.005%
29	6.300	853	855	859	rVB2	573	645	0.07%	0.009%
30	6.330	859	860	862	rBV2	485	330	0.03%	0.005%
31	6.367	863	866	872	rVB4	528	982	0.10%	0.014%
32	6.592	901	903	907	rBV3	271	386	0.04%	0.005%
33	6.647	909	912	915	rBV2	412	717	0.07%	0.010%
34	6.678	915	917	918	rBV	469	324	0.03%	0.005%
35	6.757	921	930	948	rBV	233859	571364	57.84%	7.965%
36	7.086	981	984	985	rBV2	312	376	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043525.D
 Acq On : 25 Oct 2024 16:01
 Operator : JC/MD
 Sample : P4429-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

37	7.306	1011	1020	1037	rBV	196512	441920	44.74%	6.161%
38	7.525	1054	1056	1059	rVB2	475	553	0.06%	0.008%
39	7.781	1096	1098	1100	rBV2	431	466	0.05%	0.006%
40	7.970	1126	1129	1131	rVV2	721	770	0.08%	0.011%
41	8.031	1137	1139	1142	rBV3	306	387	0.04%	0.005%
42	8.055	1142	1143	1146	rBV2	356	373	0.04%	0.005%
43	8.086	1146	1148	1150	rBV2	375	348	0.04%	0.005%
44	8.238	1169	1173	1176	rBV2	530	811	0.08%	0.011%
45	8.269	1176	1178	1181	rBV	337	331	0.03%	0.005%
46	8.324	1181	1187	1202	rBV	114864	195824	19.82%	2.730%
47	8.647	1234	1240	1257	rBV	468786	767067	77.65%	10.694%
48	8.952	1284	1290	1297	rBV	83867	127418	12.90%	1.776%
49	9.092	1311	1313	1315	rVB	561	478	0.05%	0.007%
50	9.269	1339	1342	1347	rVB2	2862	3771	0.38%	0.053%
51	9.391	1356	1362	1374	rBV	312512	494489	50.06%	6.894%
52	9.866	1437	1440	1441	rBV	346	348	0.04%	0.005%
53	10.055	1465	1471	1486	rBV	458734	665911	67.41%	9.283%
54	10.189	1492	1493	1495	rBV2	730	589	0.06%	0.008%
55	10.311	1507	1513	1518	rBV4	819	1804	0.18%	0.025%
56	10.390	1524	1526	1529	rBV	453	386	0.04%	0.005%
57	10.555	1552	1553	1556	rVB	598	368	0.04%	0.005%
58	10.646	1565	1568	1569	rBV2	571	567	0.06%	0.008%
59	10.774	1584	1589	1590	rVB	480	374	0.04%	0.005%
60	10.902	1607	1610	1612	rVV3	346	338	0.03%	0.005%
61	10.921	1612	1613	1615	rVV2	419	337	0.03%	0.005%
62	10.963	1618	1620	1624	rVV3	846	1066	0.11%	0.015%
63	11.024	1627	1630	1632	rVB2	469	591	0.06%	0.008%
64	11.049	1632	1634	1637	rBV2	476	472	0.05%	0.007%
65	11.195	1652	1658	1667	rBV	377886	511004	51.73%	7.124%
66	11.311	1674	1677	1681	rVB2	1559	1673	0.17%	0.023%
67	11.433	1695	1697	1698	rBV	538	387	0.04%	0.005%
68	11.457	1698	1701	1704	rVV3	1401	1780	0.18%	0.025%
69	11.506	1706	1709	1710	rBV	483	470	0.05%	0.007%
70	11.555	1714	1717	1718	rBV2	433	375	0.04%	0.005%
71	11.902	1771	1774	1775	rBV2	389	386	0.04%	0.005%
72	11.975	1782	1786	1788	rBV4	1935	2531	0.26%	0.035%
73	12.024	1788	1794	1804	rVV	423935	569288	57.63%	7.936%
74	12.097	1804	1806	1813	rVB6	1002	1602	0.16%	0.022%
75	12.225	1822	1827	1828	rBV3	950	1373	0.14%	0.019%
76	12.317	1837	1842	1857	rBV	500096	645547	65.35%	9.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043525.D
 Acq On : 25 Oct 2024 16:01
 Operator : JC/MD
 Sample : P4429-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	12.536	1876	1878	1880	rVB	792	479	0.05%	0.007%
78	12.579	1883	1885	1888	rVB2	393	415	0.04%	0.006%
79	12.823	1924	1925	1927	rBV	553	415	0.04%	0.006%
80	13.116	1969	1973	1977	rVB3	1611	2114	0.21%	0.029%
81	13.335	2008	2009	2011	rBV2	539	421	0.04%	0.006%
82	13.457	2026	2029	2032	rBV2	401	481	0.05%	0.007%
83	13.591	2048	2051	2057	rVV4	2261	3165	0.32%	0.044%
84	13.780	2076	2082	2087	rVB4	1295	2655	0.27%	0.037%
85	13.914	2101	2104	2106	rVV3	447	428	0.04%	0.006%
86	13.963	2108	2112	2116	rVV3	1594	2026	0.21%	0.028%
87	14.042	2124	2125	2128	rBV2	522	448	0.05%	0.006%
88	14.146	2140	2142	2144	rVB2	429	366	0.04%	0.005%
89	14.170	2144	2146	2148	rBV	480	502	0.05%	0.007%
90	14.231	2155	2156	2159	rBV2	503	416	0.04%	0.006%
91	14.701	2232	2233	2234	rBV	671	413	0.04%	0.006%
92	14.762	2242	2243	2246	rVB	737	461	0.05%	0.006%
93	14.792	2246	2248	2249	rBV2	445	429	0.04%	0.006%
94	15.005	2281	2283	2284	rBV2	442	342	0.03%	0.005%
95	15.097	2296	2298	2300	rBV2	528	495	0.05%	0.007%
96	15.493	2362	2363	2366	rBV3	755	477	0.05%	0.007%
97	15.767	2407	2408	2411	rVB2	662	579	0.06%	0.008%
98	15.816	2413	2416	2417	rBV2	462	561	0.06%	0.008%
99	16.286	2492	2493	2497	rBV3	823	891	0.09%	0.012%
100	16.414	2512	2514	2516	rBV2	736	573	0.06%	0.008%




Sum of corrected areas: 7173087

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043525.D
Acq On : 25 Oct 2024 16:01
Operator : JC/MD
Sample : P4429-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

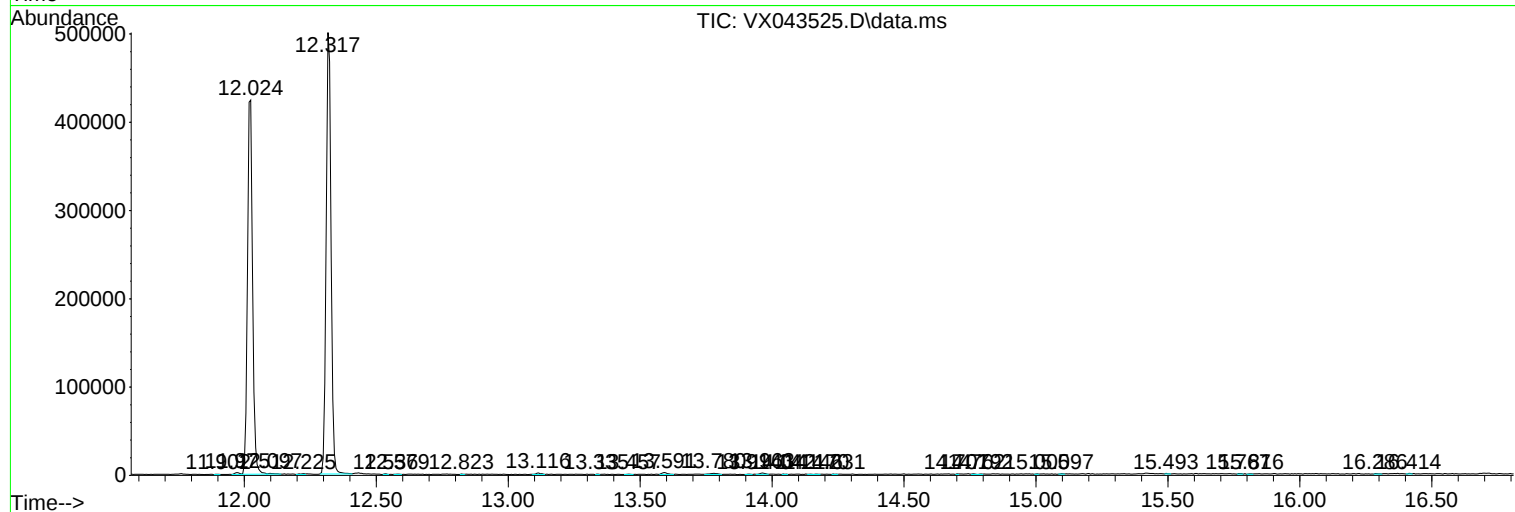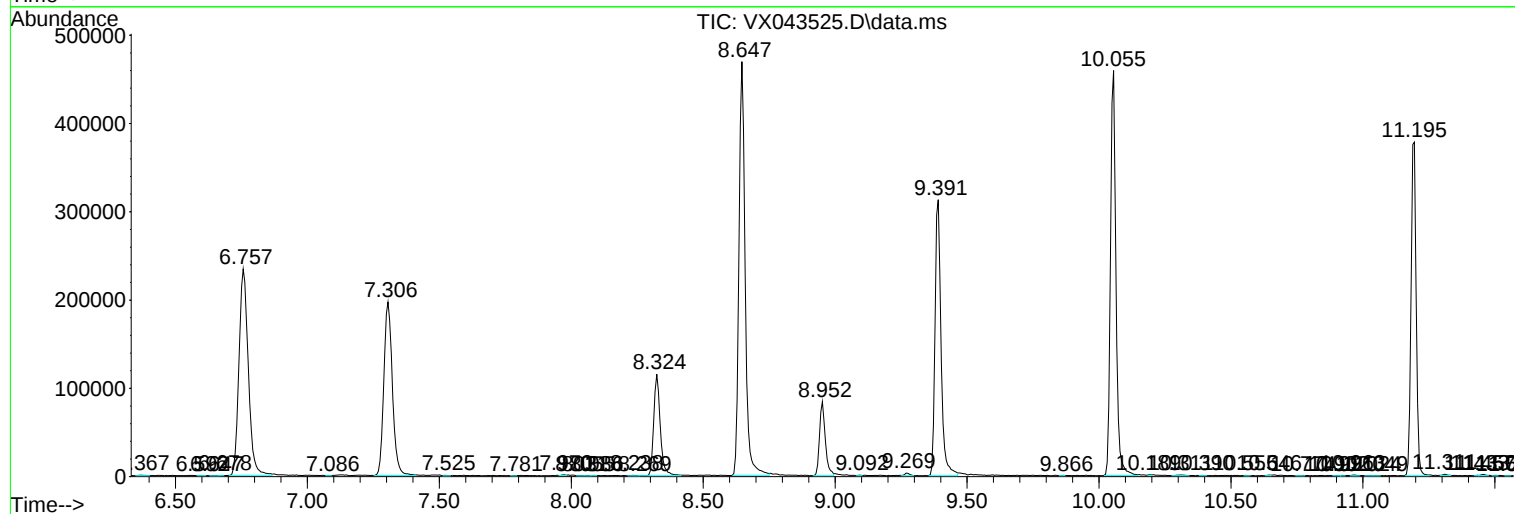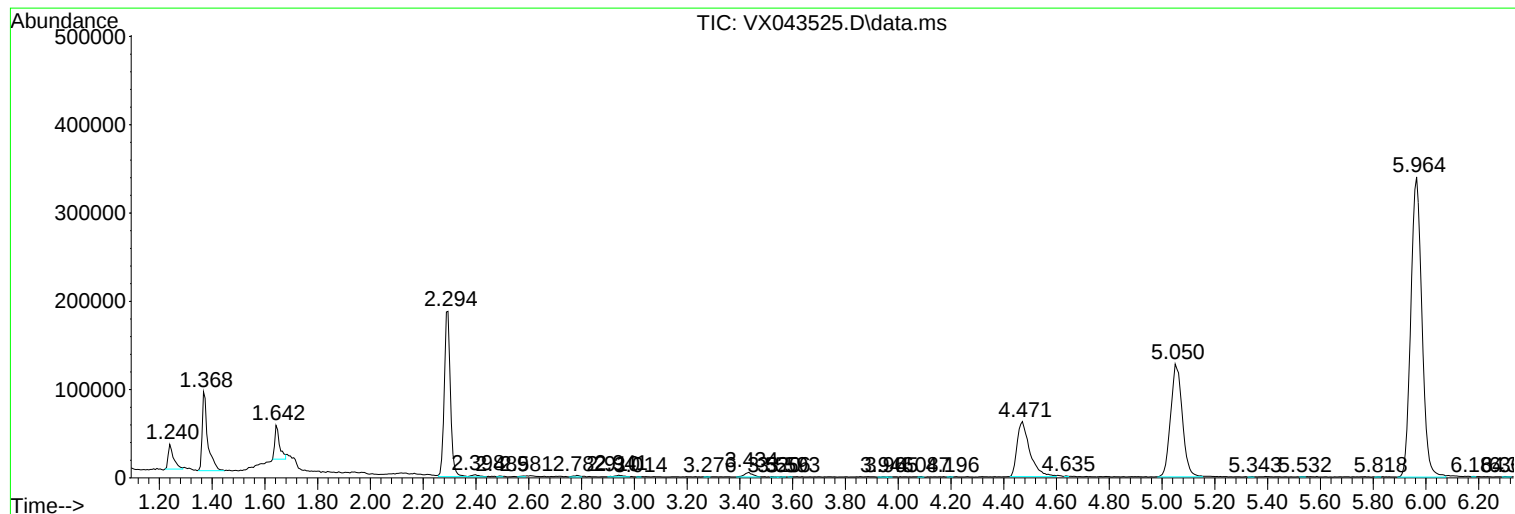

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043525.D
Acq On : 25 Oct 2024 16:01
Operator : JC/MD
Sample : P4429-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043525.D
Acq On : 25 Oct 2024 16:01
Operator : JC/MD
Sample : P4429-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc