

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043526.D
 Acq On : 25 Oct 2024 16:24
 Operator : JC/MD
 Sample : P4415-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV	30009	44489	4.55%	0.623%
2	1.368	43	46	57	rVB	90695	124449	12.71%	1.743%
3	1.642	89	91	110	rVB	50011	136748	13.97%	1.915%
4	2.288	191	197	209	rVB	190533	296425	30.28%	4.152%
5	2.569	241	243	245	rBV2	554	538	0.05%	0.008%
6	2.782	275	278	282	rVB4	1593	2527	0.26%	0.035%
7	2.953	300	306	309	rBV3	1258	2868	0.29%	0.040%
8	3.111	331	332	334	rVB	631	277	0.03%	0.004%
9	3.129	334	335	337	rBV2	307	263	0.03%	0.004%
10	3.258	352	356	357	rBV2	360	397	0.04%	0.006%
11	3.379	374	376	377	rBV2	359	342	0.03%	0.005%
12	3.428	377	384	393	rVB3	6180	15665	1.60%	0.219%
13	3.550	401	404	405	rBV2	442	343	0.04%	0.005%
14	3.696	426	428	429	rBV2	405	321	0.03%	0.004%
15	3.751	432	437	438	rBV2	431	615	0.06%	0.009%
16	3.873	455	457	461	rBV2	382	446	0.05%	0.006%
17	4.032	481	483	486	rBV	352	365	0.04%	0.005%
18	4.123	497	498	502	rBV	373	345	0.04%	0.005%
19	4.251	517	519	521	rVB2	561	431	0.04%	0.006%
20	4.318	528	530	532	rVB	386	329	0.03%	0.005%
21	4.471	547	555	578	rBV2	56391	205428	20.99%	2.878%
22	4.873	619	621	622	rVB	499	246	0.03%	0.003%
23	5.050	638	650	672	rBV	128298	394860	40.34%	5.531%
24	5.379	702	704	705	rBV	397	396	0.04%	0.006%
25	5.580	735	737	738	rVB2	882	534	0.05%	0.007%
26	5.653	748	749	754	rVB3	574	560	0.06%	0.008%
27	5.702	754	757	759	rBV	628	743	0.08%	0.010%
28	5.745	763	764	767	rVB2	363	331	0.03%	0.005%
29	5.788	767	771	774	rVB3	431	477	0.05%	0.007%
30	5.849	777	781	782	rBV2	416	606	0.06%	0.008%
31	5.964	788	800	822	rBV2	326531	978794	100.00%	13.710%
32	6.318	855	858	859	rBV2	364	366	0.04%	0.005%
33	6.355	861	864	865	rBV	509	430	0.04%	0.006%
34	6.434	873	877	879	rBV2	324	491	0.05%	0.007%
35	6.483	883	885	886	rVB2	488	250	0.03%	0.004%
36	6.568	898	899	902	rVB2	501	388	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043526.D
 Acq On : 25 Oct 2024 16:24
 Operator : JC/MD
 Sample : P4415-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

37	6.611	904	906	907	rVV2	452	266	0.03%	0.004%
38	6.629	907	909	912	rVB2	414	357	0.04%	0.005%
39	6.757	921	930	948	rBV	236118	573588	58.60%	8.035%
40	7.062	978	980	981	rBV	425	310	0.03%	0.004%
41	7.123	984	990	992	rBV5	889	1608	0.16%	0.023%
42	7.178	998	999	1001	rBV2	500	497	0.05%	0.007%
43	7.208	1001	1004	1006	rVV3	596	830	0.08%	0.012%
44	7.306	1012	1020	1033	rBV	196447	433142	44.25%	6.067%
45	7.440	1040	1042	1045	rBV3	602	791	0.08%	0.011%
46	7.580	1062	1065	1067	rBV	500	382	0.04%	0.005%
47	7.610	1067	1070	1071	rVV2	488	436	0.04%	0.006%
48	7.647	1075	1076	1078	rBV2	416	268	0.03%	0.004%
49	7.812	1100	1103	1104	rBV2	253	291	0.03%	0.004%
50	7.952	1124	1126	1127	rVV2	602	391	0.04%	0.005%
51	8.049	1139	1142	1144	rBV2	416	437	0.04%	0.006%
52	8.092	1148	1149	1151	rBV	292	269	0.03%	0.004%
53	8.214	1167	1169	1172	rBV	434	410	0.04%	0.006%
54	8.324	1181	1187	1202	rBV	115241	195426	19.97%	2.737%
55	8.647	1234	1240	1257	rBV	467628	764817	78.14%	10.713%
56	8.952	1285	1290	1305	rBV	77467	125639	12.84%	1.760%
57	9.110	1314	1316	1320	rVB2	535	455	0.05%	0.006%
58	9.275	1339	1343	1350	rBV3	2150	3085	0.32%	0.043%
59	9.330	1350	1352	1354	rVB	502	274	0.03%	0.004%
60	9.391	1357	1362	1387	rVV	296236	479947	49.03%	6.723%
61	9.927	1449	1450	1452	rVB	483	244	0.02%	0.003%
62	10.055	1465	1471	1485	rBV	447687	657550	67.18%	9.211%
63	10.311	1510	1513	1515	rBV2	709	728	0.07%	0.010%
64	10.384	1523	1525	1528	rVB2	470	425	0.04%	0.006%
65	10.646	1566	1568	1571	rBV3	524	629	0.06%	0.009%
66	10.744	1582	1584	1586	rBV	530	470	0.05%	0.007%
67	10.890	1606	1608	1611	rVB2	568	614	0.06%	0.009%
68	10.927	1611	1614	1616	rBV2	448	592	0.06%	0.008%
69	10.963	1616	1620	1621	rBV2	549	671	0.07%	0.009%
70	11.189	1652	1657	1667	rBV	356461	483203	49.37%	6.768%
71	11.658	1732	1734	1735	rBV2	334	261	0.03%	0.004%
72	11.683	1737	1738	1740	rBV2	443	283	0.03%	0.004%
73	11.756	1747	1750	1753	rBV3	1091	1338	0.14%	0.019%
74	11.823	1759	1761	1762	rVB	491	279	0.03%	0.004%
75	11.847	1763	1765	1768	rBV2	415	352	0.04%	0.005%
76	11.945	1779	1781	1782	rVV	567	339	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043526.D
 Acq On : 25 Oct 2024 16:24
 Operator : JC/MD
 Sample : P4415-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	11.969	1782	1785	1788	rVV3	1631	2219	0.23%	0.031%
78	12.018	1788	1793	1812	rVB	412490	554544	56.66%	7.768%
79	12.317	1837	1842	1850	rBV	476129	621407	63.49%	8.704%
80	12.500	1871	1872	1878	rVB5	696	948	0.10%	0.013%
81	12.762	1913	1915	1917	rVB2	489	392	0.04%	0.005%
82	13.085	1966	1968	1970	rBV	373	293	0.03%	0.004%
83	13.115	1970	1973	1976	rVV3	1684	1918	0.20%	0.027%
84	13.170	1980	1982	1986	rVV3	525	519	0.05%	0.007%
85	13.402	2019	2020	2022	rBV	354	293	0.03%	0.004%
86	13.457	2028	2029	2034	rBV3	511	689	0.07%	0.010%
87	13.512	2036	2038	2040	rBV2	444	409	0.04%	0.006%
88	13.591	2048	2051	2057	rVB4	1459	1866	0.19%	0.026%
89	13.689	2066	2067	2069	rBV	539	441	0.05%	0.006%
90	13.780	2078	2082	2085	rVB4	911	1248	0.13%	0.017%
91	13.963	2109	2112	2117	rVB2	1754	1997	0.20%	0.028%
92	14.030	2121	2123	2125	rVB2	565	494	0.05%	0.007%
93	14.097	2133	2134	2137	rBV2	333	286	0.03%	0.004%
94	14.195	2147	2150	2154	rBV3	604	938	0.10%	0.013%
95	14.384	2179	2181	2186	rBV3	827	600	0.06%	0.008%
96	14.853	2257	2258	2259	rBV	475	327	0.03%	0.005%
97	14.999	2279	2282	2283	rBV2	679	576	0.06%	0.008%
98	15.066	2291	2293	2295	rBV2	524	420	0.04%	0.006%
99	15.719	2397	2400	2401	rBV2	754	719	0.07%	0.010%
100	16.414	2513	2514	2516	rVB	741	505	0.05%	0.007%




Sum of corrected areas: 7139025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043526.D
Acq On : 25 Oct 2024 16:24
Operator : JC/MD
Sample : P4415-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

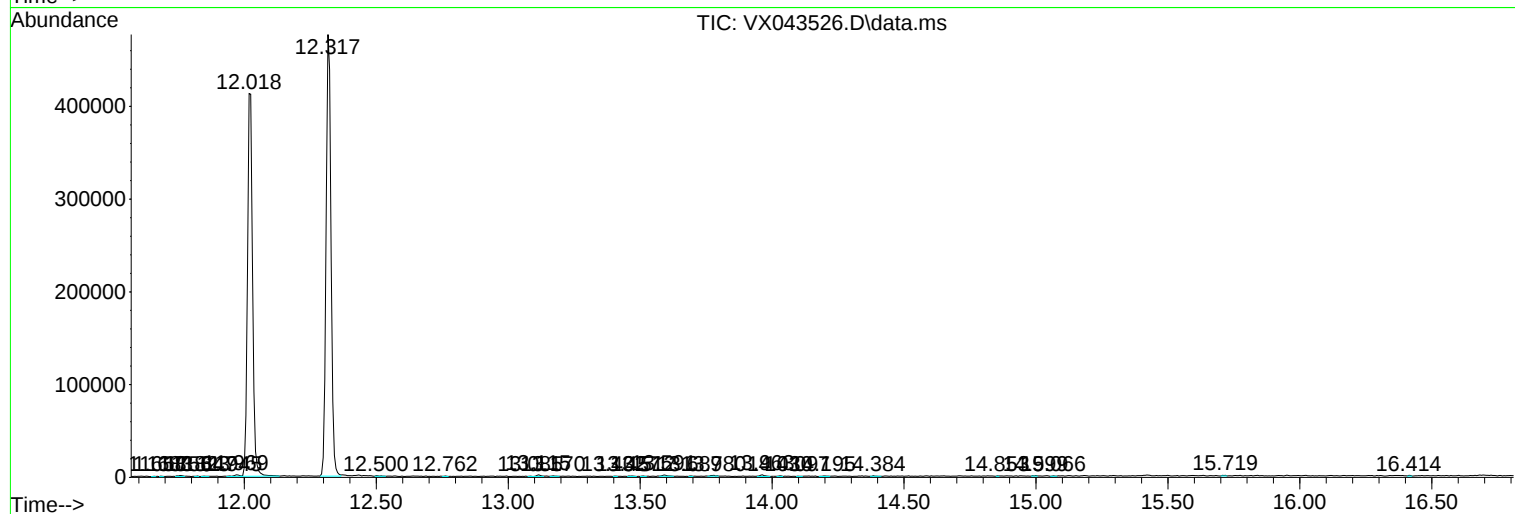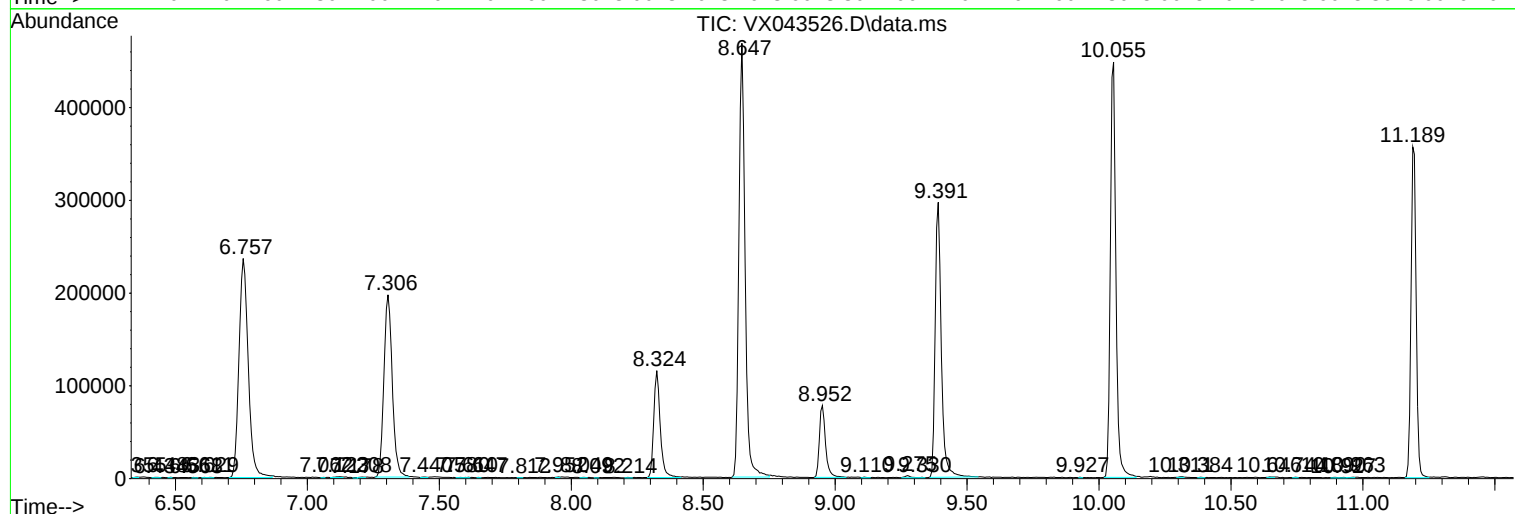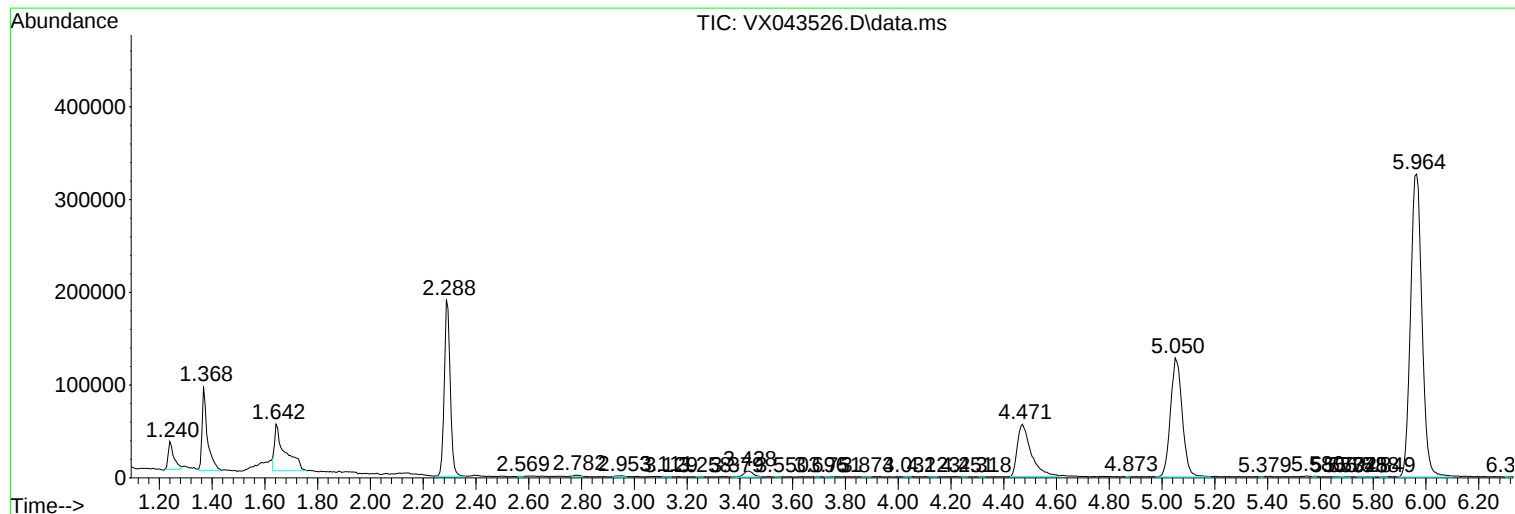

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043526.D
Acq On : 25 Oct 2024 16:24
Operator : JC/MD
Sample : P4415-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043526.D
Acq On : 25 Oct 2024 16:24
Operator : JC/MD
Sample : P4415-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc