

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043527.D
 Acq On : 25 Oct 2024 16:47
 Operator : JC/MD
 Sample : P4436-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV	36434	50534	6.35%	0.804%
2	1.368	43	46	59	rVB	65690	90130	11.33%	1.434%
3	1.642	89	91	102	rBV	27389	45220	5.68%	0.720%
4	2.288	191	197	205	rBV	138433	213535	26.84%	3.398%
5	2.575	240	244	245	rBV3	840	1262	0.16%	0.020%
6	2.684	260	262	264	rVB	404	321	0.04%	0.005%
7	2.782	276	278	283	rVB4	1423	1820	0.23%	0.029%
8	2.947	298	305	311	rBV3	1572	3836	0.48%	0.061%
9	3.081	325	327	329	rBV3	380	368	0.05%	0.006%
10	3.221	346	350	353	rVB3	294	510	0.06%	0.008%
11	3.258	353	356	357	rBV	393	386	0.05%	0.006%
12	3.434	379	385	393	rVV2	6630	14296	1.80%	0.227%
13	3.666	419	423	424	rBV2	305	342	0.04%	0.005%
14	4.007	477	479	482	rVB	324	323	0.04%	0.005%
15	4.093	491	493	494	rBV	449	358	0.05%	0.006%
16	4.276	520	523	524	rBV	412	402	0.05%	0.006%
17	4.471	545	555	578	rBV	52966	194216	24.41%	3.090%
18	5.056	638	651	666	rBV	104558	324475	40.79%	5.163%
19	5.214	676	677	682	rVB	497	528	0.07%	0.008%
20	5.385	703	705	706	rBV	637	509	0.06%	0.008%
21	5.477	718	720	725	rVB2	615	934	0.12%	0.015%
22	5.525	725	728	730	rBV2	517	626	0.08%	0.010%
23	5.550	730	732	736	rBV2	534	487	0.06%	0.008%
24	5.653	747	749	753	rVB2	321	345	0.04%	0.005%
25	5.964	788	800	817	rBV3	274910	795530	100.00%	12.659%
26	6.196	835	838	840	rBV2	471	592	0.07%	0.009%
27	6.361	862	865	866	rBV3	499	585	0.07%	0.009%
28	6.434	875	877	879	rBV2	346	391	0.05%	0.006%
29	6.678	915	917	918	rBV	346	351	0.04%	0.006%
30	6.757	921	930	944	rBV	243454	586660	73.74%	9.335%
31	7.013	969	972	976	rBV3	597	991	0.12%	0.016%
32	7.123	985	990	993	rBV6	791	1456	0.18%	0.023%
33	7.208	1002	1004	1005	rBV	659	596	0.07%	0.009%
34	7.306	1011	1020	1036	rBV	166236	368381	46.31%	5.862%
35	7.684	1080	1082	1085	rVB3	398	335	0.04%	0.005%
36	7.885	1113	1115	1117	rBV2	342	331	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043527.D
 Acq On : 25 Oct 2024 16:47
 Operator : JC/MD
 Sample : P4436-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
 Title : VOC Analysis

37	7.909	1117	1119	1121	rVB	442	319	0.04%	0.005%
38	7.964	1125	1128	1131	rBV3	831	1157	0.15%	0.018%
39	8.110	1151	1152	1155	rBV2	335	327	0.04%	0.005%
40	8.214	1167	1169	1171	rBV	396	372	0.05%	0.006%
41	8.324	1181	1187	1200	rBV	99716	171183	21.52%	2.724%
42	8.464	1208	1210	1212	rVB3	463	362	0.05%	0.006%
43	8.647	1233	1240	1258	rBV	364695	602425	75.73%	9.586%
44	8.952	1285	1290	1300	rBV	69122	108685	13.66%	1.729%
45	9.104	1313	1315	1318	rVB	634	618	0.08%	0.010%
46	9.134	1318	1320	1322	rVV3	368	427	0.05%	0.007%
47	9.159	1322	1324	1326	rVB3	539	414	0.05%	0.007%
48	9.256	1335	1340	1341	rBV2	692	775	0.10%	0.012%
49	9.275	1341	1343	1349	rVB3	1685	2214	0.28%	0.035%
50	9.336	1349	1353	1354	rBV	416	459	0.06%	0.007%
51	9.391	1356	1362	1382	rBV	269617	443470	55.75%	7.057%
52	9.677	1408	1409	1413	rVB3	541	562	0.07%	0.009%
53	9.726	1415	1417	1420	rVV2	365	433	0.05%	0.007%
54	9.915	1446	1448	1450	rBV3	395	380	0.05%	0.006%
55	9.958	1453	1455	1459	rBV3	328	512	0.06%	0.008%
56	10.055	1465	1471	1486	rBV	463910	675265	84.88%	10.745%
57	10.195	1492	1494	1496	rVV2	829	513	0.06%	0.008%
58	10.244	1500	1502	1505	rVB	441	421	0.05%	0.007%
59	10.293	1508	1510	1511	rBV2	388	335	0.04%	0.005%
60	10.311	1511	1513	1516	rVB2	714	716	0.09%	0.011%
61	10.640	1566	1567	1568	rBV	501	328	0.04%	0.005%
62	10.713	1577	1579	1584	rVB2	452	759	0.10%	0.012%
63	10.854	1600	1602	1604	rBV2	698	685	0.09%	0.011%
64	10.927	1612	1614	1616	rBV3	350	411	0.05%	0.007%
65	11.195	1652	1658	1669	rVV	328162	436184	54.83%	6.941%
66	11.305	1675	1676	1677	rBV	664	314	0.04%	0.005%
67	11.451	1695	1700	1706	rBV3	1011	2248	0.28%	0.036%
68	11.555	1714	1717	1718	rBV2	464	425	0.05%	0.007%
69	11.622	1725	1728	1730	rBV	487	537	0.07%	0.009%
70	11.756	1746	1750	1755	rVB3	644	762	0.10%	0.012%
71	11.927	1777	1778	1782	rBV3	435	557	0.07%	0.009%
72	11.975	1783	1786	1788	rBV	1367	1182	0.15%	0.019%
73	12.024	1788	1794	1806	rBV	431982	570007	71.65%	9.070%
74	12.219	1825	1826	1829	rVB2	527	330	0.04%	0.005%
75	12.317	1837	1842	1852	rBV	412879	540714	67.97%	8.604%
76	12.634	1891	1894	1896	rBV	493	556	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043527.D
 Acq On : 25 Oct 2024 16:47
 Operator : JC/MD
 Sample : P4436-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	12.786	1918	1919	1923	rVB	529	480	0.06%	0.008%
78	12.835	1923	1927	1928	rBV	533	514	0.06%	0.008%
79	12.914	1939	1940	1944	rVB2	373	331	0.04%	0.005%
80	13.024	1955	1958	1959	rVB	513	450	0.06%	0.007%
81	13.042	1959	1961	1963	rBV2	401	491	0.06%	0.008%
82	13.085	1966	1968	1970	rVV2	341	364	0.05%	0.006%
83	13.115	1970	1973	1976	rVB2	936	1226	0.15%	0.020%
84	13.323	2005	2007	2009	rVB2	412	324	0.04%	0.005%
85	13.402	2018	2020	2023	rBV2	377	506	0.06%	0.008%
86	13.591	2047	2051	2056	rVB3	1398	1680	0.21%	0.027%
87	13.640	2056	2059	2061	rBV3	433	406	0.05%	0.006%
88	13.682	2065	2066	2068	rBV	404	413	0.05%	0.007%
89	13.963	2109	2112	2114	rBV3	1284	1223	0.15%	0.019%
90	14.079	2129	2131	2133	rVB2	476	423	0.05%	0.007%
91	14.280	2160	2164	2165	rBV2	532	652	0.08%	0.010%
92	14.353	2172	2176	2177	rVB3	773	695	0.09%	0.011%
93	14.384	2177	2181	2182	rBV2	437	640	0.08%	0.010%
94	14.475	2194	2196	2198	rBV2	454	407	0.05%	0.006%
95	14.536	2205	2206	2207	rBV	584	333	0.04%	0.005%
96	14.615	2217	2219	2221	rBV	526	430	0.05%	0.007%
97	14.737	2237	2239	2242	rBV4	588	590	0.07%	0.009%
98	15.280	2327	2328	2329	rBV	623	369	0.05%	0.006%
99	15.859	2422	2423	2425	rBV	683	533	0.07%	0.008%
100	16.597	2542	2544	2545	rBV	667	540	0.07%	0.009%




Sum of corrected areas: 6284325

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043527.D
Acq On : 25 Oct 2024 16:47
Operator : JC/MD
Sample : P4436-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

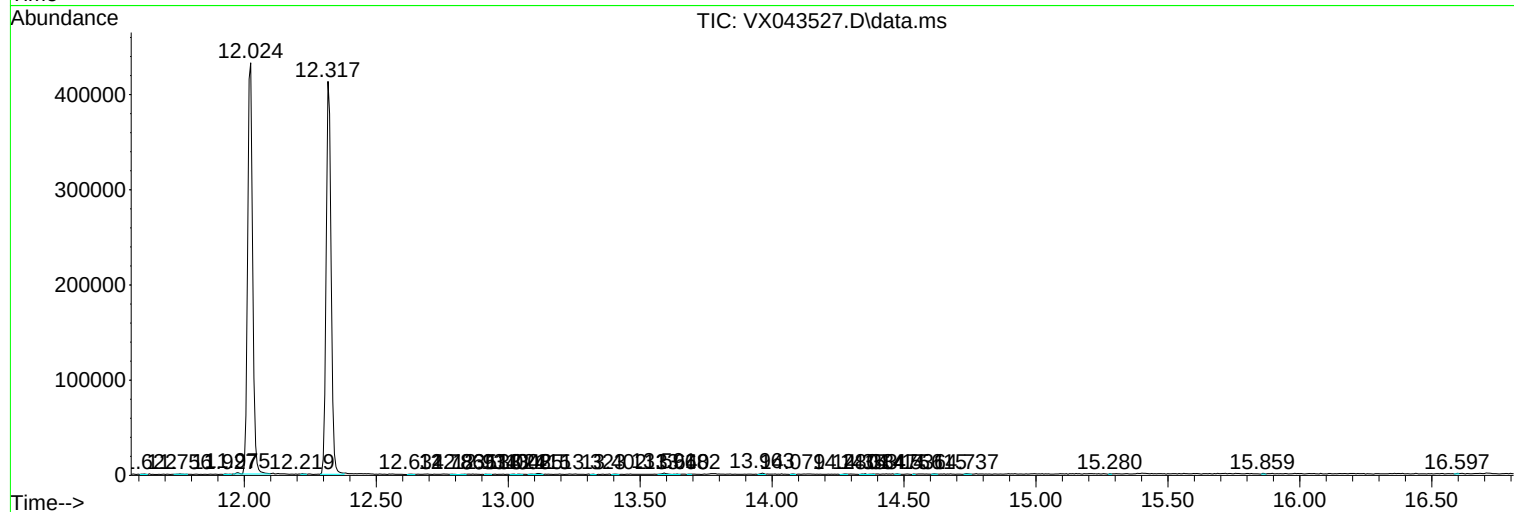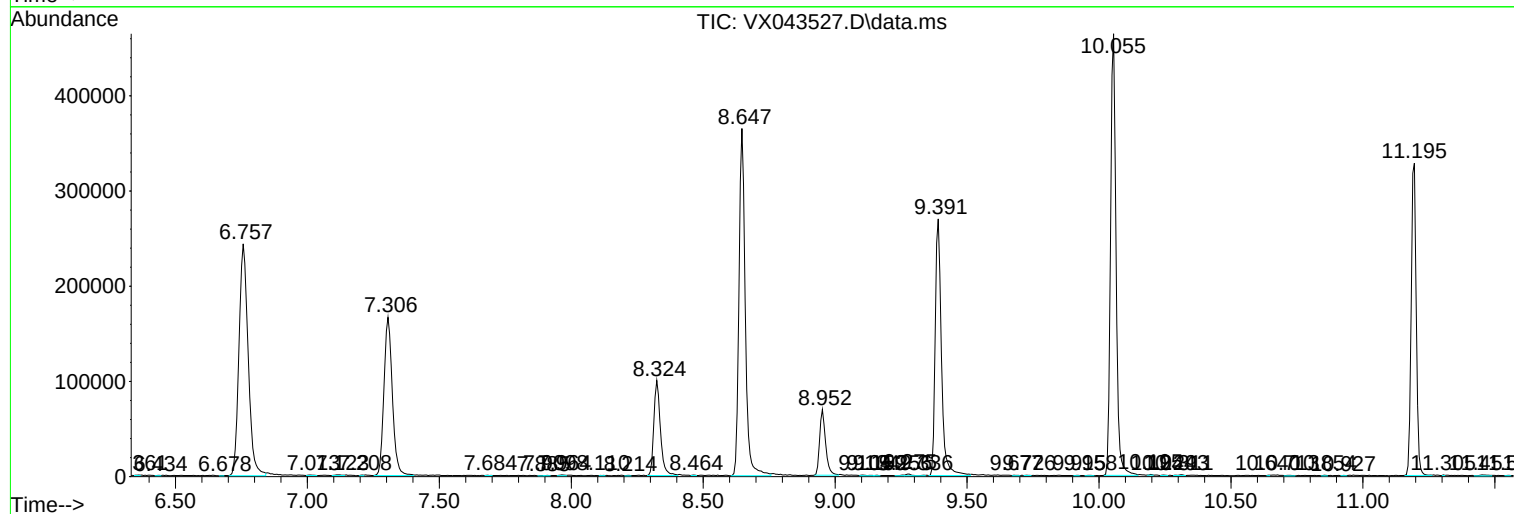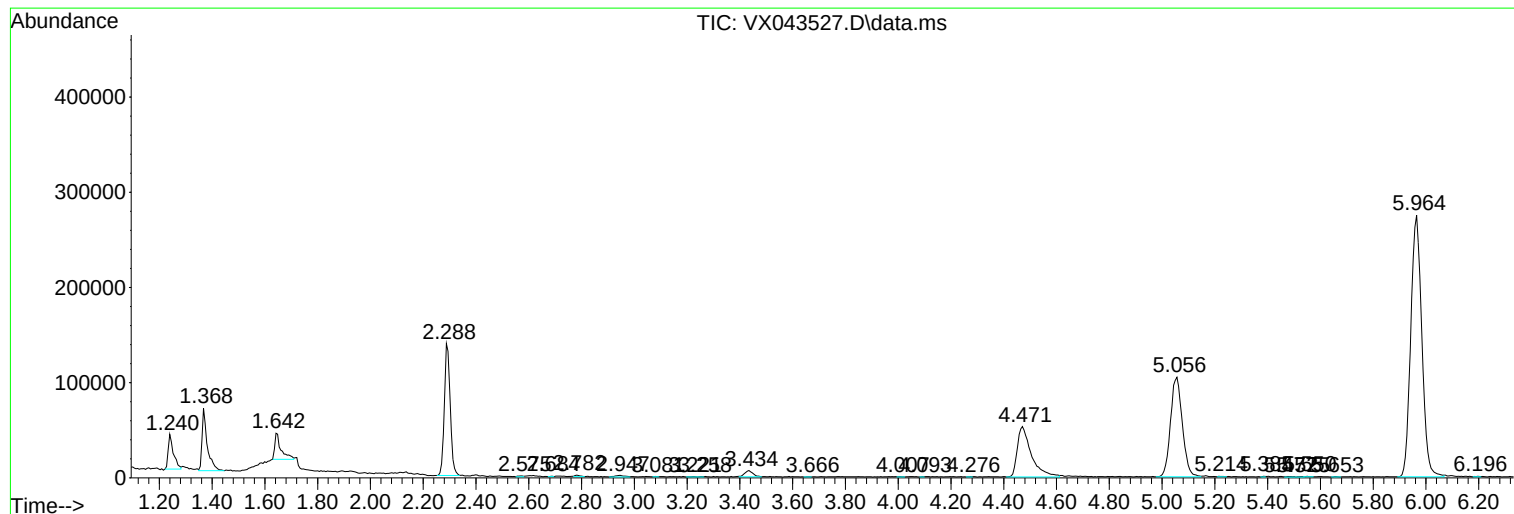

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043527.D
Acq On : 25 Oct 2024 16:47
Operator : JC/MD
Sample : P4436-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043527.D
Acq On : 25 Oct 2024 16:47
Operator : JC/MD
Sample : P4436-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc