

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043528.D
 Acq On : 25 Oct 2024 17:10
 Operator : JC/MD
 Sample : P4493-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	33	rBV	48949	70398	8.72%	1.120%
2	1.367	43	46	59	rVB	68730	97395	12.06%	1.550%
3	1.642	89	91	94	rBV	28022	31742	3.93%	0.505%
4	2.294	192	198	207	rVB	139665	223856	27.72%	3.563%
5	2.392	211	214	216	rBV3	1795	2087	0.26%	0.033%
6	2.581	242	245	248	rBV3	563	764	0.09%	0.012%
7	2.611	248	250	251	rBV	653	512	0.06%	0.008%
8	2.776	273	277	284	rVB5	1520	3194	0.40%	0.051%
9	2.843	284	288	289	rVB3	503	608	0.08%	0.010%
10	2.867	289	292	293	rBV2	402	546	0.07%	0.009%
11	2.928	298	302	304	rBV2	1001	1426	0.18%	0.023%
12	2.946	304	305	311	rVB3	1388	1587	0.20%	0.025%
13	3.087	326	328	330	rVB	436	324	0.04%	0.005%
14	3.135	334	336	339	rBV2	324	346	0.04%	0.006%
15	3.434	378	385	395	rVB2	6499	14298	1.77%	0.228%
16	3.501	395	396	398	rBV	616	292	0.04%	0.005%
17	3.666	421	423	425	rBV2	802	844	0.10%	0.013%
18	3.690	425	427	428	rVV2	448	362	0.04%	0.006%
19	3.727	431	433	435	rVV	545	529	0.07%	0.008%
20	3.770	439	440	443	rVB2	402	353	0.04%	0.006%
21	3.806	443	446	447	rBV2	351	439	0.05%	0.007%
22	4.117	495	497	498	rBV	485	262	0.03%	0.004%
23	4.135	498	500	502	rVB	281	243	0.03%	0.004%
24	4.379	539	540	543	rBV2	322	262	0.03%	0.004%
25	4.471	547	555	577	rBV	53661	197045	24.40%	3.136%
26	4.849	616	617	620	rVB	508	249	0.03%	0.004%
27	5.056	639	651	667	rBV	106400	333263	41.27%	5.304%
28	5.391	702	706	712	rBV3	805	1860	0.23%	0.030%
29	5.458	715	717	719	rVV	360	267	0.03%	0.004%
30	5.739	759	763	764	rBV2	434	570	0.07%	0.009%
31	5.861	781	783	786	rBV2	340	414	0.05%	0.007%
32	5.964	788	800	814	rBV2	275484	807523	100.00%	12.853%
33	6.214	840	841	844	rVB3	609	402	0.05%	0.006%
34	6.287	850	853	854	rBV2	395	397	0.05%	0.006%
35	6.379	863	868	871	rBV3	630	1130	0.14%	0.018%
36	6.464	880	882	884	rBV	516	327	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043528.D
 Acq On : 25 Oct 2024 17:10
 Operator : JC/MD
 Sample : P4493-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

37	6.489	884	886	887	rVV	363	244	0.03%	0.004%
38	6.623	905	908	910	rBV2	381	366	0.05%	0.006%
39	6.702	919	921	922	rBV2	552	431	0.05%	0.007%
40	6.757	922	930	946	rVV	230523	559068	69.23%	8.898%
41	7.202	1002	1003	1004	rBV	712	445	0.06%	0.007%
42	7.305	1012	1020	1037	rVB	169460	373390	46.24%	5.943%
43	7.488	1048	1050	1052	rVB	616	429	0.05%	0.007%
44	7.738	1089	1091	1092	rBV	419	257	0.03%	0.004%
45	7.775	1096	1097	1099	rBV	399	324	0.04%	0.005%
46	7.830	1103	1106	1108	rBV2	406	418	0.05%	0.007%
47	7.854	1108	1110	1112	rVV	476	313	0.04%	0.005%
48	7.885	1114	1115	1117	rBV	370	332	0.04%	0.005%
49	8.031	1136	1139	1140	rBV2	403	447	0.06%	0.007%
50	8.104	1147	1151	1152	rBV2	394	502	0.06%	0.008%
51	8.263	1175	1177	1181	rBV	512	649	0.08%	0.010%
52	8.324	1181	1187	1199	rBV	100701	172999	21.42%	2.754%
53	8.513	1217	1218	1219	rBV	492	321	0.04%	0.005%
54	8.647	1233	1240	1257	rBV	366654	610320	75.58%	9.714%
55	8.951	1285	1290	1304	rBV	74560	115600	14.32%	1.840%
56	9.183	1326	1328	1330	rBV	703	640	0.08%	0.010%
57	9.275	1339	1343	1346	rBV3	1569	1871	0.23%	0.030%
58	9.342	1352	1354	1356	rBV	356	260	0.03%	0.004%
59	9.390	1356	1362	1374	rBV	283607	452935	56.09%	7.209%
60	9.653	1404	1405	1408	rBV	457	379	0.05%	0.006%
61	10.055	1465	1471	1485	rBV	436591	643535	79.69%	10.243%
62	10.311	1509	1513	1517	rVB4	829	1324	0.16%	0.021%
63	10.433	1531	1533	1534	rVB	426	300	0.04%	0.005%
64	10.854	1600	1602	1604	rVB2	362	255	0.03%	0.004%
65	10.933	1612	1615	1618	rBV2	468	632	0.08%	0.010%
66	10.969	1618	1621	1622	rBV2	583	572	0.07%	0.009%
67	11.049	1631	1634	1637	rBV3	355	649	0.08%	0.010%
68	11.189	1652	1657	1667	rBV	335132	448949	55.60%	7.146%
69	11.311	1675	1677	1682	rVB3	1364	1432	0.18%	0.023%
70	11.451	1695	1700	1705	rBV2	721	1311	0.16%	0.021%
71	11.762	1746	1751	1754	rVV4	720	1023	0.13%	0.016%
72	11.805	1757	1758	1760	rBV2	350	287	0.04%	0.005%
73	11.908	1774	1775	1776	rBV	604	298	0.04%	0.005%
74	11.975	1782	1786	1788	rBV3	1238	1325	0.16%	0.021%
75	12.018	1788	1793	1802	rBV	401673	536576	66.45%	8.540%
76	12.146	1812	1814	1815	rBV2	589	369	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043528.D
 Acq On : 25 Oct 2024 17:10
 Operator : JC/MD
 Sample : P4493-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1852	rBV	411445	539449	66.80%	8.586%
78	12.762	1912	1915	1919	rVB3	617	773	0.10%	0.012%
79	12.823	1923	1925	1926	rBV	551	359	0.04%	0.006%
80	13.115	1970	1973	1977	rVB	1224	1040	0.13%	0.017%
81	13.341	2008	2010	2011	rBV	450	282	0.03%	0.004%
82	13.597	2048	2052	2054	rBV3	1028	1422	0.18%	0.023%
83	13.634	2056	2058	2060	rBV2	368	357	0.04%	0.006%
84	13.786	2078	2083	2085	rBV3	906	1545	0.19%	0.025%
85	13.871	2095	2097	2098	rVB	519	241	0.03%	0.004%
86	13.914	2102	2104	2106	rBV	448	461	0.06%	0.007%
87	13.963	2109	2112	2117	rBV4	868	1192	0.15%	0.019%
88	14.201	2149	2151	2154	rBV	644	734	0.09%	0.012%
89	14.274	2161	2163	2167	rBV3	406	645	0.08%	0.010%
90	14.444	2189	2191	2198	rVB3	633	1143	0.14%	0.018%
91	14.505	2198	2201	2202	rBV	633	593	0.07%	0.009%
92	14.877	2260	2262	2264	rVB2	555	355	0.04%	0.006%
93	14.902	2264	2266	2268	rBV3	453	422	0.05%	0.007%
94	14.926	2268	2270	2272	rVB2	427	361	0.04%	0.006%
95	15.133	2302	2304	2307	rBV2	555	614	0.08%	0.010%
96	15.463	2356	2358	2360	rBV2	731	806	0.10%	0.013%
97	15.841	2418	2420	2423	rBV3	653	589	0.07%	0.009%
98	15.901	2428	2430	2432	rBV2	714	433	0.05%	0.007%
99	16.487	2524	2526	2528	rBV2	683	730	0.09%	0.012%
100	16.633	2548	2550	2551	rBV	646	314	0.04%	0.005%




Sum of corrected areas: 6282753

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043528.D
Acq On : 25 Oct 2024 17:10
Operator : JC/MD
Sample : P4493-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

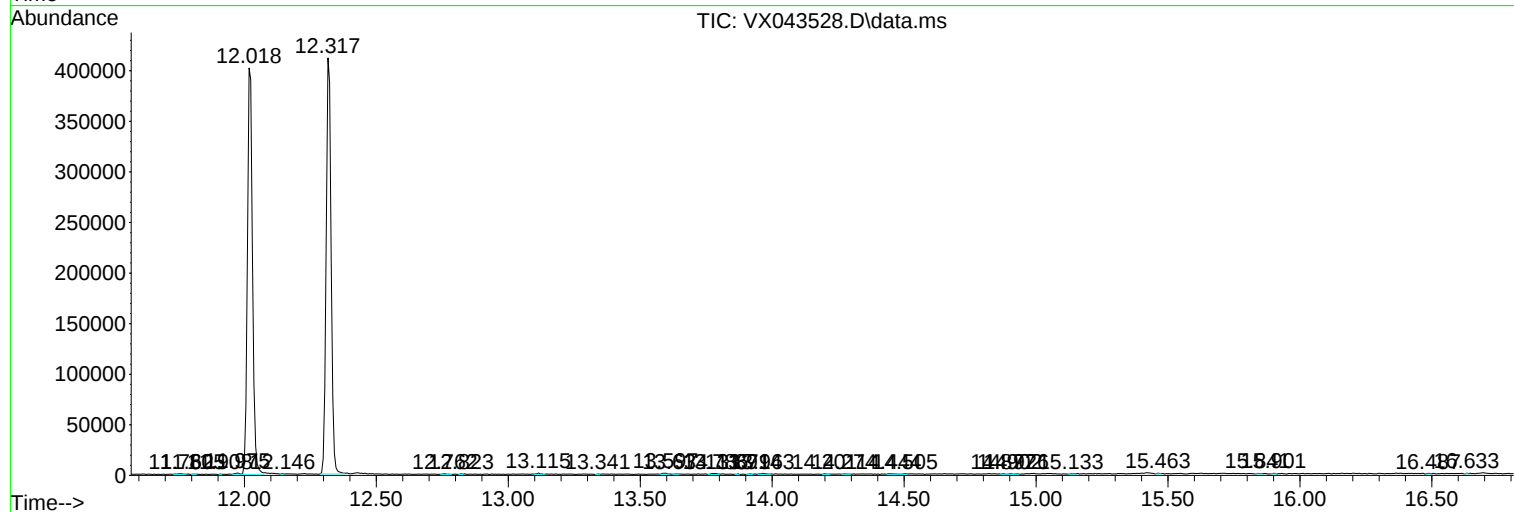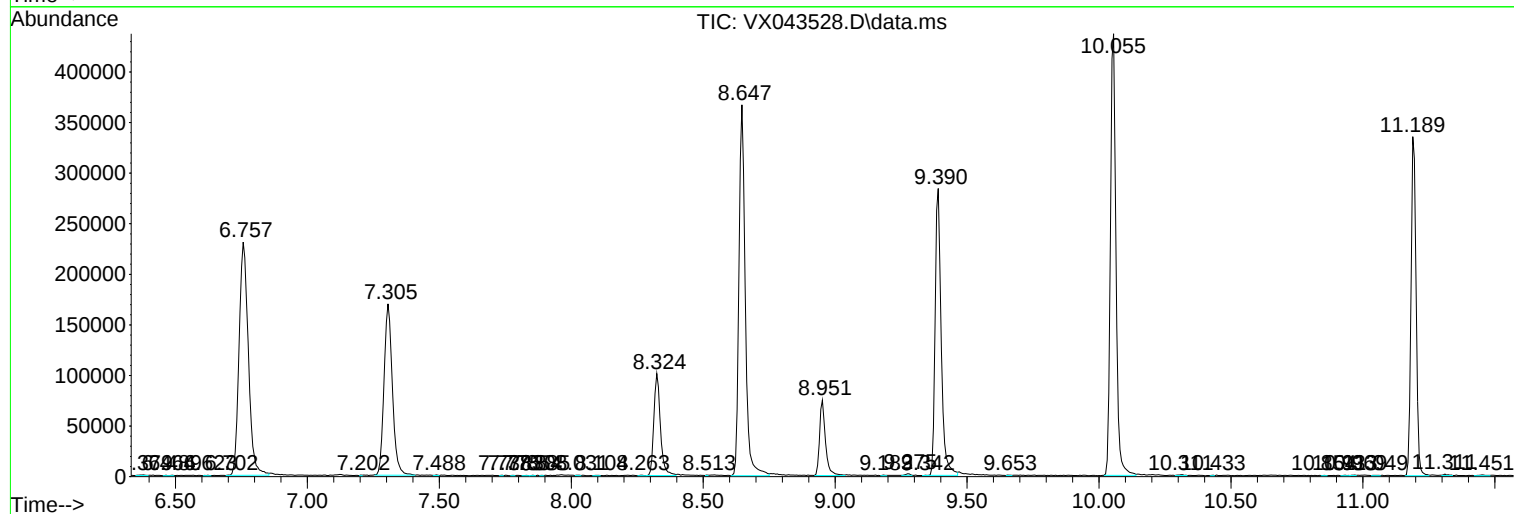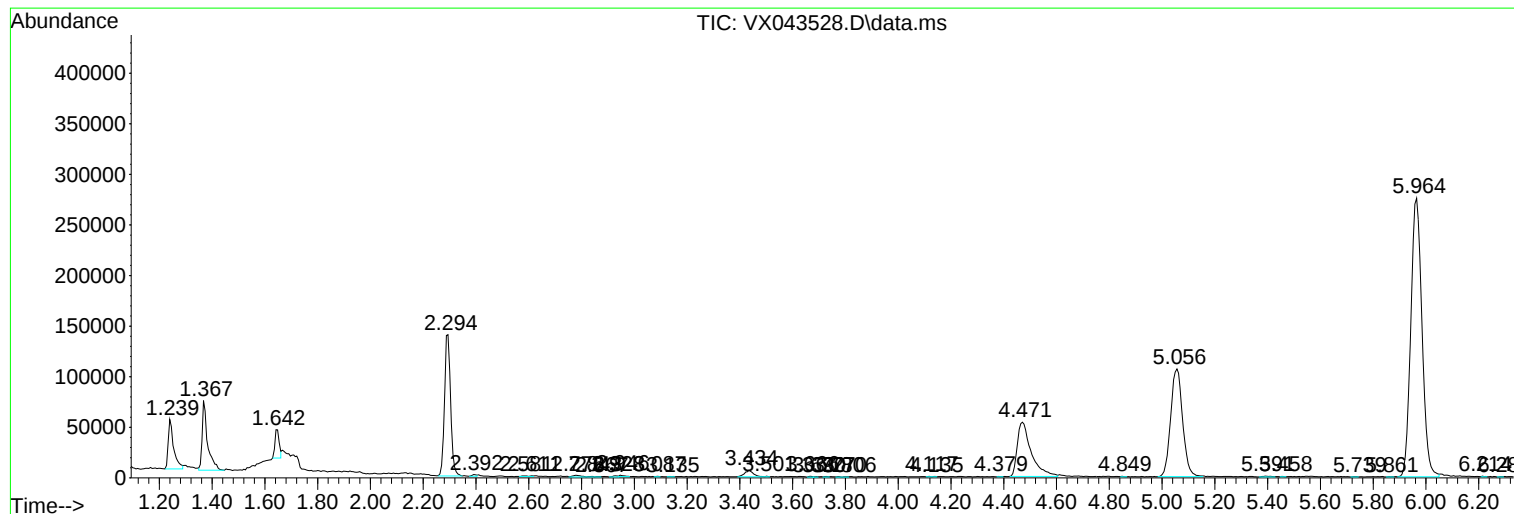

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043528.D
Acq On : 25 Oct 2024 17:10
Operator : JC/MD
Sample : P4493-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043528.D
Acq On : 25 Oct 2024 17:10
Operator : JC/MD
Sample : P4493-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
