

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043529.D
 Acq On : 25 Oct 2024 17:34
 Operator : JC/MD
 Sample : P4492-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV	39293	51823	6.63%	0.857%
2	1.368	43	46	58	rVB	62927	94527	12.08%	1.564%
3	1.642	89	91	97	rBV	27184	40073	5.12%	0.663%
4	2.288	191	197	210	rVB	136037	218226	27.90%	3.611%
5	2.563	240	242	243	rBV2	552	356	0.05%	0.006%
6	2.581	243	245	247	rBV2	609	585	0.07%	0.010%
7	3.038	317	320	322	rBV2	359	478	0.06%	0.008%
8	3.209	346	348	349	rBV2	324	316	0.04%	0.005%
9	3.300	360	363	366	rBV2	382	679	0.09%	0.011%
10	3.434	376	385	396	rVV4	8584	20500	2.62%	0.339%
11	3.715	430	431	433	rVV	395	337	0.04%	0.006%
12	3.800	443	445	448	rVV2	288	312	0.04%	0.005%
13	3.892	457	460	461	rBV2	348	386	0.05%	0.006%
14	4.007	477	479	481	rVB2	406	279	0.04%	0.005%
15	4.471	547	555	574	rBV	51618	189393	24.21%	3.134%
16	4.739	598	599	603	rVB2	791	700	0.09%	0.012%
17	4.776	603	605	606	rBV	352	354	0.05%	0.006%
18	5.050	639	650	665	rBV	102435	315791	40.37%	5.225%
19	5.239	679	681	682	rVB	573	295	0.04%	0.005%
20	5.440	712	714	717	rVB2	389	313	0.04%	0.005%
21	5.471	717	719	721	rBV2	456	444	0.06%	0.007%
22	5.513	724	726	727	rBV	455	377	0.05%	0.006%
23	5.666	749	751	753	rBV	279	321	0.04%	0.005%
24	5.714	756	759	761	rBV2	277	342	0.04%	0.006%
25	5.873	783	785	787	rBV	380	316	0.04%	0.005%
26	5.964	788	800	818	rBV2	267124	782192	100.00%	12.941%
27	6.245	844	846	850	rBV2	401	612	0.08%	0.010%
28	6.348	860	863	864	rBV2	556	458	0.06%	0.008%
29	6.367	864	866	867	rBV2	445	332	0.04%	0.005%
30	6.476	883	884	887	rVB	513	413	0.05%	0.007%
31	6.568	898	899	904	rVB2	380	559	0.07%	0.009%
32	6.611	904	906	909	rBV2	531	613	0.08%	0.010%
33	6.659	913	914	917	rVB	663	433	0.06%	0.007%
34	6.757	921	930	947	rBV	223457	539895	69.02%	8.933%
35	7.086	982	984	985	rBV2	436	332	0.04%	0.005%
36	7.306	1012	1020	1037	rBV	162934	359013	45.90%	5.940%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043529.D
 Acq On : 25 Oct 2024 17:34
 Operator : JC/MD
 Sample : P4492-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

37	7.751	1087	1093	1096	rBV3	384	792	0.10%	0.013%
38	7.958	1124	1127	1128	rBV	972	801	0.10%	0.013%
39	8.086	1146	1148	1150	rBV2	531	359	0.05%	0.006%
40	8.324	1181	1187	1200	rBV	98097	167094	21.36%	2.765%
41	8.427	1202	1204	1207	rVB2	791	759	0.10%	0.013%
42	8.452	1207	1208	1210	rBV2	591	521	0.07%	0.009%
43	8.647	1234	1240	1256	rBV	361242	589873	75.41%	9.760%
44	8.952	1285	1290	1299	rBV	67356	105638	13.51%	1.748%
45	9.067	1307	1309	1310	rBV	524	297	0.04%	0.005%
46	9.104	1314	1315	1317	rVB2	642	345	0.04%	0.006%
47	9.153	1320	1323	1325	rBV2	394	491	0.06%	0.008%
48	9.250	1336	1339	1340	rBV2	380	457	0.06%	0.008%
49	9.275	1340	1343	1346	rVB3	1397	1710	0.22%	0.028%
50	9.391	1356	1362	1381	rBV	264336	438696	56.09%	7.258%
51	9.750	1420	1421	1424	rVB2	380	346	0.04%	0.006%
52	9.805	1428	1430	1431	rBV3	372	314	0.04%	0.005%
53	9.878	1441	1442	1444	rBV2	403	298	0.04%	0.005%
54	10.055	1465	1471	1485	rBV	412421	617088	78.89%	10.210%
55	10.195	1491	1494	1495	rBV3	680	658	0.08%	0.011%
56	10.299	1510	1511	1514	rBV2	464	572	0.07%	0.009%
57	10.512	1544	1546	1549	rVB2	255	311	0.04%	0.005%
58	10.701	1575	1577	1580	rBV2	354	380	0.05%	0.006%
59	10.787	1587	1591	1594	rVB2	490	670	0.09%	0.011%
60	10.842	1598	1600	1603	rBV	368	313	0.04%	0.005%
61	10.957	1617	1619	1625	rVB2	635	1120	0.14%	0.019%
62	11.012	1625	1628	1629	rBV2	264	283	0.04%	0.005%
63	11.073	1636	1638	1640	rBV2	288	288	0.04%	0.005%
64	11.189	1652	1657	1668	rBV	327639	437643	55.95%	7.241%
65	11.354	1683	1684	1686	rVB	487	292	0.04%	0.005%
66	11.451	1698	1700	1702	rBV2	592	439	0.06%	0.007%
67	11.555	1712	1717	1720	rBV3	427	688	0.09%	0.011%
68	11.640	1729	1731	1734	rBV2	271	288	0.04%	0.005%
69	11.884	1769	1771	1775	rBV3	274	329	0.04%	0.005%
70	11.975	1783	1786	1788	rBV2	850	820	0.10%	0.014%
71	12.024	1788	1794	1803	rBV	387080	510441	65.26%	8.445%
72	12.317	1837	1842	1858	rBV	399747	524299	67.03%	8.675%
73	12.561	1880	1882	1883	rVV2	447	278	0.04%	0.005%
74	12.829	1924	1926	1930	rBV3	296	318	0.04%	0.005%
75	12.927	1940	1942	1944	rBV2	296	320	0.04%	0.005%
76	12.969	1947	1949	1951	rBV2	370	432	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043529.D
 Acq On : 25 Oct 2024 17:34
 Operator : JC/MD
 Sample : P4492-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	13.085	1966	1968	1970	rBV2	400	303	0.04%	0.005%
78	13.116	1970	1973	1978	rVV2	1096	1153	0.15%	0.019%
79	13.231	1991	1992	1994	rVB	678	346	0.04%	0.006%
80	13.280	1998	2000	2002	rBV2	364	340	0.04%	0.006%
81	13.329	2005	2008	2010	rBV2	255	363	0.05%	0.006%
82	13.487	2032	2034	2037	rBV2	296	281	0.04%	0.005%
83	13.597	2049	2052	2057	rVB4	1033	1204	0.15%	0.020%
84	13.701	2066	2069	2071	rBV3	454	608	0.08%	0.010%
85	13.737	2071	2075	2077	rVV2	529	778	0.10%	0.013%
86	13.780	2080	2082	2087	rVB2	860	1122	0.14%	0.019%
87	13.841	2091	2092	2094	rBV	287	273	0.03%	0.005%
88	14.128	2134	2139	2142	rBV2	508	894	0.11%	0.015%
89	14.195	2147	2150	2153	rBV2	482	715	0.09%	0.012%
90	14.249	2157	2159	2161	rBV2	371	430	0.05%	0.007%
91	14.298	2165	2167	2168	rBV2	458	412	0.05%	0.007%
92	14.408	2184	2185	2188	rVB	649	428	0.05%	0.007%
93	14.445	2189	2191	2193	rVB	477	399	0.05%	0.007%
94	14.609	2217	2218	2222	rVB3	598	470	0.06%	0.008%
95	15.286	2327	2329	2332	rBV2	784	1024	0.13%	0.017%
96	15.390	2344	2346	2348	rBV2	1022	900	0.12%	0.015%
97	15.877	2424	2426	2427	rBV2	691	470	0.06%	0.008%
98	16.213	2480	2481	2482	rBV	723	314	0.04%	0.005%
99	16.371	2505	2507	2511	rBV3	671	627	0.08%	0.010%
100	16.438	2516	2518	2522	rBV4	546	776	0.10%	0.013%




Sum of corrected areas: 6044066

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043529.D
Acq On : 25 Oct 2024 17:34
Operator : JC/MD
Sample : P4492-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

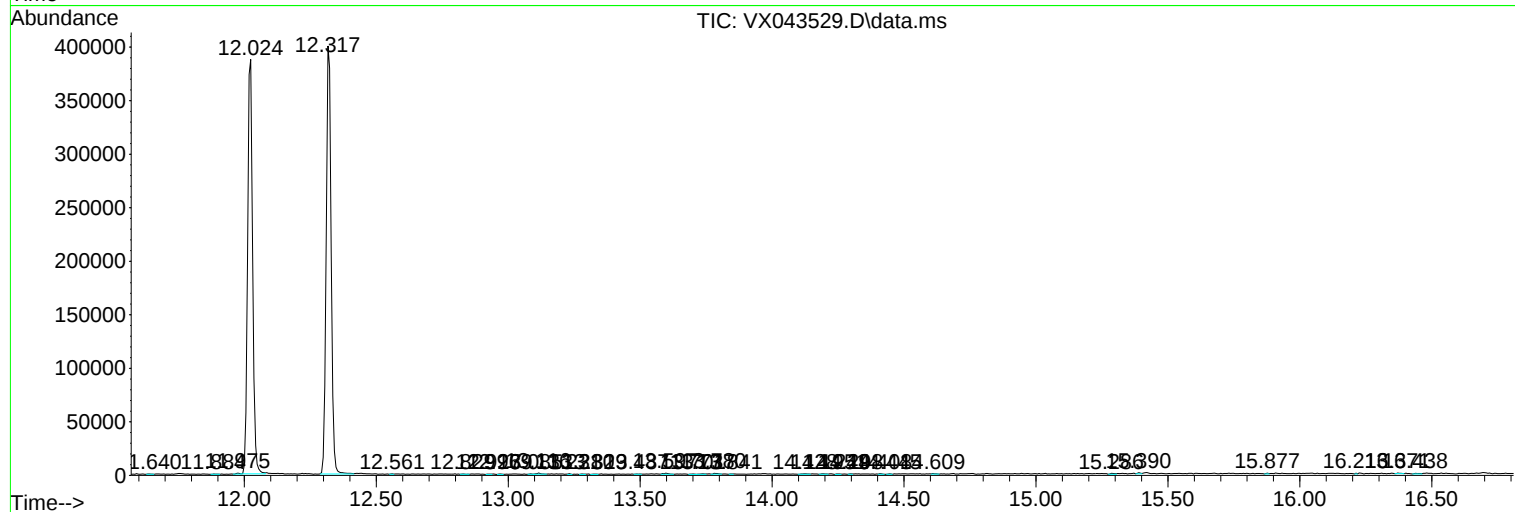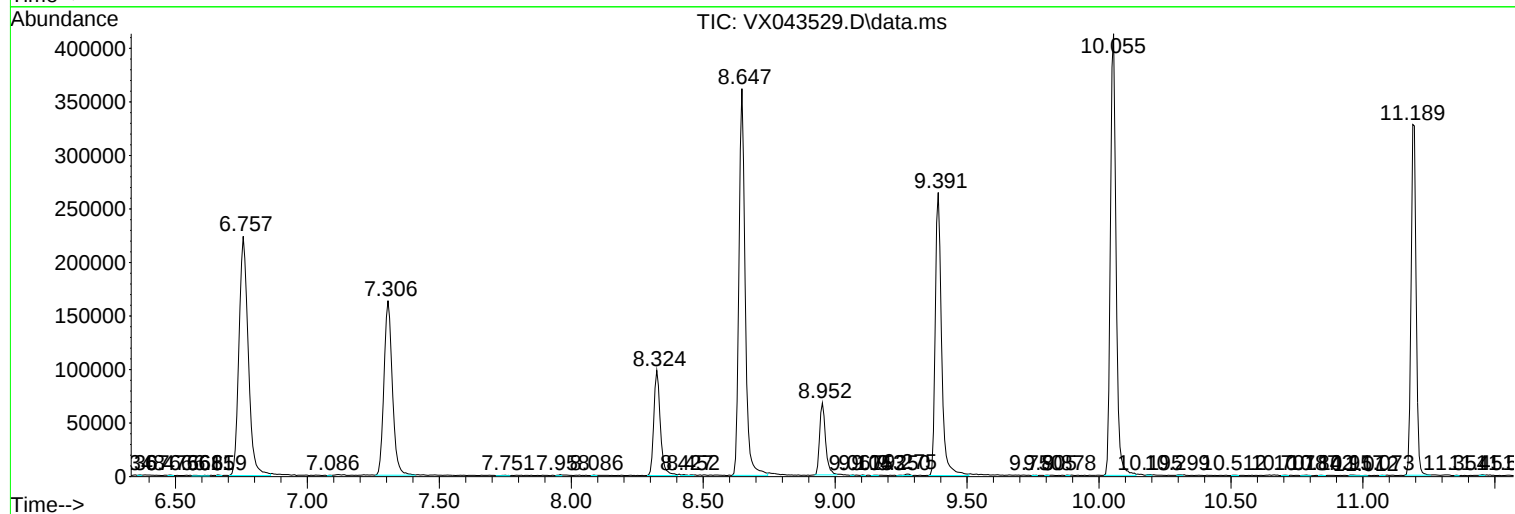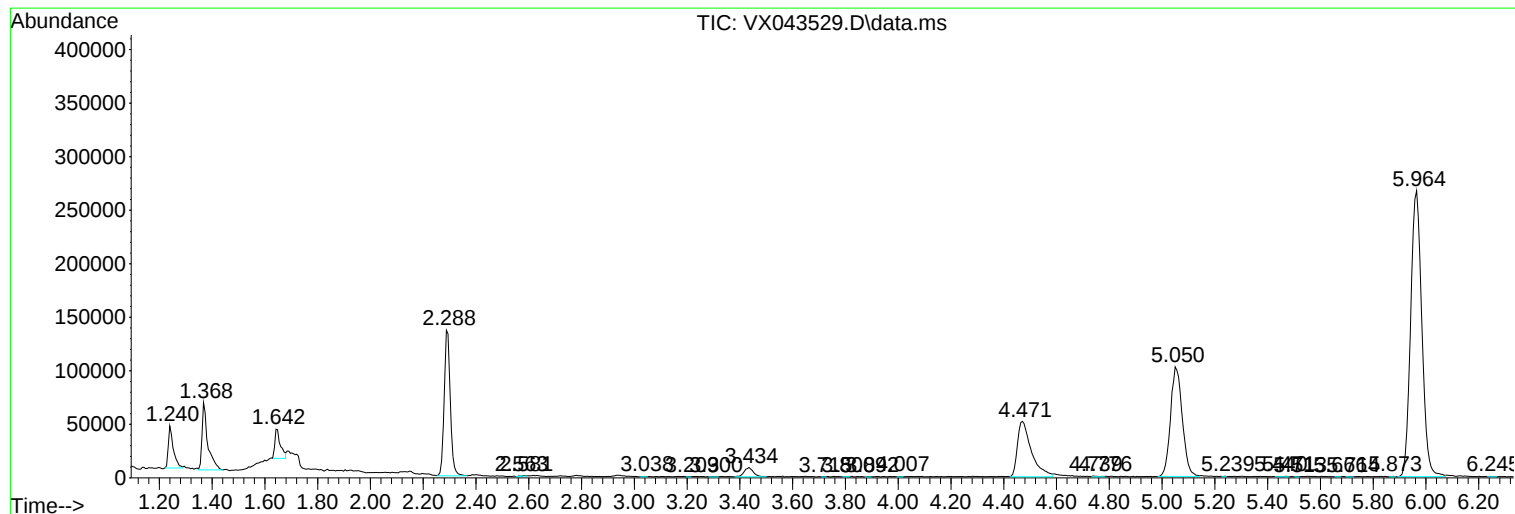

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043529.D
Acq On : 25 Oct 2024 17:34
Operator : JC/MD
Sample : P4492-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043529.D
Acq On : 25 Oct 2024 17:34
Operator : JC/MD
Sample : P4492-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc