

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043530.D
 Acq On : 25 Oct 2024 17:57
 Operator : JC/MD
 Sample : P4568-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	36	rBV	40841	61694	7.52%	0.927%
2	1.368	43	46	58	rVB	66124	96107	11.71%	1.444%
3	1.642	89	91	99	rBV	28538	43675	5.32%	0.656%
4	2.294	192	198	208	rVB	139346	221122	26.94%	3.323%
5	2.398	208	215	225	rBV	13430	25767	3.14%	0.387%
6	2.526	234	236	239	rBV2	443	402	0.05%	0.006%
7	2.575	242	244	246	rBV2	1171	1132	0.14%	0.017%
8	3.209	343	348	349	rBV2	387	547	0.07%	0.008%
9	3.221	349	350	354	rBV2	347	410	0.05%	0.006%
10	3.258	354	356	359	rBV2	424	420	0.05%	0.006%
11	3.349	369	371	373	rBV2	349	412	0.05%	0.006%
12	3.434	378	385	393	rVV4	6699	15124	1.84%	0.227%
13	3.910	459	463	466	rBV2	459	560	0.07%	0.008%
14	4.160	502	504	506	rBV	360	377	0.05%	0.006%
15	4.215	509	513	515	rVB2	434	475	0.06%	0.007%
16	4.471	546	555	577	rBV2	52757	197192	24.03%	2.963%
17	5.050	637	650	671	rVV	110214	340969	41.54%	5.124%
18	5.233	679	680	683	rBV3	520	564	0.07%	0.008%
19	5.306	690	692	697	rVB4	412	449	0.05%	0.007%
20	5.550	729	732	733	rBV2	566	549	0.07%	0.008%
21	5.635	744	746	751	rBV2	426	722	0.09%	0.011%
22	5.806	771	774	776	rBV	319	368	0.04%	0.006%
23	5.964	789	800	815	rBV2	281035	820756	100.00%	12.333%
24	6.355	861	864	865	rBV2	367	474	0.06%	0.007%
25	6.513	888	890	895	rVB2	481	764	0.09%	0.011%
26	6.598	901	904	909	rVB3	426	519	0.06%	0.008%
27	6.635	909	910	913	rBV2	395	397	0.05%	0.006%
28	6.757	921	930	953	rBV	252278	620594	75.61%	9.325%
29	7.111	986	988	990	rBV2	678	614	0.07%	0.009%
30	7.208	1002	1004	1007	rBV3	607	621	0.08%	0.009%
31	7.239	1007	1009	1012	rBV3	470	572	0.07%	0.009%
32	7.306	1012	1020	1035	rVV2	171007	379948	46.29%	5.709%
33	7.452	1042	1044	1046	rVB2	735	524	0.06%	0.008%
34	7.488	1048	1050	1053	rVB2	663	578	0.07%	0.009%
35	7.610	1068	1070	1071	rBV	434	447	0.05%	0.007%
36	7.720	1087	1088	1092	rVB2	692	648	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043530.D
 Acq On : 25 Oct 2024 17:57
 Operator : JC/MD
 Sample : P4568-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

37	7.757	1092	1094	1095	rBV	530	388	0.05%	0.006%
38	7.958	1123	1127	1129	rBV3	685	831	0.10%	0.012%
39	8.232	1169	1172	1173	rBV	352	390	0.05%	0.006%
40	8.324	1181	1187	1199	rBV	105213	175953	21.44%	2.644%
41	8.501	1215	1216	1218	rVB	938	450	0.05%	0.007%
42	8.531	1218	1221	1224	rBV4	515	843	0.10%	0.013%
43	8.647	1234	1240	1258	rBV	376899	621979	75.78%	9.346%
44	8.952	1284	1290	1302	rBV	72772	117401	14.30%	1.764%
45	9.183	1326	1328	1333	rVB2	573	639	0.08%	0.010%
46	9.269	1339	1342	1346	rVB4	798	925	0.11%	0.014%
47	9.391	1356	1362	1377	rBV	282207	451175	54.97%	6.780%
48	9.610	1397	1398	1402	rVB3	911	801	0.10%	0.012%
49	9.750	1419	1421	1423	rBV3	618	568	0.07%	0.009%
50	9.830	1432	1434	1437	rVB	480	407	0.05%	0.006%
51	9.884	1440	1443	1444	rBV	323	369	0.04%	0.006%
52	10.055	1465	1471	1492	rBV	492008	726761	88.55%	10.921%
53	10.305	1509	1512	1514	rBV4	720	826	0.10%	0.012%
54	10.372	1520	1523	1528	rBV2	456	687	0.08%	0.010%
55	10.494	1540	1543	1544	rVB2	438	373	0.05%	0.006%
56	10.787	1588	1591	1592	rBV2	363	429	0.05%	0.006%
57	10.866	1600	1604	1607	rBV2	307	425	0.05%	0.006%
58	10.963	1617	1620	1623	rBV2	467	627	0.08%	0.009%
59	10.994	1623	1625	1628	rBV3	370	479	0.06%	0.007%
60	11.031	1628	1631	1633	rBV3	740	842	0.10%	0.013%
61	11.110	1641	1644	1647	rBV2	399	481	0.06%	0.007%
62	11.189	1652	1657	1665	rBV	334466	453445	55.25%	6.814%
63	11.354	1682	1684	1689	rVB2	391	596	0.07%	0.009%
64	11.457	1698	1701	1702	rBV2	636	410	0.05%	0.006%
65	11.567	1716	1719	1720	rBV2	602	469	0.06%	0.007%
66	11.658	1731	1734	1736	rBV3	535	570	0.07%	0.009%
67	11.738	1745	1747	1748	rBV2	342	360	0.04%	0.005%
68	11.756	1748	1750	1754	rVB3	836	819	0.10%	0.012%
69	11.805	1754	1758	1765	rBV5	1169	2154	0.26%	0.032%
70	11.854	1765	1766	1768	rVB	688	360	0.04%	0.005%
71	11.884	1768	1771	1773	rBV2	507	559	0.07%	0.008%
72	11.969	1781	1785	1788	rBV4	1180	1387	0.17%	0.021%
73	12.018	1788	1793	1802	rBV	472050	612413	74.62%	9.202%
74	12.219	1821	1826	1837	rBV3	9130	18056	2.20%	0.271%
75	12.317	1837	1842	1856	rVV	441734	560842	68.33%	8.428%
76	12.518	1874	1875	1878	rBV2	500	499	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043530.D
 Acq On : 25 Oct 2024 17:57
 Operator : JC/MD
 Sample : P4568-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4FF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	12.579	1881	1885	1890	rVV4	8399	11245	1.37%	0.169%
78	12.689	1902	1903	1906	rBV2	888	638	0.08%	0.010%
79	12.768	1914	1916	1920	rBV4	1045	1150	0.14%	0.017%
80	12.817	1920	1924	1929	rBV2	16930	21727	2.65%	0.326%
81	12.969	1947	1949	1952	rBV4	522	713	0.09%	0.011%
82	13.091	1968	1969	1970	rBV	820	538	0.07%	0.008%
83	13.219	1988	1990	1993	rBV2	522	633	0.08%	0.010%
84	13.463	2026	2030	2032	rBV2	1157	1272	0.15%	0.019%
85	13.597	2047	2052	2058	rVV3	3267	5568	0.68%	0.084%
86	13.908	2101	2103	2105	rVB2	419	374	0.05%	0.006%
87	13.963	2109	2112	2119	rVB5	1496	2453	0.30%	0.037%
88	14.042	2122	2125	2126	rBV3	456	450	0.05%	0.007%
89	14.128	2134	2139	2140	rBV4	891	1355	0.17%	0.020%
90	14.189	2147	2149	2150	rVB2	635	397	0.05%	0.006%
91	14.207	2150	2152	2153	rBV	445	395	0.05%	0.006%
92	14.298	2164	2167	2169	rBV2	707	680	0.08%	0.010%
93	14.317	2169	2170	2172	rVV	614	529	0.06%	0.008%
94	14.341	2172	2174	2176	rVB	510	387	0.05%	0.006%
95	14.396	2181	2183	2186	rVB2	511	452	0.06%	0.007%
96	14.457	2186	2193	2196	rBV5	971	1842	0.22%	0.028%
97	14.731	2234	2238	2241	rVB3	1044	1536	0.19%	0.023%
98	14.987	2277	2280	2284	rVB3	2024	2394	0.29%	0.036%
99	15.493	2360	2363	2371	rBV5	1243	2734	0.33%	0.041%
100	16.408	2511	2513	2518	rBV3	607	914	0.11%	0.014%




Sum of corrected areas: 6654857

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043530.D
Acq On : 25 Oct 2024 17:57
Operator : JC/MD
Sample : P4568-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

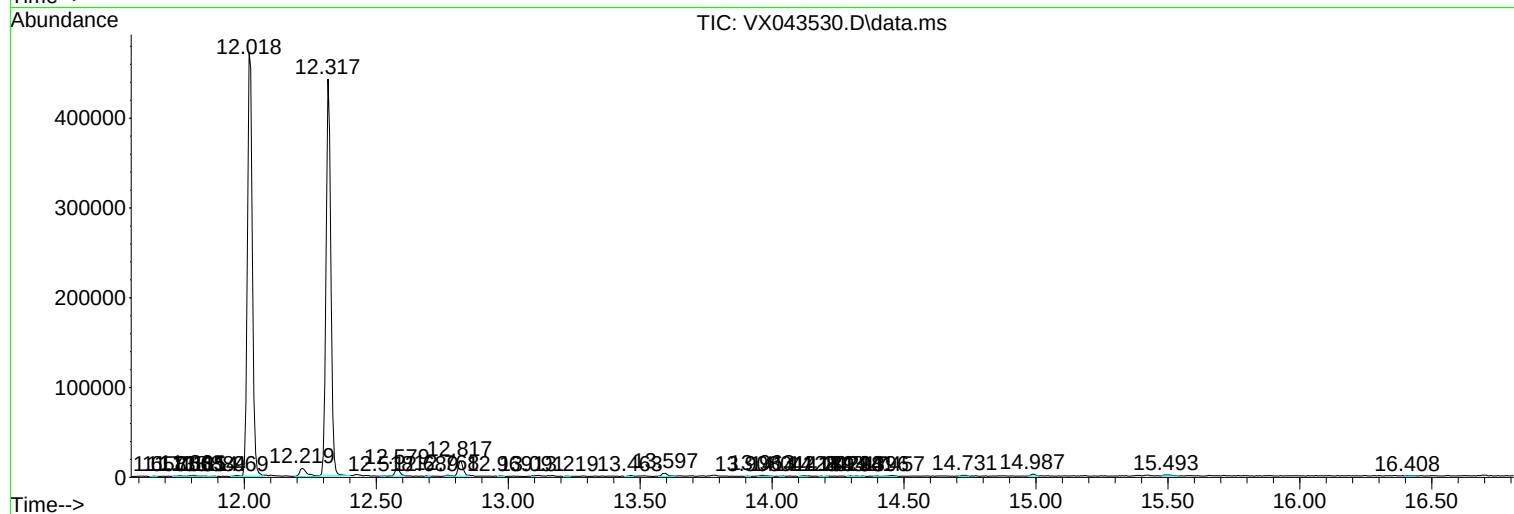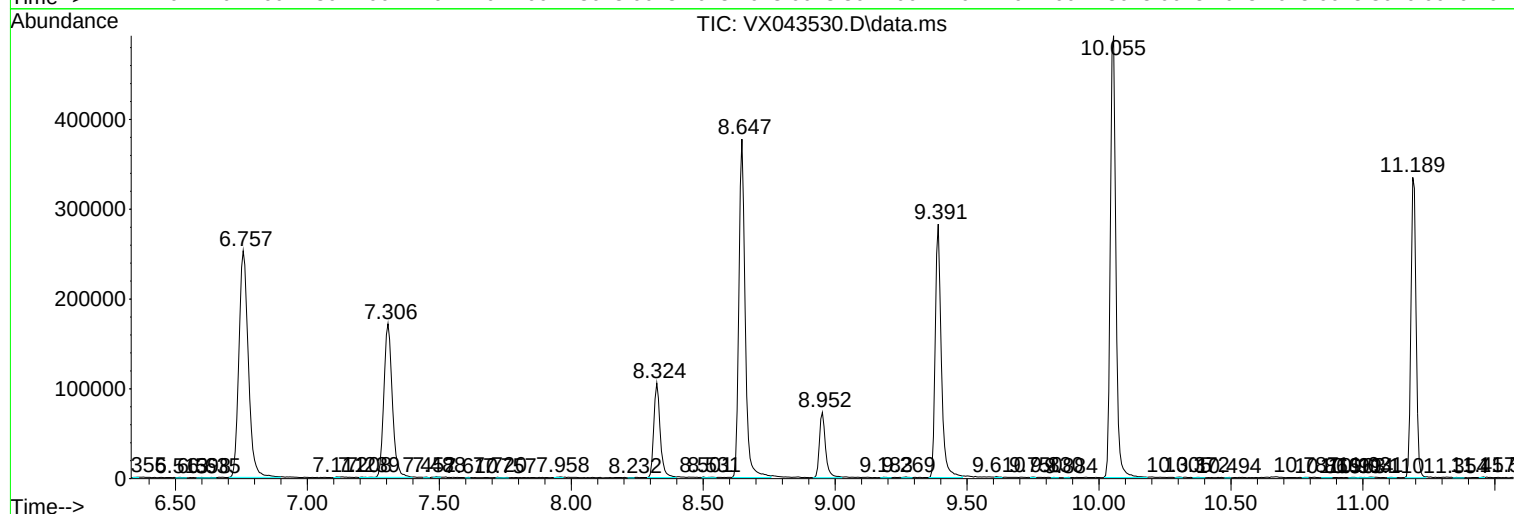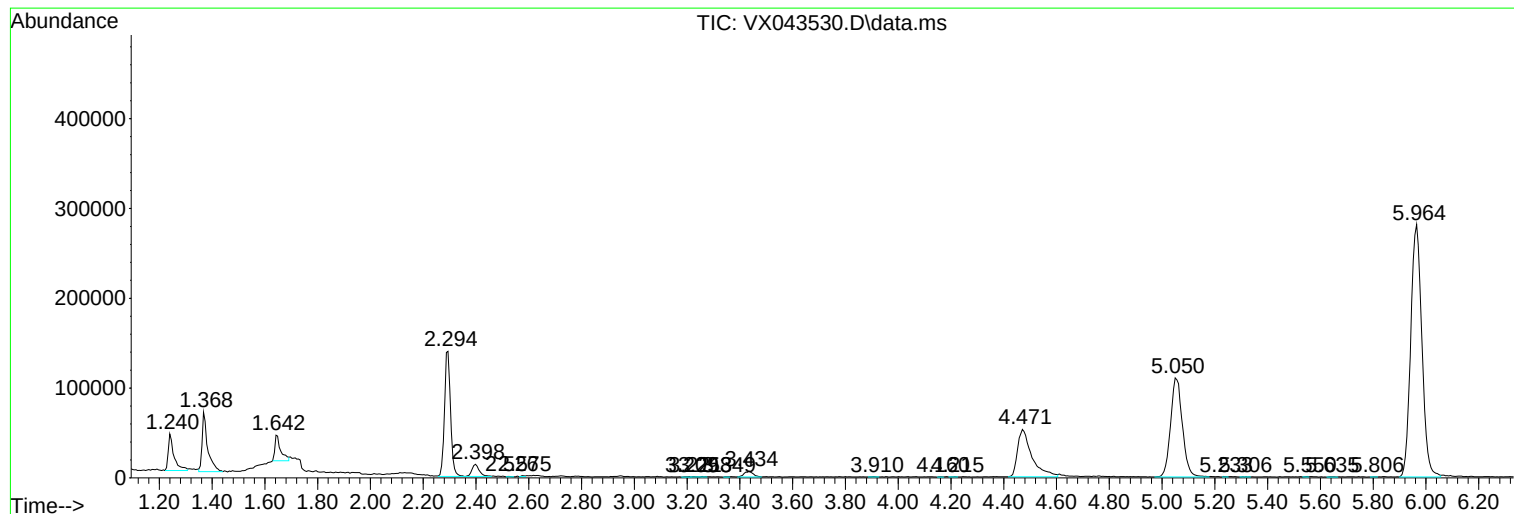

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043530.D
Acq On : 25 Oct 2024 17:57
Operator : JC/MD
Sample : P4568-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043530.D
Acq On : 25 Oct 2024 17:57
Operator : JC/MD
Sample : P4568-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4FF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
