

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043531.D
 Acq On : 25 Oct 2024 18:20
 Operator : JC/MD
 Sample : P4568-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

Signal : TIC: VX043531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	38	rBV	36994	50378	6.79%	0.879%
2	1.368	43	46	57	rVB	59879	84556	11.40%	1.475%
3	1.648	89	92	97	rBV	22472	33561	4.53%	0.586%
4	2.288	192	197	210	rVB	124215	201618	27.19%	3.518%
5	2.569	241	243	244	rBV	591	392	0.05%	0.007%
6	2.782	274	278	283	rVB5	1729	2729	0.37%	0.048%
7	2.941	298	304	310	rBV3	1135	2189	0.30%	0.038%
8	3.075	324	326	327	rBV	546	403	0.05%	0.007%
9	3.434	377	385	396	rBV3	8416	21147	2.85%	0.369%
10	3.739	433	435	436	rBV2	432	347	0.05%	0.006%
11	3.837	447	451	452	rBV2	281	388	0.05%	0.007%
12	3.928	465	466	472	rBV3	464	467	0.06%	0.008%
13	4.008	475	479	480	rVB2	469	510	0.07%	0.009%
14	4.026	480	482	483	rBV	510	369	0.05%	0.006%
15	4.264	519	521	525	rVV	390	338	0.05%	0.006%
16	4.355	535	536	538	rBV2	412	330	0.04%	0.006%
17	4.471	546	555	575	rBV	49005	182163	24.57%	3.178%
18	4.849	615	617	620	rBV3	298	417	0.06%	0.007%
19	4.922	628	629	631	rBV	399	332	0.04%	0.006%
20	4.959	634	635	638	rVV2	455	490	0.07%	0.009%
21	5.056	638	651	668	rVV	101317	303619	40.95%	5.297%
22	5.434	712	713	716	rVB2	627	486	0.07%	0.008%
23	5.458	716	717	720	rVV2	365	414	0.06%	0.007%
24	5.550	729	732	736	rBV3	684	859	0.12%	0.015%
25	5.623	738	744	746	rVB3	340	562	0.08%	0.010%
26	5.782	766	770	771	rBV	524	579	0.08%	0.010%
27	5.873	782	785	787	rBV2	394	308	0.04%	0.005%
28	5.964	789	800	815	rBV2	253635	741462	100.00%	12.936%
29	6.599	901	904	907	rBV2	348	346	0.05%	0.006%
30	6.641	907	911	913	rBV2	240	368	0.05%	0.006%
31	6.672	914	916	917	rVB	598	368	0.05%	0.006%
32	6.757	921	930	945	rBV	211618	521669	70.36%	9.101%
33	7.050	976	978	980	rVB2	539	310	0.04%	0.005%
34	7.123	988	990	993	rVB3	943	958	0.13%	0.017%
35	7.196	1001	1002	1004	rBV	412	347	0.05%	0.006%
36	7.306	1010	1020	1039	rBV	156628	344563	46.47%	6.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043531.D
 Acq On : 25 Oct 2024 18:20
 Operator : JC/MD
 Sample : P4568-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102524WMA.M
 Title : VOC Analysis

37	7.653	1073	1077	1079	rBV3	387	442	0.06%	0.008%
38	7.830	1102	1106	1108	rBV2	355	559	0.08%	0.010%
39	7.958	1125	1127	1132	rVB4	681	771	0.10%	0.013%
40	7.995	1132	1133	1138	rVB3	701	867	0.12%	0.015%
41	8.037	1138	1140	1142	rBV2	686	554	0.07%	0.010%
42	8.257	1175	1176	1179	rBV	320	358	0.05%	0.006%
43	8.324	1181	1187	1201	rVV	94392	158591	21.39%	2.767%
44	8.647	1233	1240	1250	rBV	333456	547885	73.89%	9.559%
45	8.952	1285	1290	1305	rVV	66047	105881	14.28%	1.847%
46	9.171	1323	1326	1327	rBV2	386	344	0.05%	0.006%
47	9.269	1340	1342	1349	rVB2	1039	1431	0.19%	0.025%
48	9.391	1356	1362	1376	rBV	259913	415966	56.10%	7.257%
49	9.604	1395	1397	1402	rVB6	458	628	0.08%	0.011%
50	10.055	1465	1471	1486	rVV	401513	593039	79.98%	10.347%
51	10.305	1511	1512	1515	rVB2	507	418	0.06%	0.007%
52	10.604	1558	1561	1565	rBV3	381	513	0.07%	0.009%
53	10.647	1565	1568	1573	rBV4	474	911	0.12%	0.016%
54	10.689	1573	1575	1576	rVV	490	302	0.04%	0.005%
55	10.903	1608	1610	1611	rBV2	432	329	0.04%	0.006%
56	10.964	1617	1620	1625	rBV3	680	1160	0.16%	0.020%
57	11.025	1629	1630	1633	rVB	523	295	0.04%	0.005%
58	11.061	1633	1636	1638	rBV2	393	511	0.07%	0.009%
59	11.098	1640	1642	1646	rVB	464	512	0.07%	0.009%
60	11.195	1652	1658	1667	rBV	301879	410743	55.40%	7.166%
61	11.537	1713	1714	1716	rBV	321	287	0.04%	0.005%
62	11.561	1716	1718	1721	rVV3	438	481	0.06%	0.008%
63	11.592	1721	1723	1726	rVV3	437	363	0.05%	0.006%
64	11.659	1732	1734	1737	rVV2	377	385	0.05%	0.007%
65	11.720	1742	1744	1747	rVV2	561	396	0.05%	0.007%
66	11.750	1747	1749	1754	rVB3	647	1147	0.15%	0.020%
67	11.787	1754	1755	1756	rBV	545	307	0.04%	0.005%
68	11.939	1778	1780	1782	rVB2	358	319	0.04%	0.006%
69	11.976	1782	1786	1788	rBV3	1048	1417	0.19%	0.025%
70	12.018	1788	1793	1804	rBV	376949	482532	65.08%	8.419%
71	12.317	1837	1842	1851	rBV	382003	484525	65.35%	8.453%
72	12.646	1894	1896	1899	rVB2	562	395	0.05%	0.007%
73	13.110	1970	1972	1977	rVB3	754	993	0.13%	0.017%
74	13.207	1986	1988	1989	rVB	502	319	0.04%	0.006%
75	13.335	2007	2009	2012	rBV3	476	602	0.08%	0.011%
76	13.384	2015	2017	2020	rVV3	413	556	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
 Data File : VX043531.D
 Acq On : 25 Oct 2024 18:20
 Operator : JC/MD
 Sample : P4568-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
 Title : VOC Analysis

77	13.439	2023	2026	2028	rBV2	464	430	0.06%	0.008%
78	13.475	2028	2032	2033	rBV3	420	488	0.07%	0.009%
79	13.585	2048	2050	2052	rBV2	404	452	0.06%	0.008%
80	13.780	2080	2082	2088	rVV3	965	933	0.13%	0.016%
81	13.841	2091	2092	2095	rVB2	416	360	0.05%	0.006%
82	14.024	2120	2122	2126	rVB2	449	595	0.08%	0.010%
83	14.122	2135	2138	2140	rBV3	559	735	0.10%	0.013%
84	14.158	2142	2144	2148	rBV	354	469	0.06%	0.008%
85	14.195	2148	2150	2153	rBV3	452	367	0.05%	0.006%
86	14.274	2161	2163	2165	rVV2	554	422	0.06%	0.007%
87	14.542	2204	2207	2208	rVB2	687	502	0.07%	0.009%
88	14.554	2208	2209	2211	rBV2	585	501	0.07%	0.009%
89	14.689	2226	2231	2233	rBV3	500	885	0.12%	0.015%
90	14.774	2243	2245	2247	rVB2	549	452	0.06%	0.008%
91	14.823	2250	2253	2255	rBV2	445	536	0.07%	0.009%
92	14.878	2259	2262	2263	rBV2	513	515	0.07%	0.009%
93	15.012	2281	2284	2285	rBV	557	516	0.07%	0.009%
94	15.073	2292	2294	2296	rVB2	491	375	0.05%	0.007%
95	15.109	2298	2300	2302	rBV2	753	558	0.08%	0.010%
96	15.256	2322	2324	2326	rVB2	568	302	0.04%	0.005%
97	15.323	2334	2335	2338	rVB2	906	658	0.09%	0.011%
98	15.359	2338	2341	2342	rBV2	567	545	0.07%	0.010%
99	15.377	2342	2344	2347	rBV2	650	740	0.10%	0.013%
100	16.676	2554	2557	2558	rBV3	845	1003	0.14%	0.017%




Sum of corrected areas: 5731715

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043531.D
Acq On : 25 Oct 2024 18:20
Operator : JC/MD
Sample : P4568-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

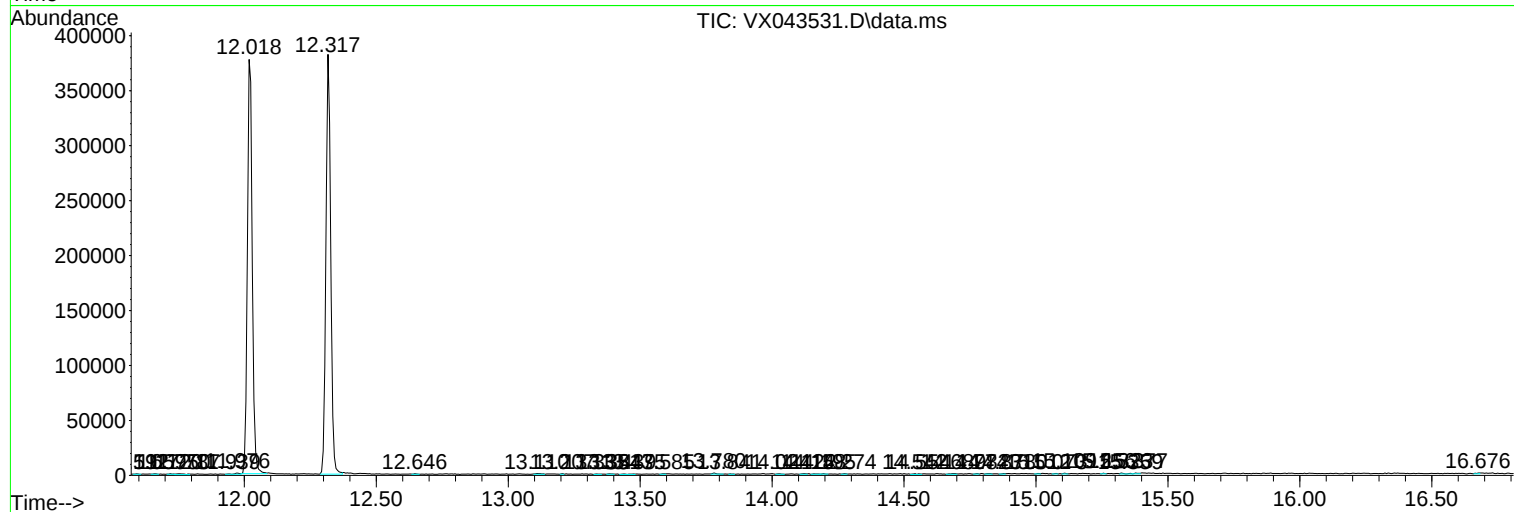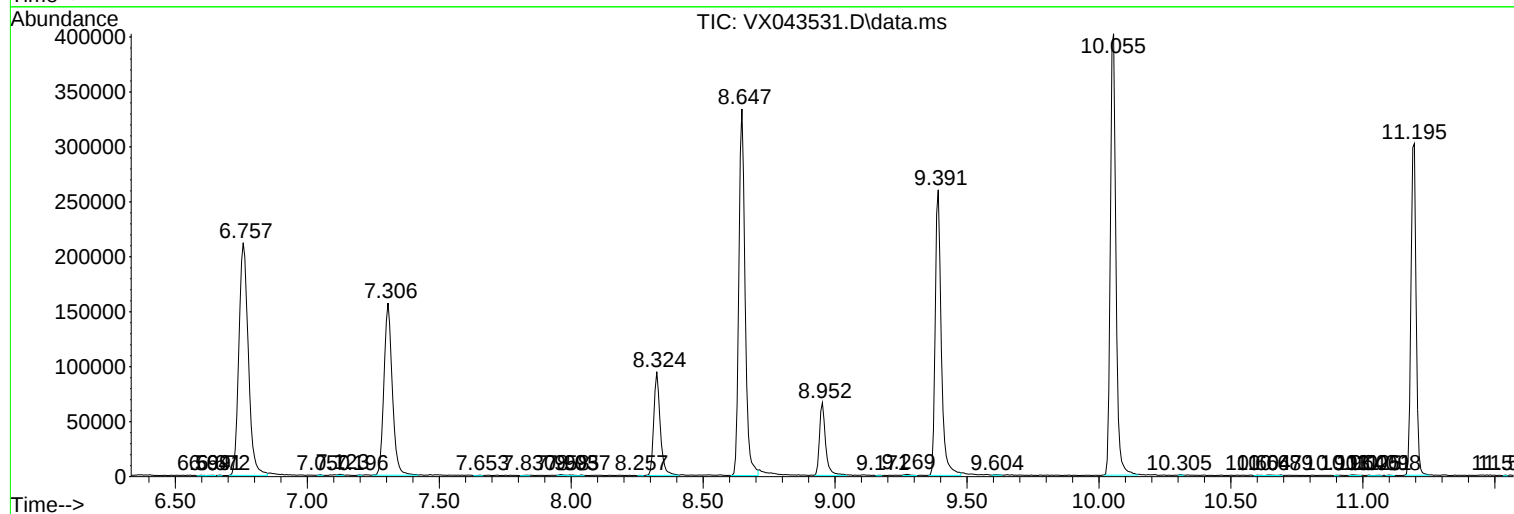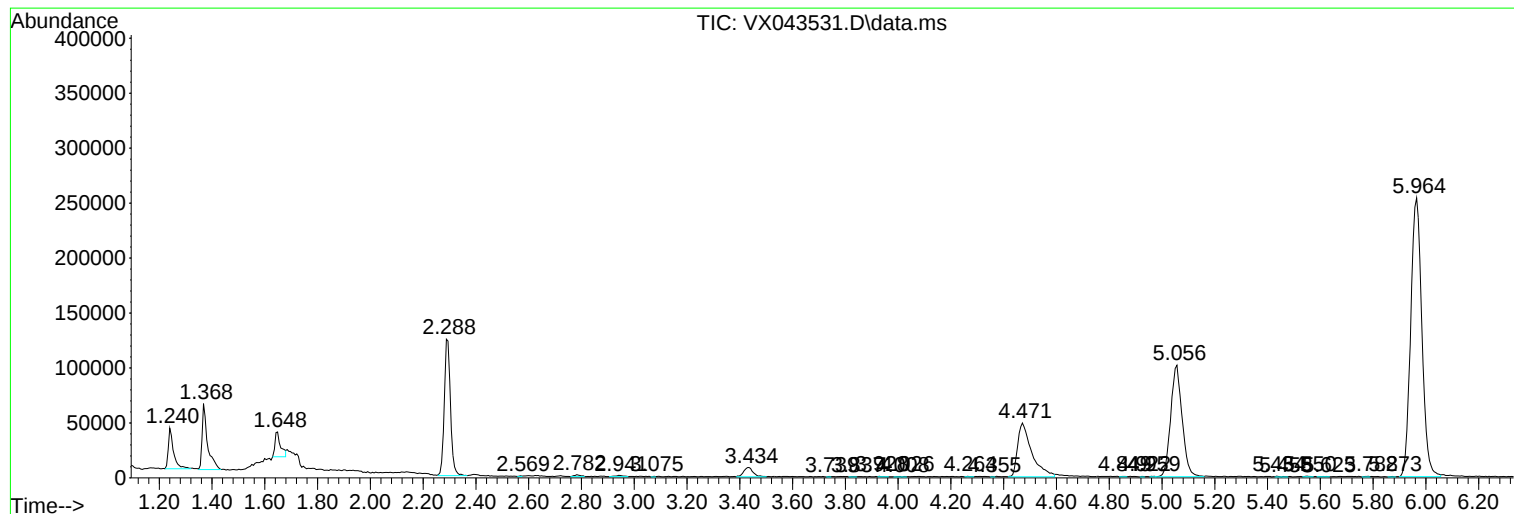

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043531.D
Acq On : 25 Oct 2024 18:20
Operator : JC/MD
Sample : P4568-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102524\
Data File : VX043531.D
Acq On : 25 Oct 2024 18:20
Operator : JC/MD
Sample : P4568-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc